
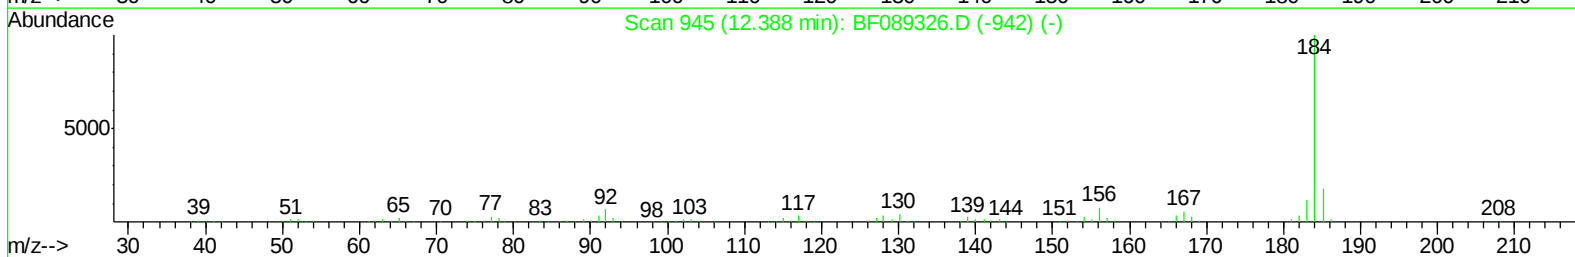
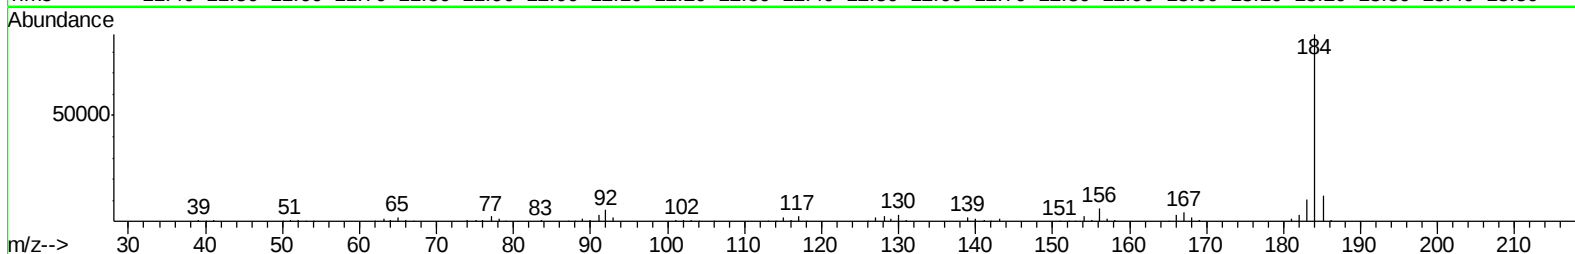


Data Path : Z:\HPCHEM1\BNA F\Data\BF073116\  
Data File : BF089487.D  
Acq On : 31 Jul 2016 23:48  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:07:16 2016  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 28 16:02:32 2016  
Response via : Initial Calibration

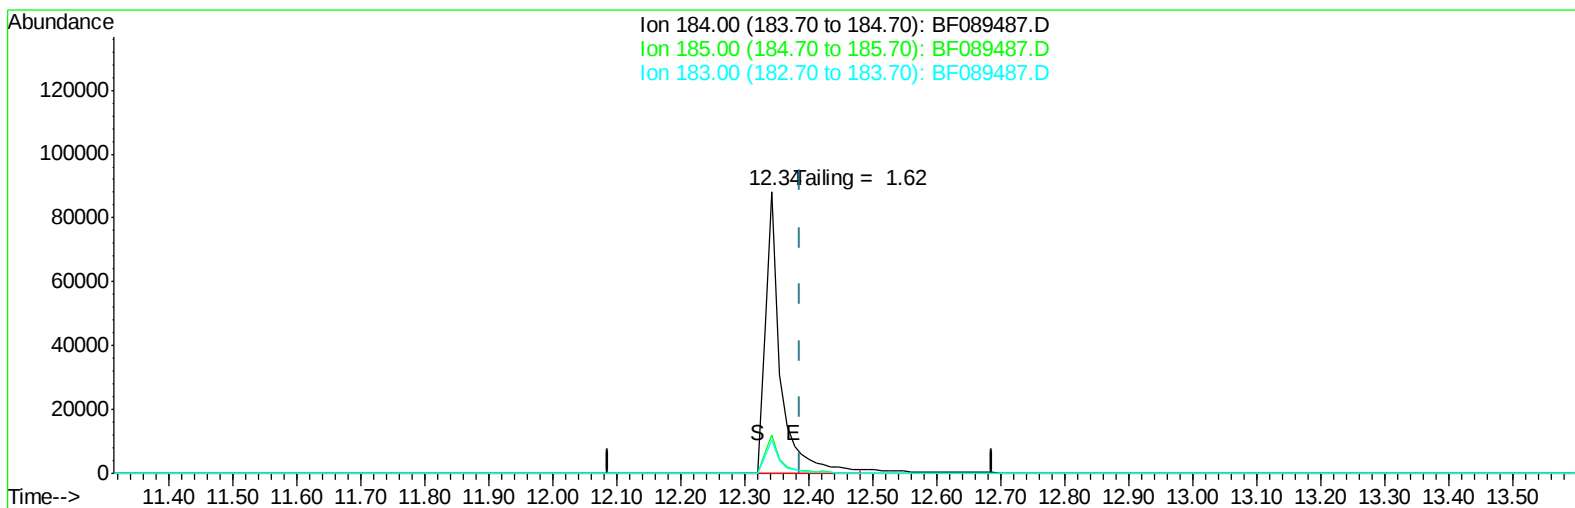

TIC: BF089487.D

(76) Benzidine




12.342min (-0.045) 0.00ng

response 151495

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 16.90 | 13.76 |
| 183.00 | 12.20 | 11.94 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\Data\BF073116\  
Data File : BF089487.D  
Acq On : 31 Jul 2016 23:48  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:07:16 2016  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Jul 28 16:02:32 2016  
Response via : Initial Calibration

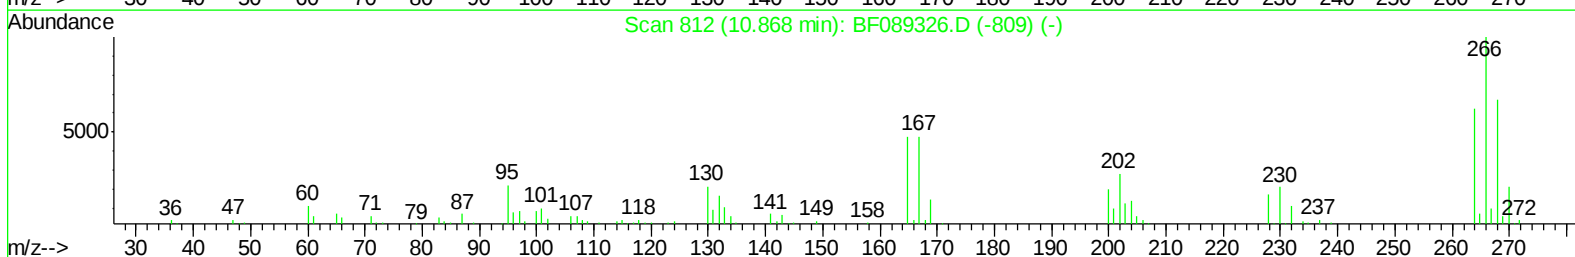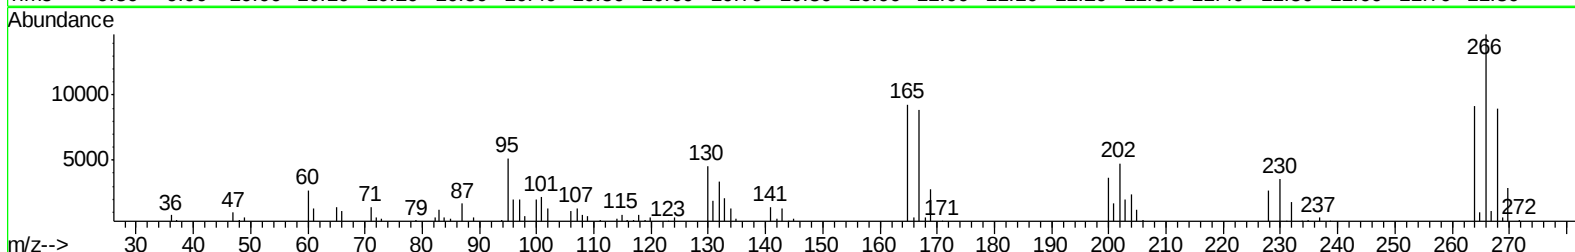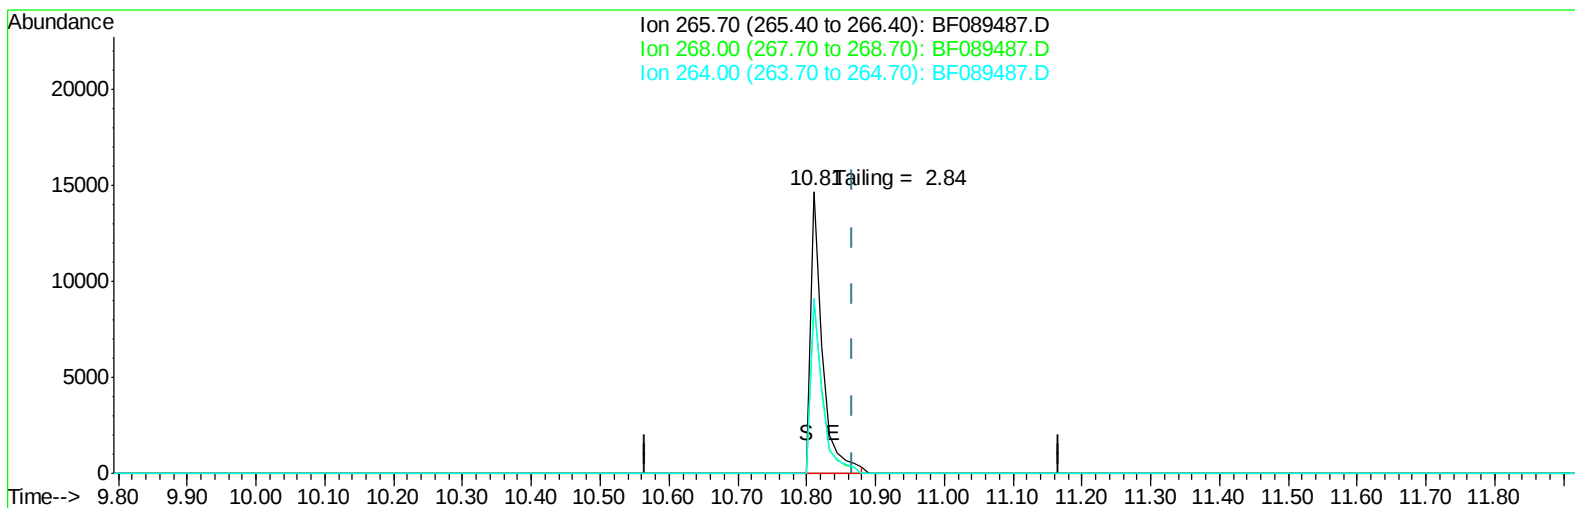

TIC: BF089487.D

(69) Pentachlorophenol (C)

10.810min (-0.057) 0.00ng

response 17693

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 61.80 | 60.87 |
| 264.00 | 62.70 | 62.41 |
| 0.00   | 0.00  | 0.00  |