

Data Path : Z:\HPCHEM1\BNA F\DATA\BF073116\
 Data File : BF089467.D
 Acq On : 31 Jul 2016 13:21
 Operator : UM/SJ
 Sample : H4284-19
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AB-SLOPE(0-4)J

Quant Time: Aug 01 05:16:54 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 01 04:11:30 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.49	152	41406	20.00	ng	-0.01
21) Naphthalene-d8	7.78	136	165669	20.00	ng	-0.01
38) Acenaphthene-d10	9.52	164	81700	20.00	ng	-0.01
63) Phenanthrene-d10	10.99	188	154708	20.00	ng	-0.01
75) Chrysene-d12	13.61	240	99577	20.00	ng	-0.01
86) Perylene-d12	14.94	264	74103	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.06	112	364985	140.75	ng	0.00
7) Phenol-d6	6.16	99	538132	157.03	ng	-0.01
23) Nitrobenzene-d5	7.06	82	298658	106.41	ng	-0.02
41) 2,4,6-Tribromophenol	10.31	330	82883	122.49	ng	-0.01
44) 2-Fluorobiphenyl	8.86	172	474031	85.15	ng	-0.01
78) Terphenyl-d14	12.57	244	376020	88.38	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.26	163	83504	13.43	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF073116\
Data File : BF089467.D
Acq On : 31 Jul 2016 13:21
Operator : UM/SJ
Sample : H4284-19
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AB-SLOPE(0-4)J

Quant Time: Aug 01 05:16:54 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 01 04:11:30 2016
Response via : Initial Calibration

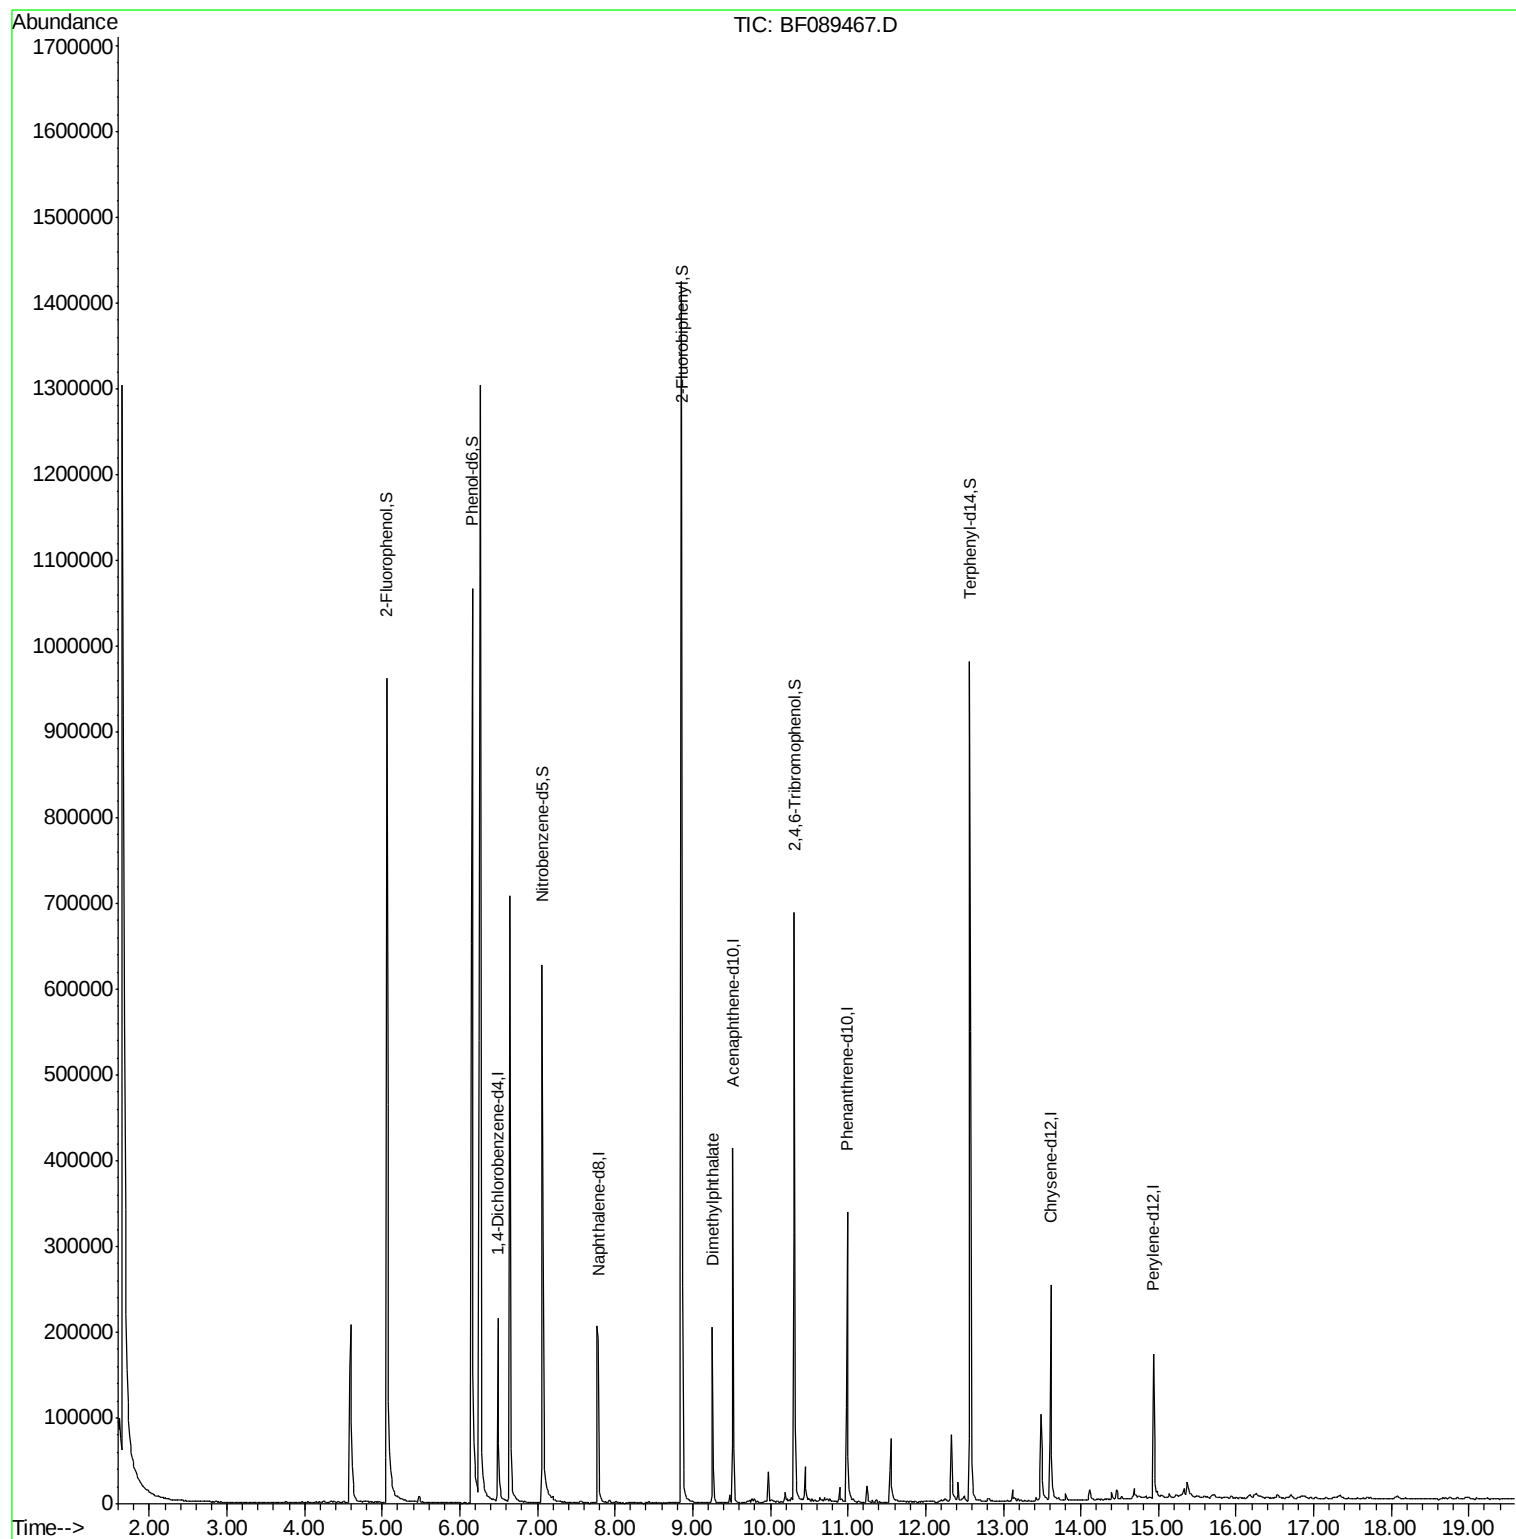

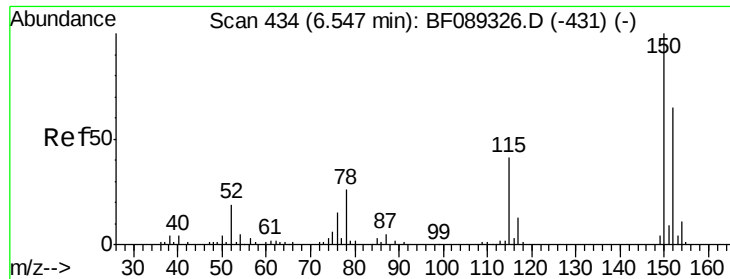

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.49 min Scan# 429

Delta R.T. -0.01 min

Lab File: BF089467.D

Acq: 31 Jul 2016 13:21

Instrument :

BNA_F

ClientSampleId :

AB-SLOPE(0-4)J


Tot Ion:152 Resp: 41406

Ion Ratio Lower Upper

152 100

150 158.4 129.5 194.3




115 67.3 51.4 77.2

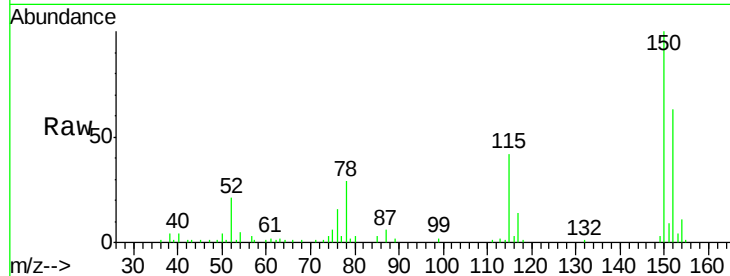

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

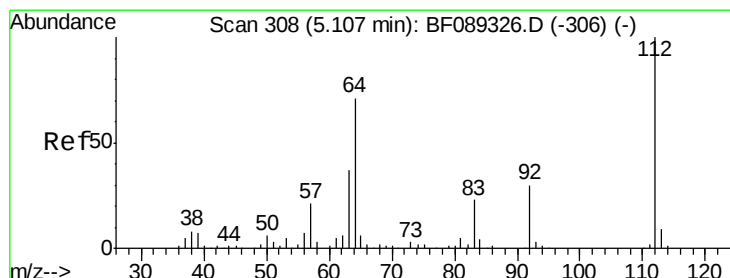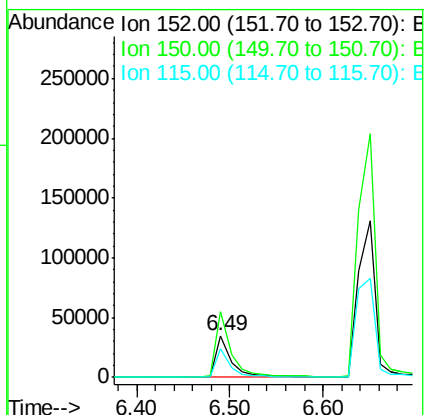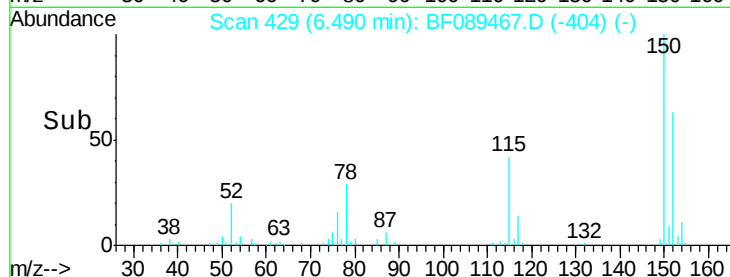

#5

2-Fluorophenol

Concen: 140.75 ng

RT: 5.06 min Scan# 304

Delta R.T. 0.00 min

Lab File: BF089467.D

Acq: 31 Jul 2016 13:21


Tgt Ion:112 Resp: 364985

Ion Ratio Lower Upper

112 100

64 62.4 55.0 82.6



63 33.9 29.4 44.2

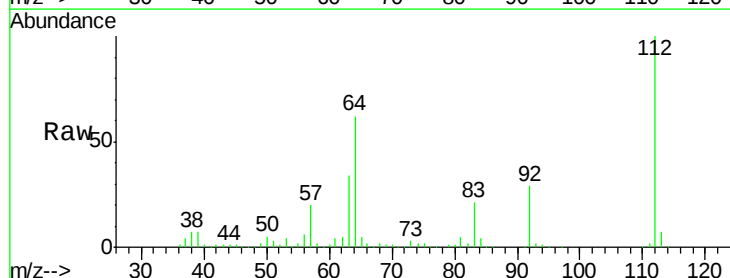


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

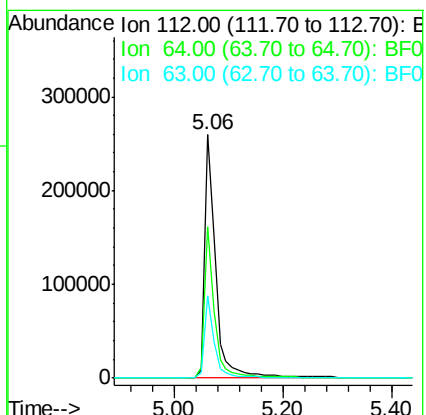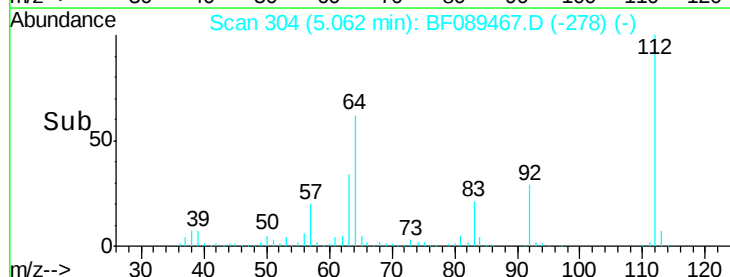

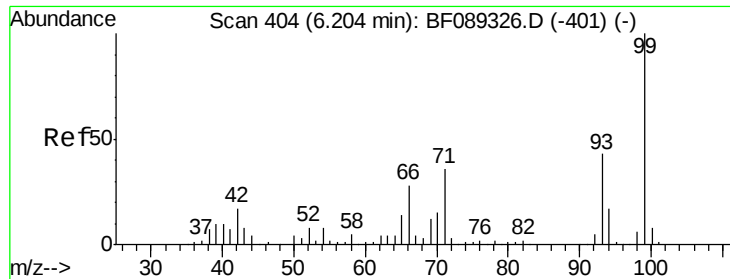

#7

Phenol-d6

Concen: 157.03 ng

RT: 6.16 min Scan# 400

Delta R.T. -0.01 min

Lab File: BF089467.D

Acq: 31 Jul 2016 13:21

Instrument :

BNA_F

ClientSampleId :

AB-SLOPE(0-4)J


Tot Ion: 99 Resp: 538132

Ion Ratio Lower Upper

99 100

42 15.8 13.6 20.4




71 35.4 29.4 44.2

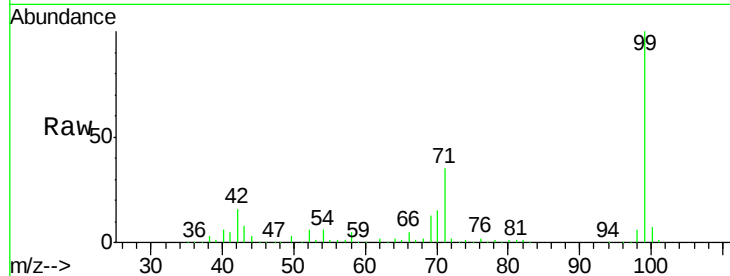

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

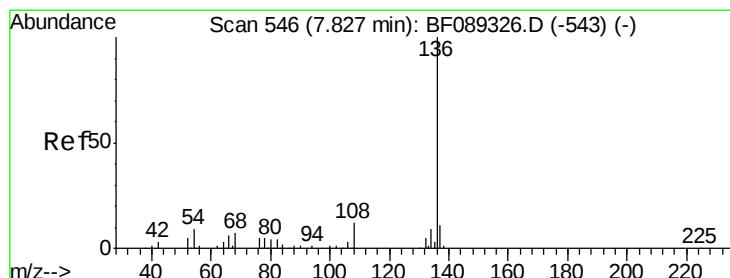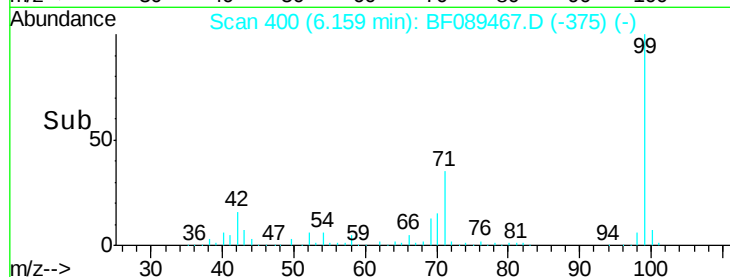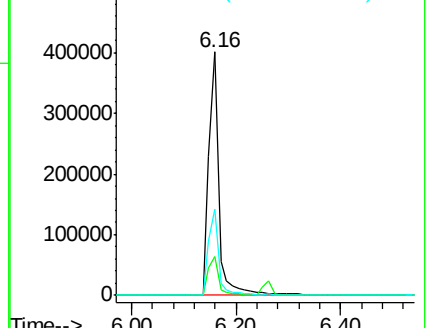

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.78 min Scan# 542

Delta R.T. -0.01 min

Lab File: BF089467.D

Acq: 31 Jul 2016 13:21

Tgt Ion: 136 Resp: 165669


Ion Ratio Lower Upper

136 100

137 10.2 8.6 13.0

54 5.7 7.0 10.4#

68 4.7 4.9 7.3#


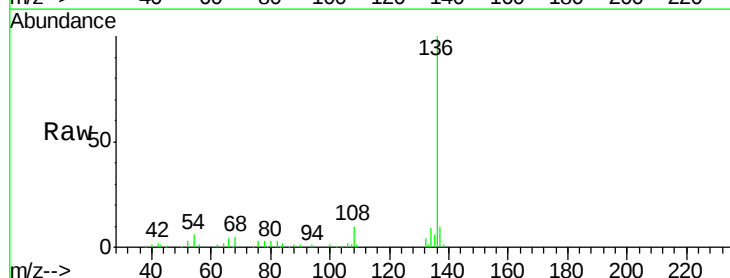



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

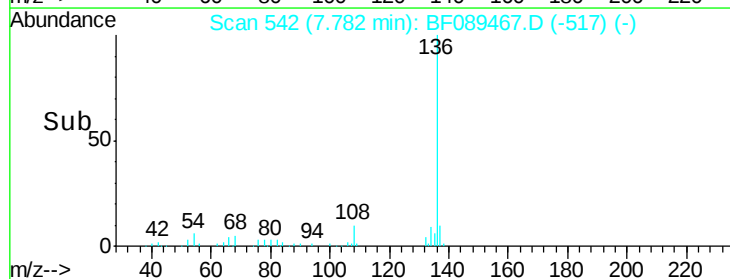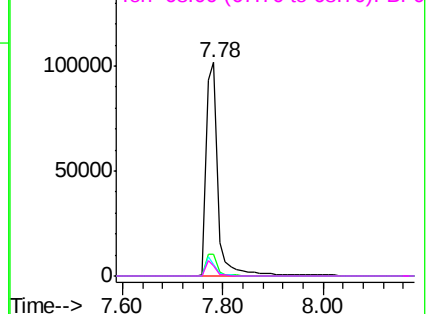


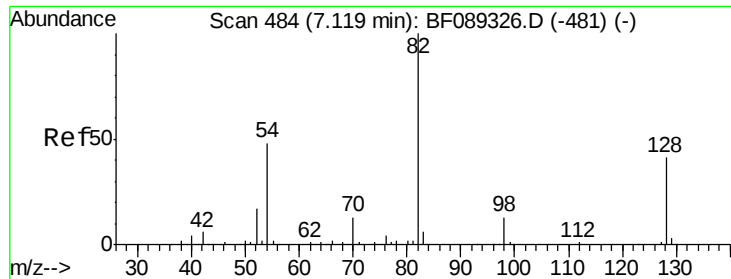




#23
 Nitrobenzene-d5
 Concen: 106.41 ng
 RT: 7.06 min Scan# 479
 Delta R.T. -0.02 min
 Lab File: BF089467.D
 Acq: 31 Jul 2016 13:21

Instrument :
 BNA_F
 ClientSampleId :
 AB-SLOPE(0-4)J

Tot Ion	82	Resp	298658
Ion Ratio	100	Lower	Upper
128	38.4	32.5	48.7
54	50.1	38.8	58.2

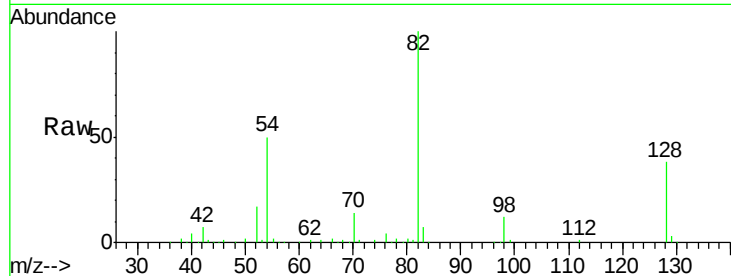


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

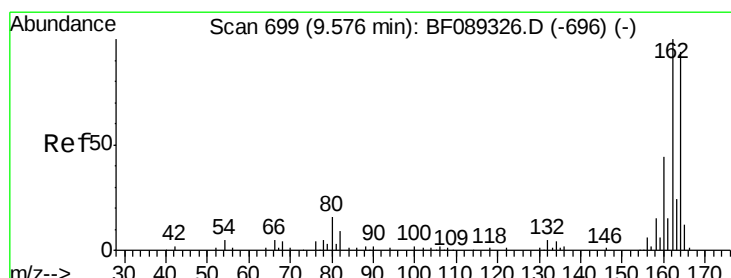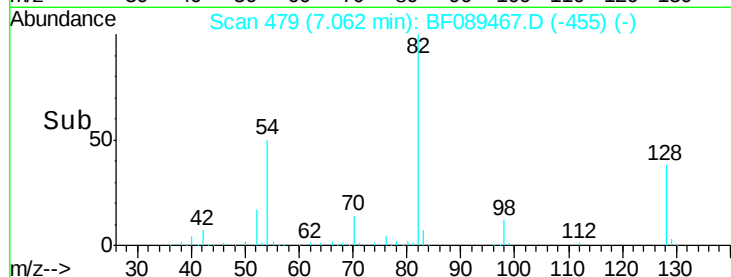
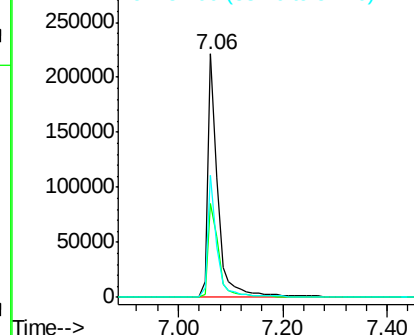



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.52 min Scan# 694
 Delta R.T. -0.01 min
 Lab File: BF089467.D
 Acq: 31 Jul 2016 13:21

Tgt Ion	164	Resp	81700
Ion Ratio	100	Lower	Upper
162	105.5	83.7	125.5
160	47.6	37.8	56.6

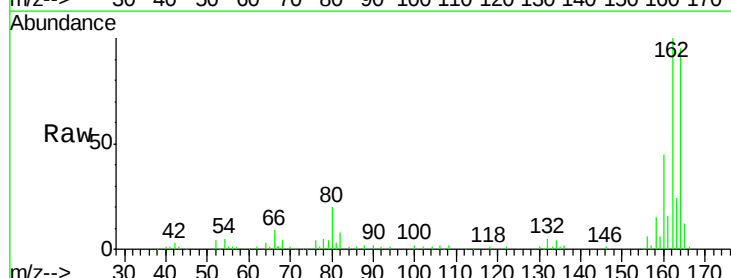

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

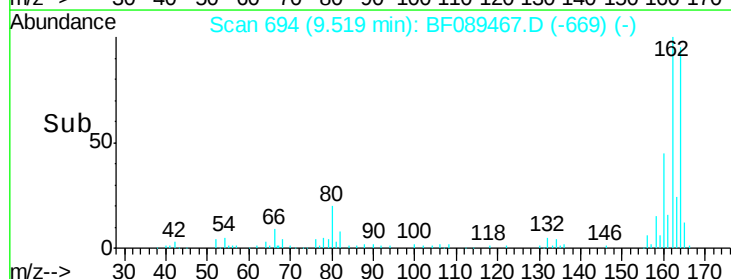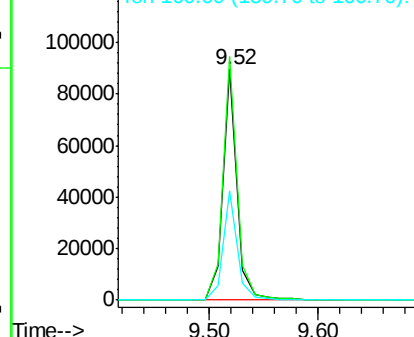


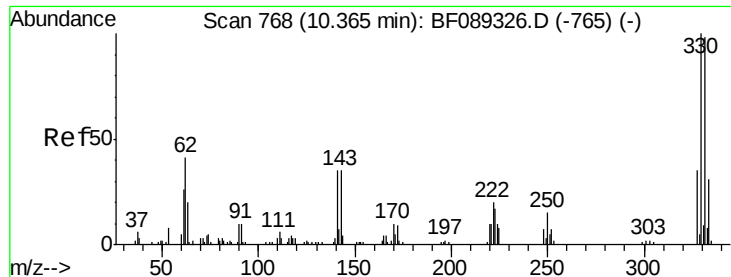




#41
 2,4,6-Tribromophenol
 Concen: 122.49 ng
 RT: 10.31 min Scan# 763
 Delta R.T. -0.01 min
 Lab File: BF089467.D
 Acq: 31 Jul 2016 13:21

Instrument :
 BNA_F
 ClientSampleId :
 AB-SLOPE(0-4)J

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.1	76.8	115.2
141	48.6	37.3	55.9

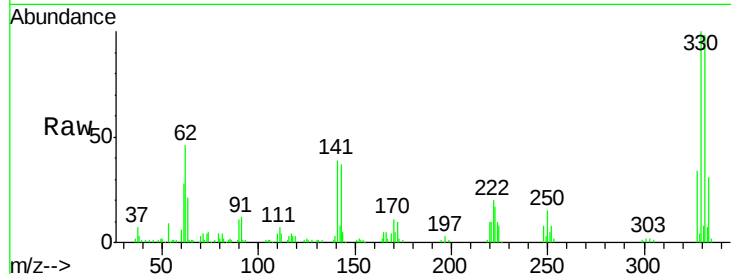


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

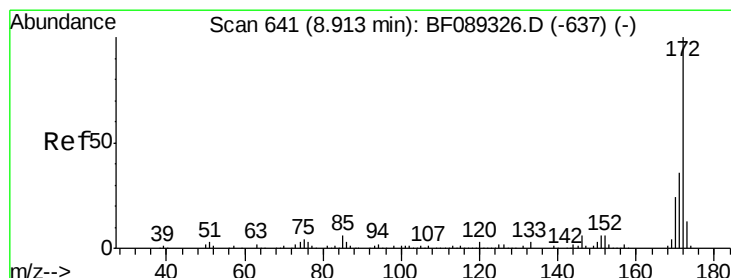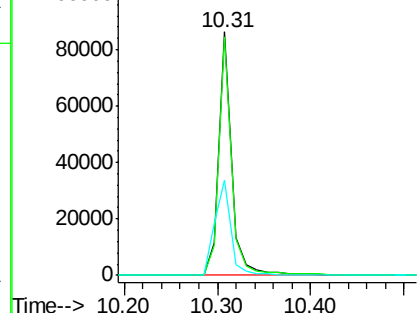
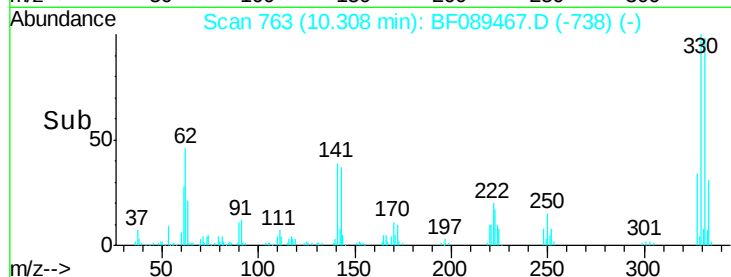



#44
 2-Fluorobiphenyl
 Concen: 85.15 ng
 RT: 8.86 min Scan# 636
 Delta R.T. -0.01 min
 Lab File: BF089467.D
 Acq: 31 Jul 2016 13:21

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.2	43.8
170	24.0	19.2	28.8

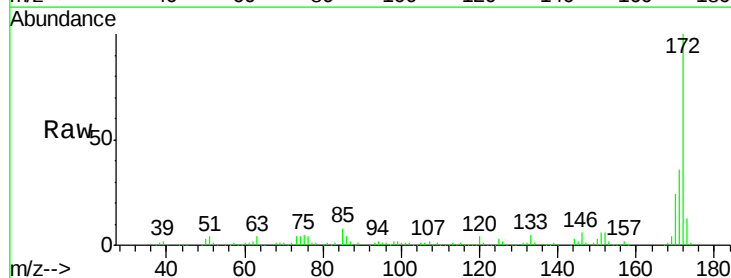

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

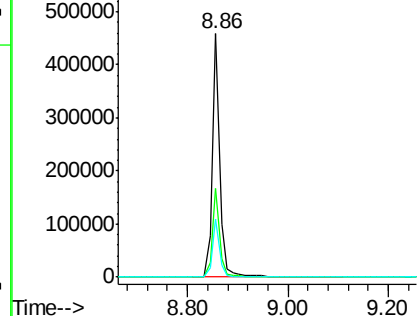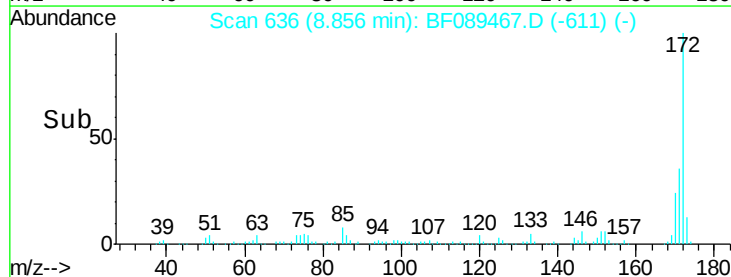


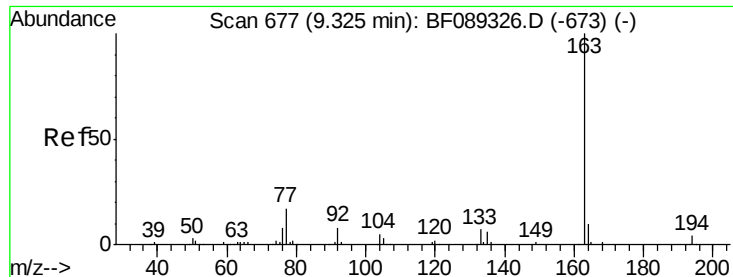




#49
Dimethylphthalate
Concen: 13.43 ng
RT: 9.26 min Scan# 671
Delta R.T. -0.02 min
Lab File: BF089467.D
Acq: 31 Jul 2016 13:21

Instrument :
BNA_F
ClientSampleId :
AB-SLOPE(0-4)J

Tot Ion:163 Resp: 83504
Ion Ratio Lower Upper
163 100
194 3.2 2.8 4.2
164 10.4 7.8 11.8

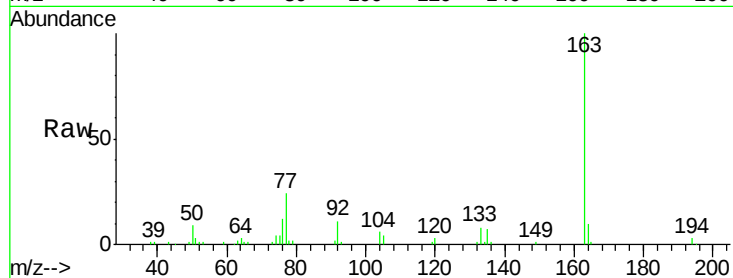


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

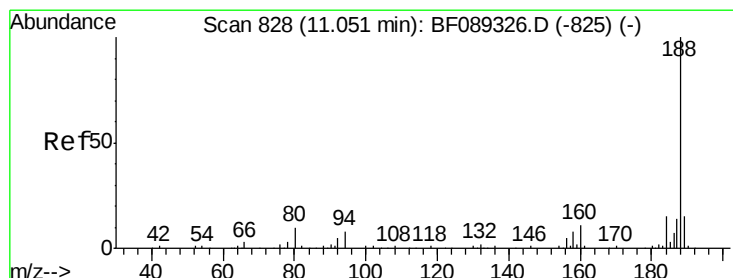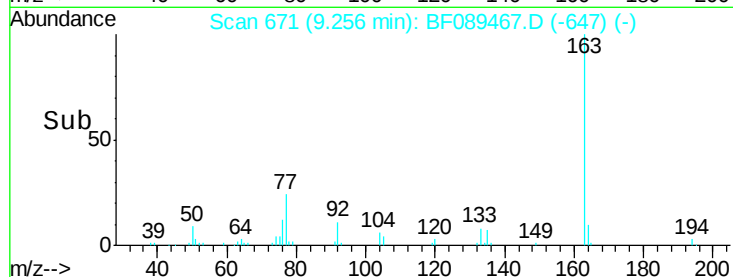
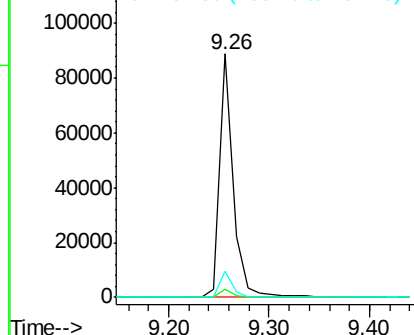



#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.99 min Scan# 823
Delta R.T. -0.01 min
Lab File: BF089467.D
Acq: 31 Jul 2016 13:21

Tgt Ion:188 Resp: 154708
Ion Ratio Lower Upper
188 100
94 8.1 6.5 9.7
80 8.9 7.2 10.8

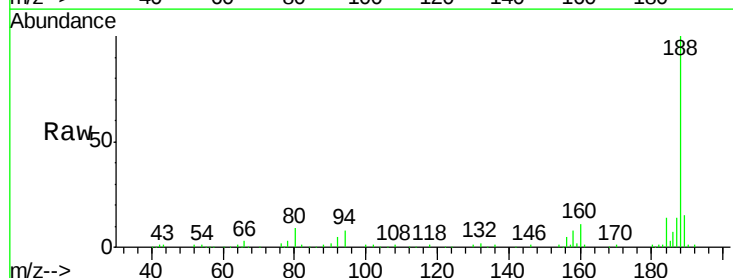

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

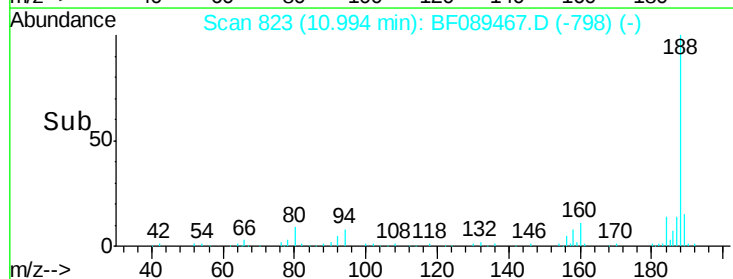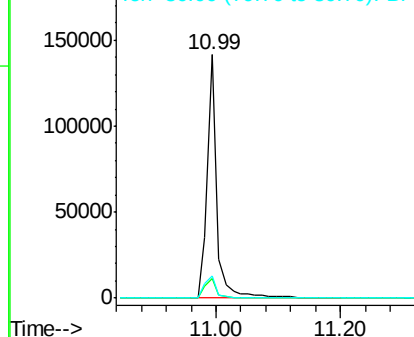

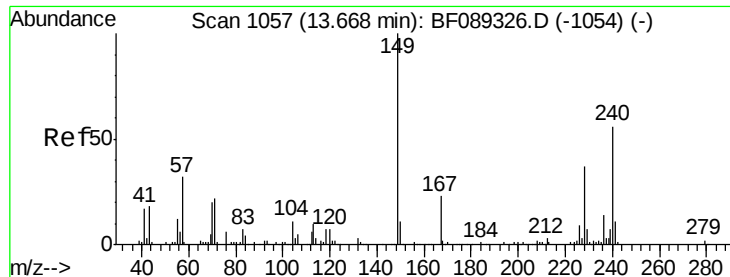

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.61 min Scan# 1052

Delta R.T. -0.01 min

Lab File: BF089467.D

Acq: 31 Jul 2016 13:21

Instrument :

BNA_F

ClientSampleId :

AB-SLOPE(0-4)J


Tot Ion:240 Resp: 99577

Ion Ratio Lower Upper

240 100

120 10.4 9.1 13.7




236 24.9 20.6 30.8

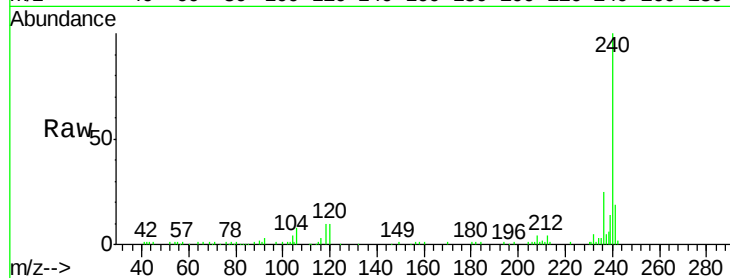

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

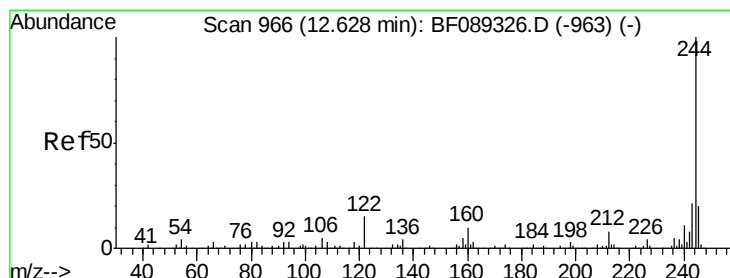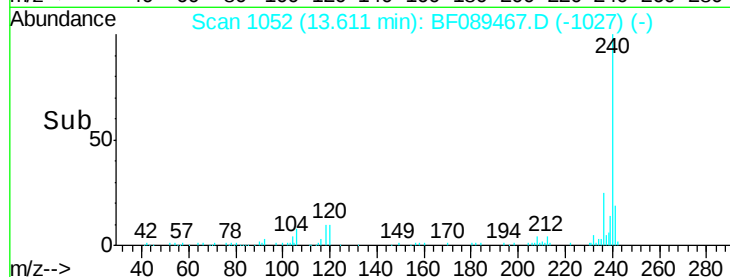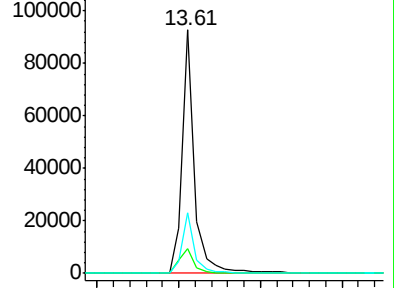

#78

Terphenyl-d14

Concen: 88.38 ng

RT: 12.57 min Scan# 961

Delta R.T. -0.01 min

Lab File: BF089467.D

Acq: 31 Jul 2016 13:21


Tgt Ion:244 Resp: 376020

Ion Ratio Lower Upper

244 100

212 8.4 6.5 9.7



122 17.0 11.4 17.0

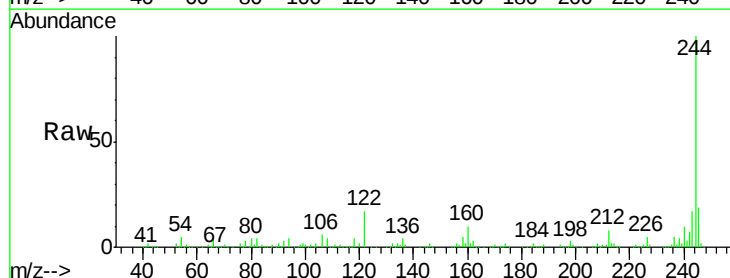


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

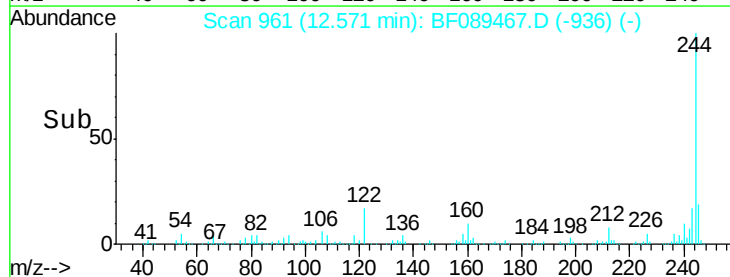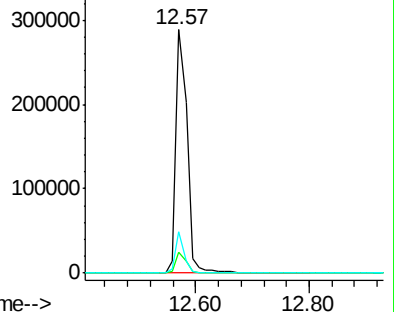


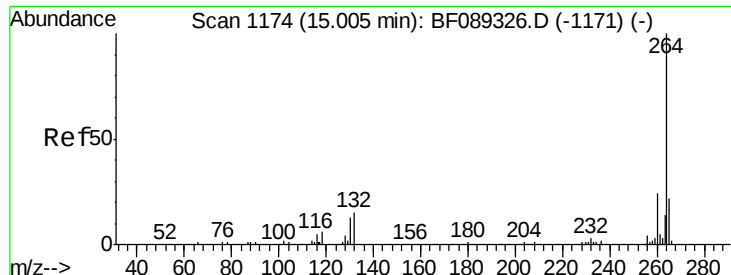

#86
Pervlene-d12
Concen: 20.00 ng
RT: 14.94 min Scan# 1168
Delta R.T. -0.01 min
Lab File: BF089467.D
Acq: 31 Jul 2016 13:21

Instrument :
BNA_F
ClientSampleId :
AB-SLOPE(0-4)J

Tot Ion:264 Resp: 74103
Ion Ratio Lower Upper
264 100
260 23.3 19.0 28.4
265 21.3 17.5 26.3

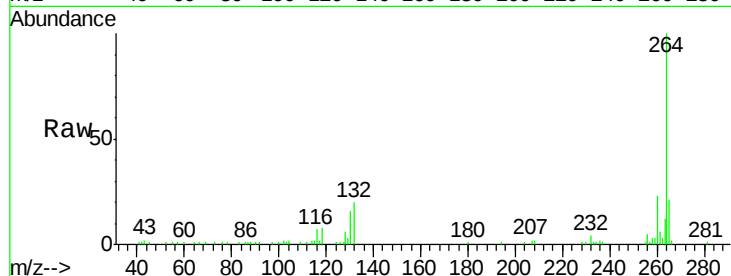

Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

