

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
 Data File : BF089484.D
 Acq On : 31 Jul 2016 21:48
 Operator : UM/SJ
 Sample : H4251-09 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSS-4

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.655	5	6	47	rVB	1292876	3524811	100.00%	73.736%
2	6.490	427	429	440	rBV	158257	184078	5.22%	3.851%
3	7.782	540	542	544	rBV	173631	193174	5.48%	4.041%
4	9.519	692	694	697	rBV	244544	214969	6.10%	4.497%
5	10.994	821	823	833	rBV	206994	201894	5.73%	4.223%
6	13.611	1050	1052	1060	rBV	254286	262264	7.44%	5.486%
7	14.937	1166	1168	1171	rBV	152609	199126	5.65%	4.166%




Sum of corrected areas: 4780316

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
Data File : BF089484.D
Acq On : 31 Jul 2016 21:48
Operator : UM/SJ
Sample : H4251-09 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSS-4

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

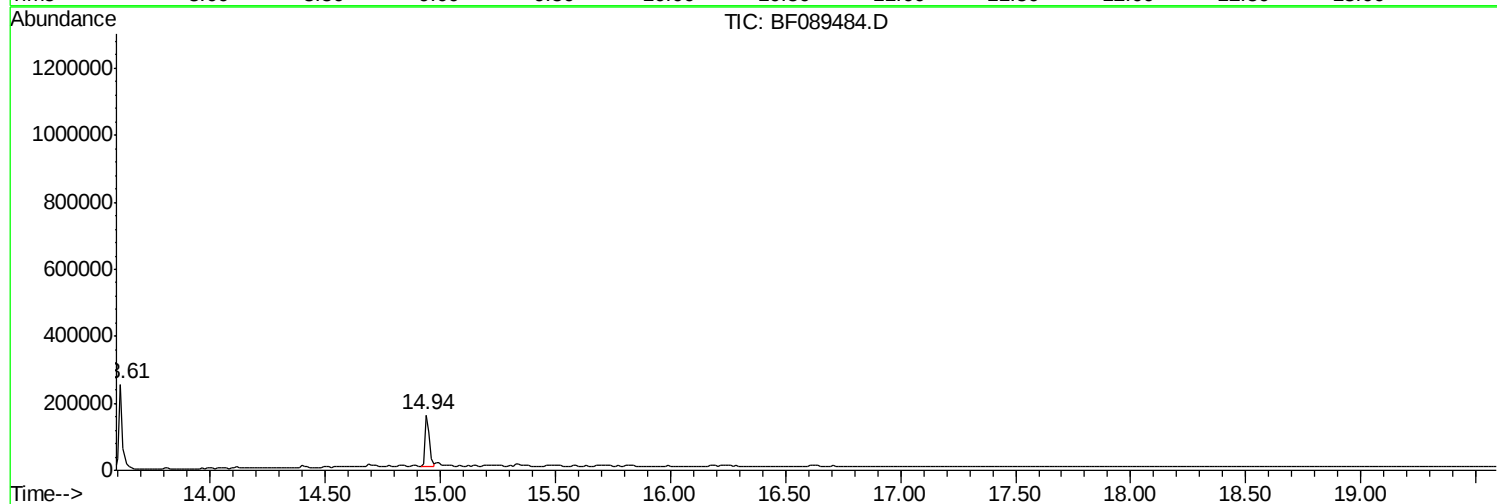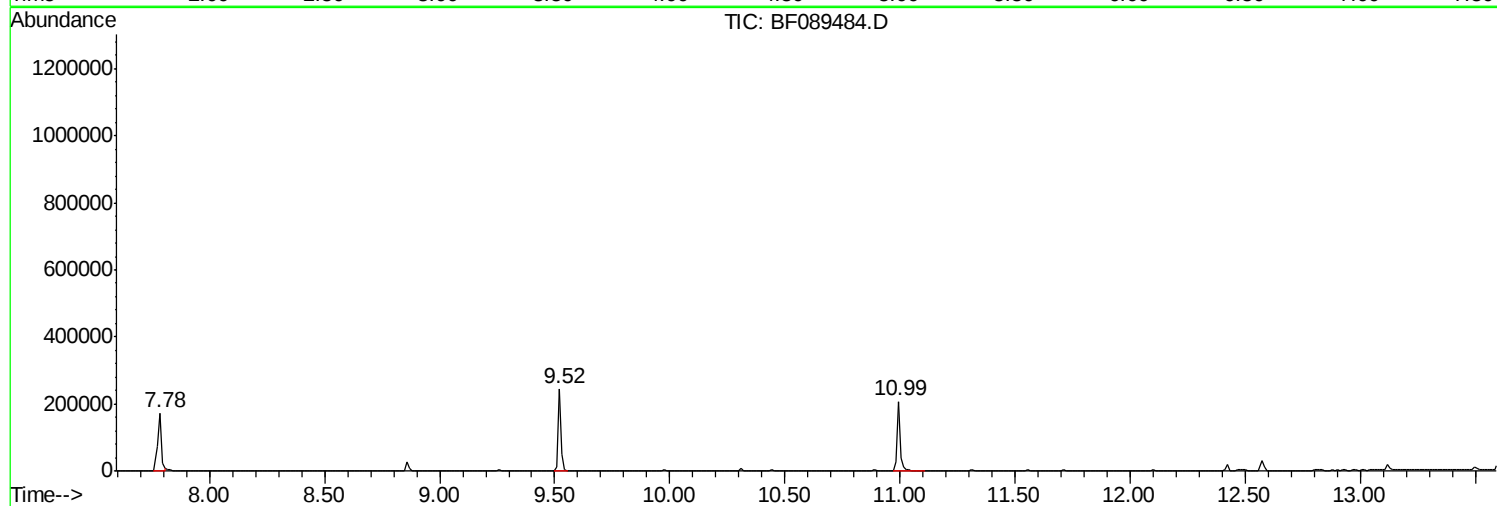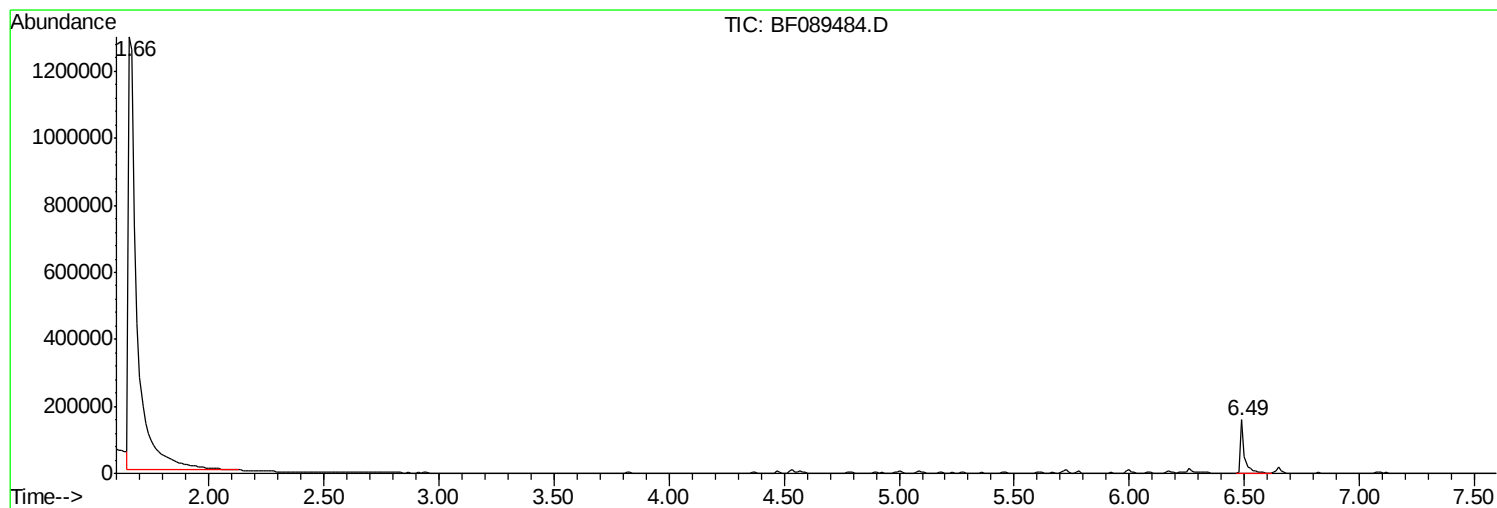

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
Data_File : BF089484.D
Acq_On : 31-Jul-2016 21:488
Operator : UM/SJJ
Sample : H4251-09_10XX
Misc :
ALS_Vial : 21 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
KSS-4

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
