

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
 Data File : BF089485.D
 Acq On : 31 Jul 2016 22:18
 Operator : UM/SJ
 Sample : H4251-10 10X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KSS-3

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.667	5	7	50	rVB	994843	2777172	100.00%	67.981%
2	6.490	427	429	440	rBV	173778	194384	7.00%	4.758%
3	7.782	540	542	544	rBV	191826	213004	7.67%	5.214%
4	9.519	692	694	697	rBV	255501	226644	8.16%	5.548%
5	10.993	821	823	836	rBV	229253	220014	7.92%	5.386%
6	13.611	1050	1052	1058	rBV	266455	267664	9.64%	6.552%
7	14.948	1166	1169	1172	rBV	118743	186361	6.71%	4.562%




Sum of corrected areas: 4085243

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
Data File : BF089485.D
Acq On : 31 Jul 2016 22:18
Operator : UM/SJ
Sample : H4251-10 10X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KSS-3

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

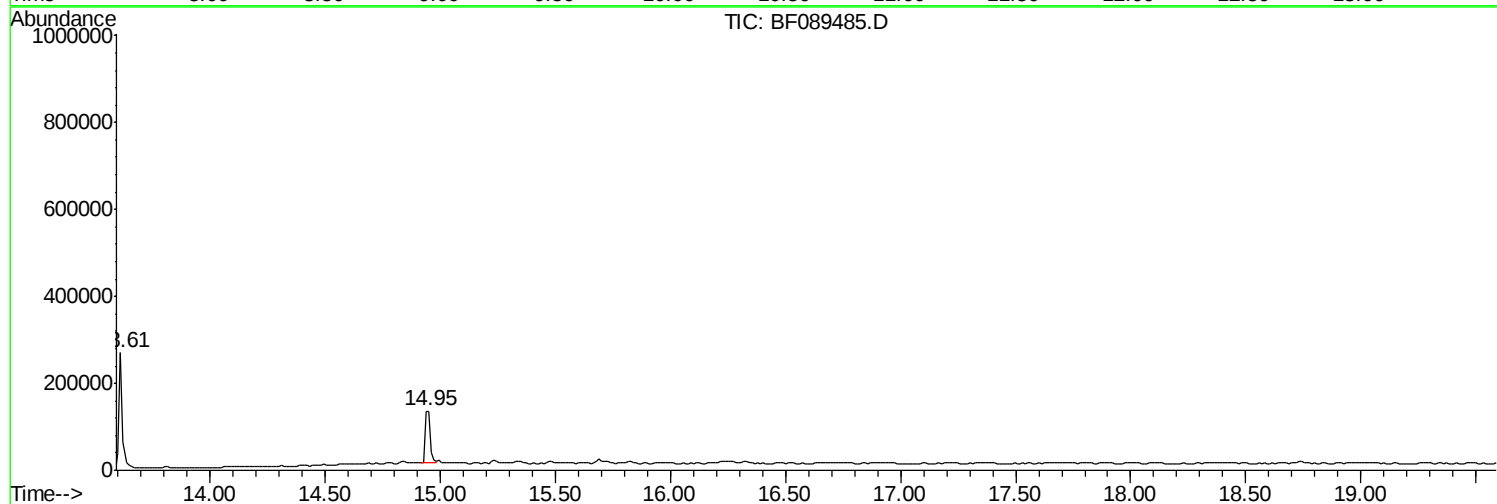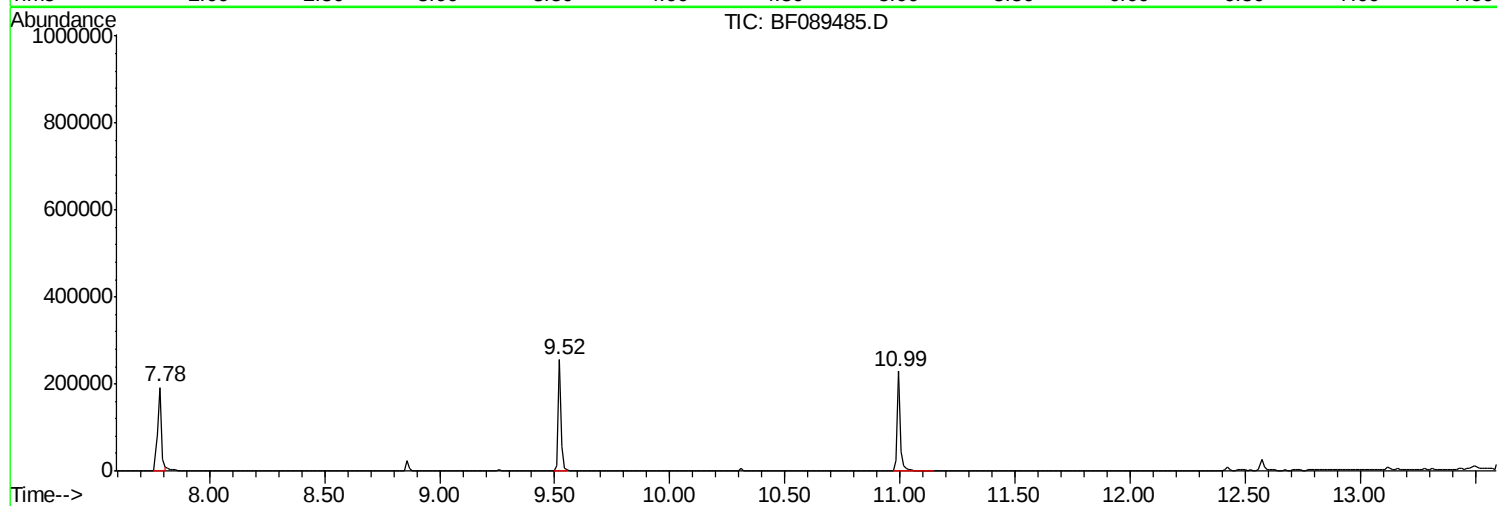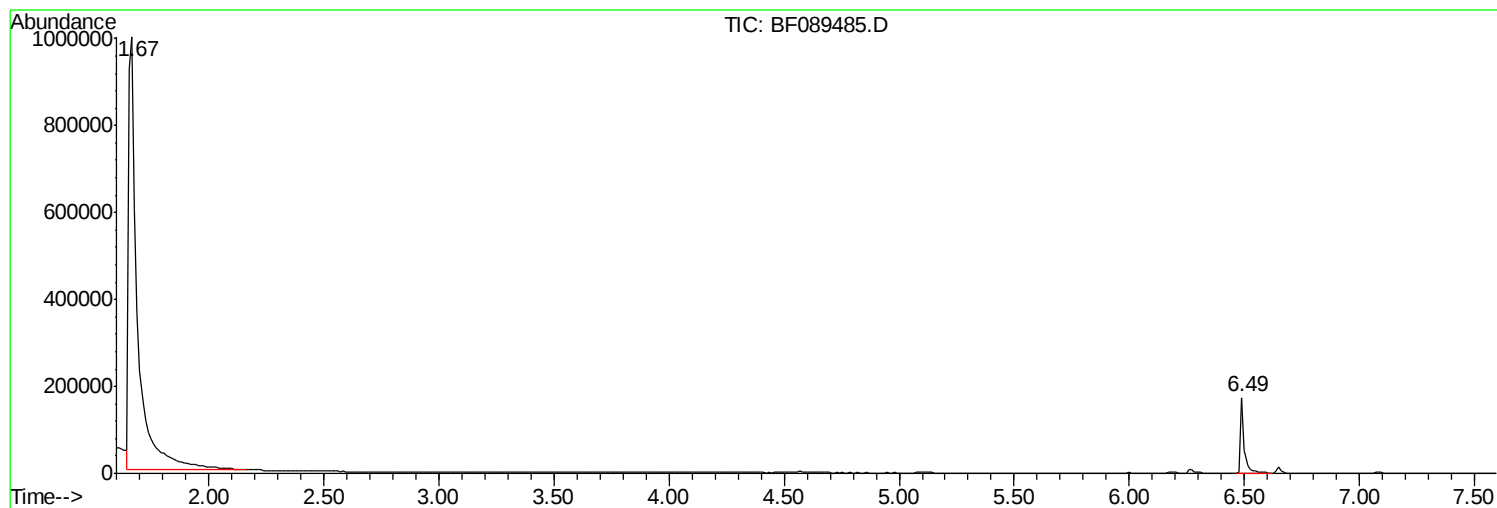

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
Data_File : BF089485.D
Acq_On : 31-Jul-2016 22:188
Operator : UM/SJJ
Sample : H4251-10_10XX
Misc :
ALS_Vial : 22 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
KSS-3

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\Database\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
				#	RT Resp Conc

No Library Search Compounds Detected
