


Data Path : Z:\HPCHEM1\BNA F\DATA\BF073116\
 Data File : BF089448.D
 Acq On : 30 Jul 2016 11:46
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 16:02:32 2016

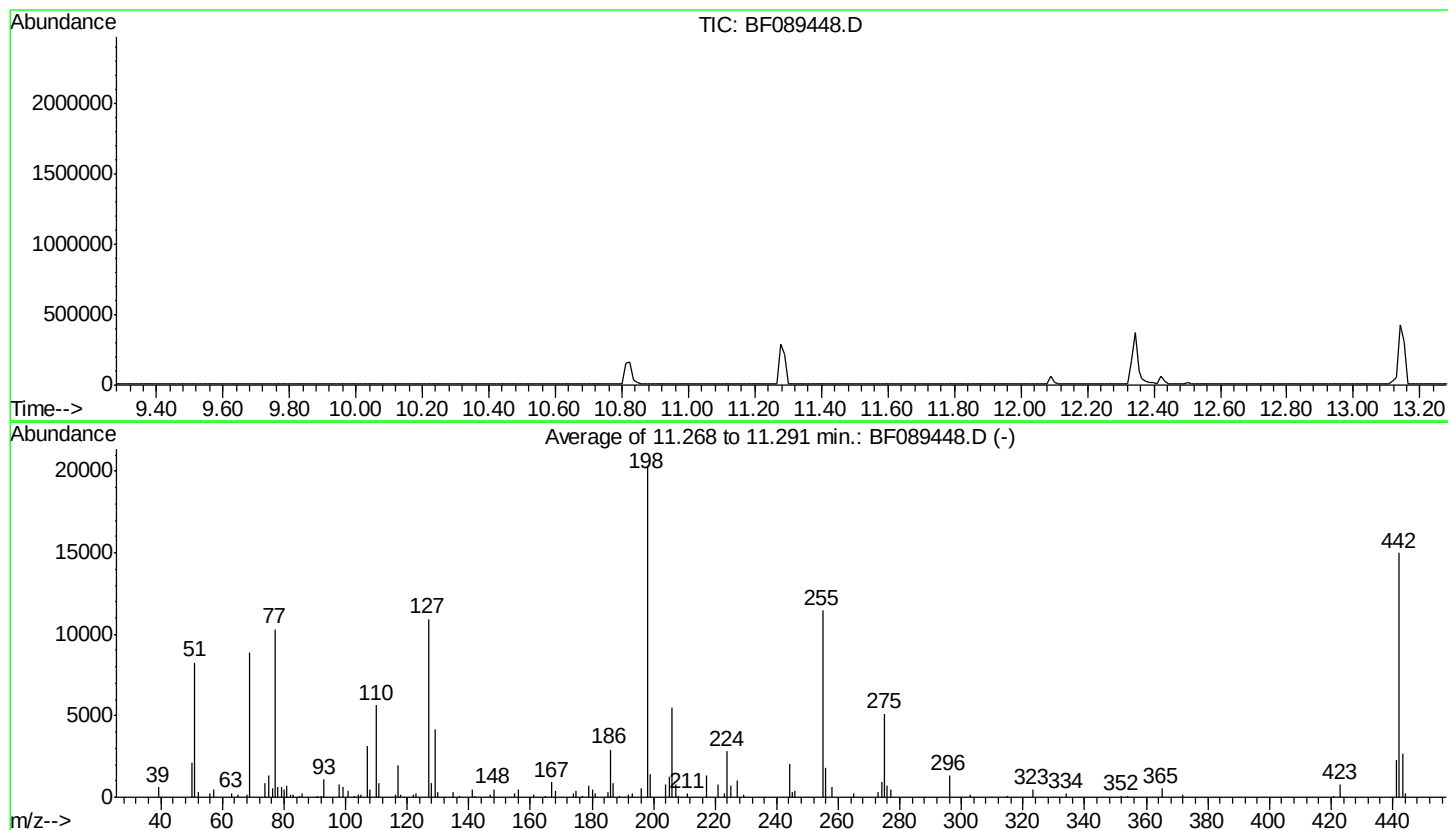

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	8274	PASS
68	69	0.00	2	1.7	150	PASS
69	198	0.00	100	43.5	8860	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.8	10942	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20349	PASS
199	198	5	9	7.0	1422	PASS
275	198	10	60	25.3	5142	PASS
365	198	1	100	2.7	549	PASS
441	442	0.01	24	15.3	2293	PASS
442	198	50	100	73.6	14982	PASS
443	442	15	24	18.0	2692	PASS