


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF073116\
 Data File : BF089464.D
 Acq On : 31 Jul 2016 10:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 16:02:32 2016

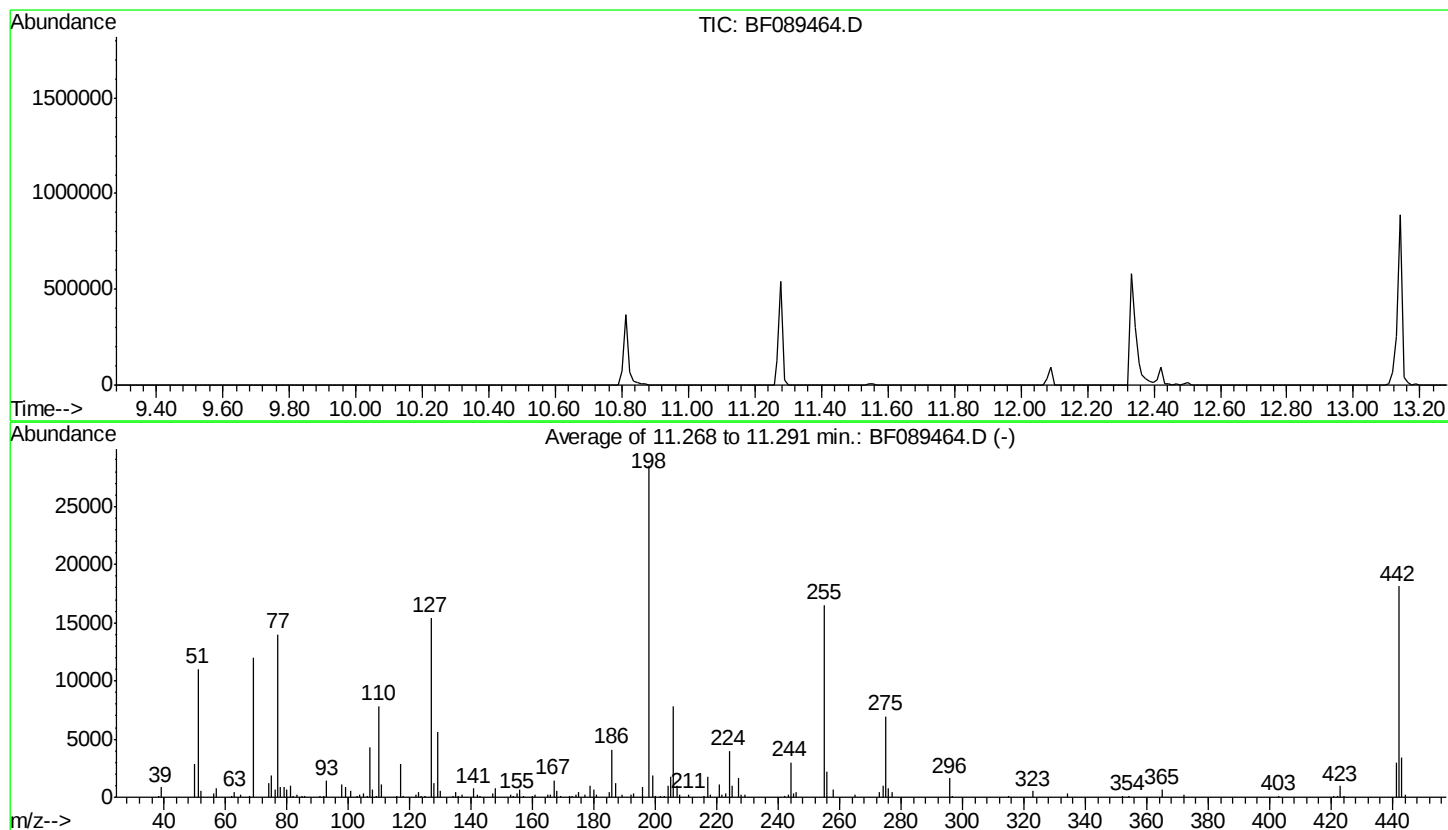

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.8	11056	PASS
68	69	0.00	2	1.3	159	PASS
69	198	0.00	100	41.9	11955	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.1	15413	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28504	PASS
199	198	5	9	6.6	1876	PASS
275	198	10	60	24.4	6948	PASS
365	198	1	100	2.3	648	PASS
441	442	0.01	24	16.3	2959	PASS
442	198	50	100	63.5	18104	PASS
443	442	15	24	19.0	3447	PASS