


Data Path : Z:\HPCHEM1\BNA F\DATA\BF073116\
 Data File : BF089487.D
 Acq On : 31 Jul 2016 23:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 16:02:32 2016

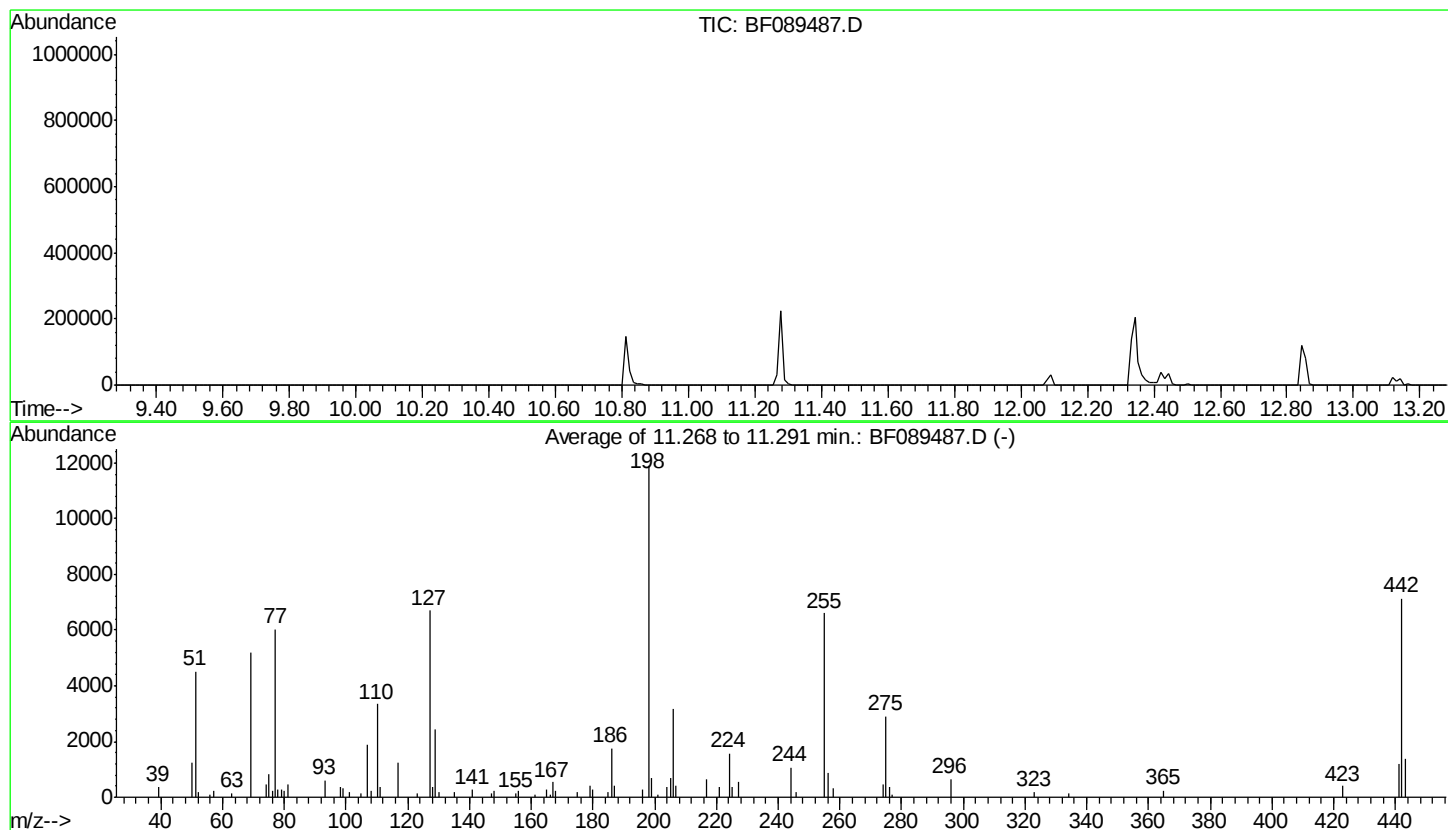

AutoFind: Scans 847, 848, 849; Background Corrected with Scan 844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.0	4526	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	43.5	5182	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.3	6698	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	11904	PASS
199	198	5	9	5.9	699	PASS
275	198	10	60	24.4	2905	PASS
365	198	1	100	2.0	238	PASS
441	442	0.01	24	16.4	1175	PASS
442	198	50	100	60.0	7144	PASS
443	442	15	24	19.5	1395	PASS