
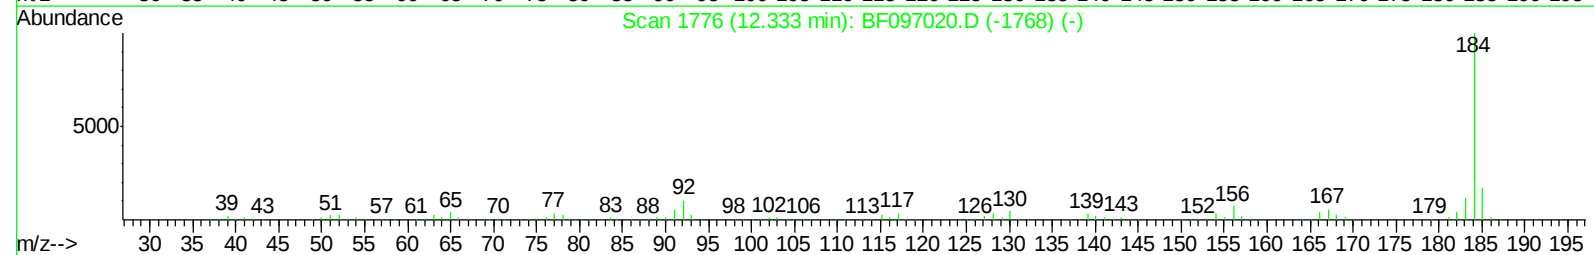
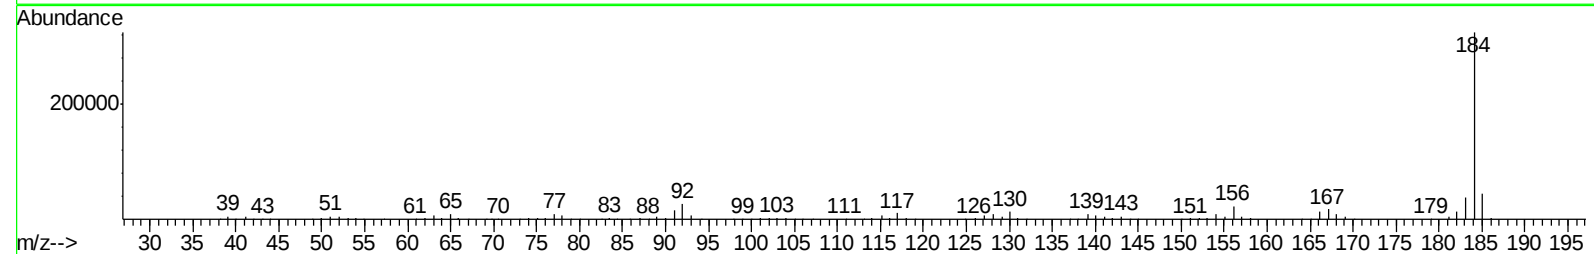


Data Path : Z:\HPCHEM1\BNA F\DATA\BF073117\
 Data File : BF097200.D
 Acq On : 31 Jul 2017 11:11
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 06:13:23 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 14:11:51 2017
 Response via : Initial Calibration

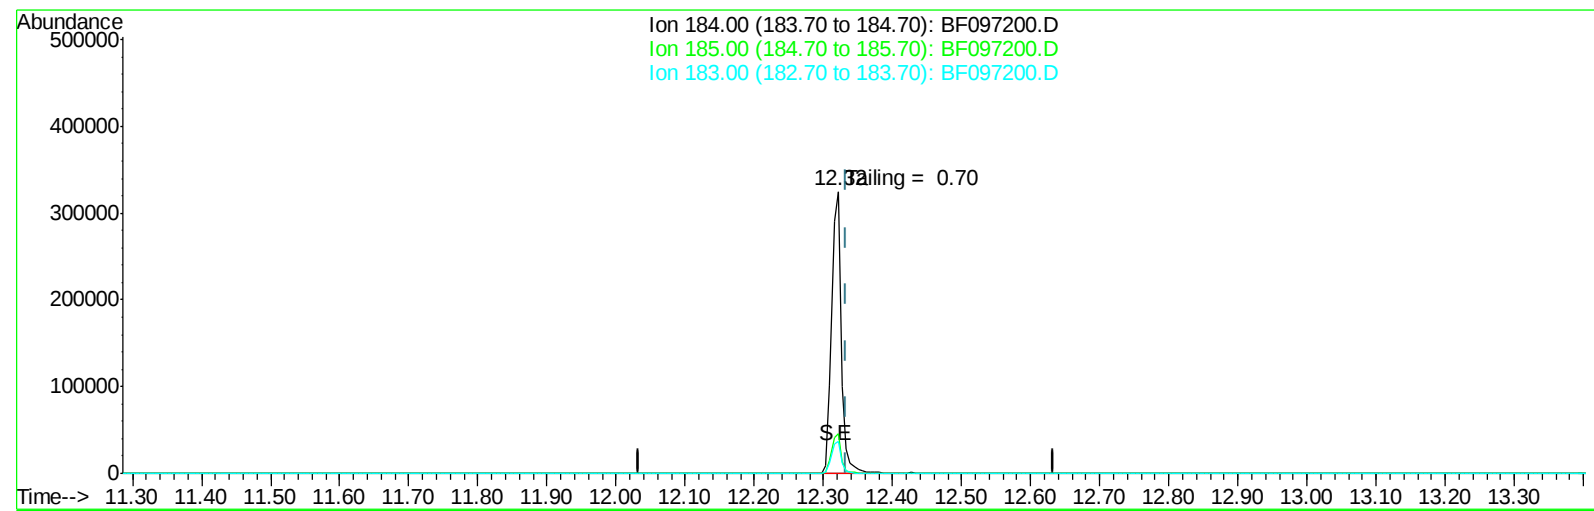

TIC: BF097200.D

(76) Benzidine




12.321min (-0.012) 73489.81ng

response 313585

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.91#
183.00	12.20	11.60
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF073117\
Data File : BF097200.D
Acq On : 31 Jul 2017 11:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 06:13:23 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

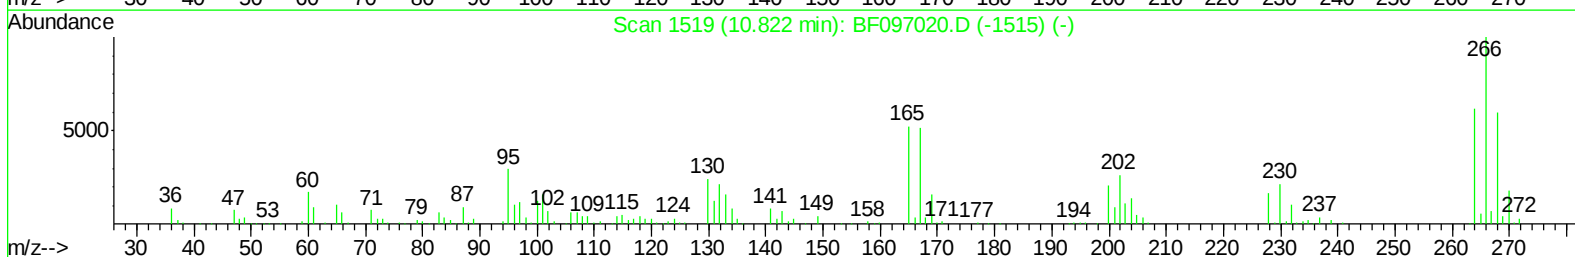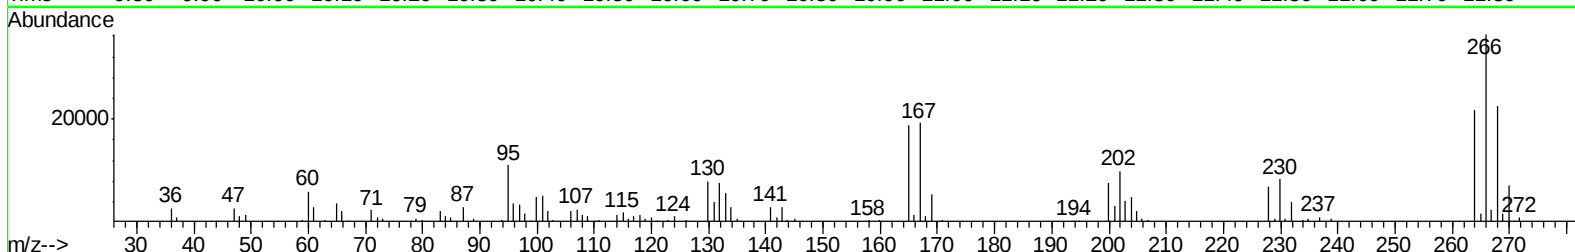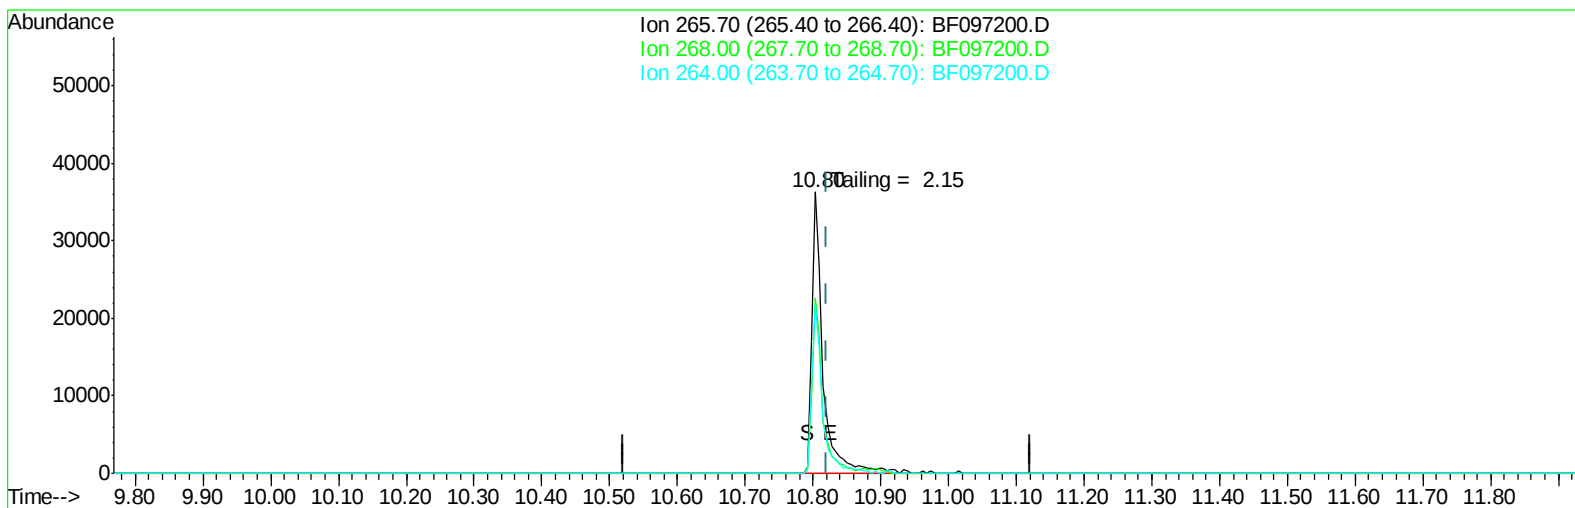

TIC: BF097200.D

(69) Pentachlorophenol (C)

10.804min (-0.017) 72368.42ng

response 41552

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.15
264.00	64.60	60.17
0.00	0.00	0.00