


Data Path : Z:\HPCHEM1\BNA F\Data\BF073117\
Data File : BF097200.D
Acq On : 31 Jul 2017 11:11
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 25 14:11:51 2017

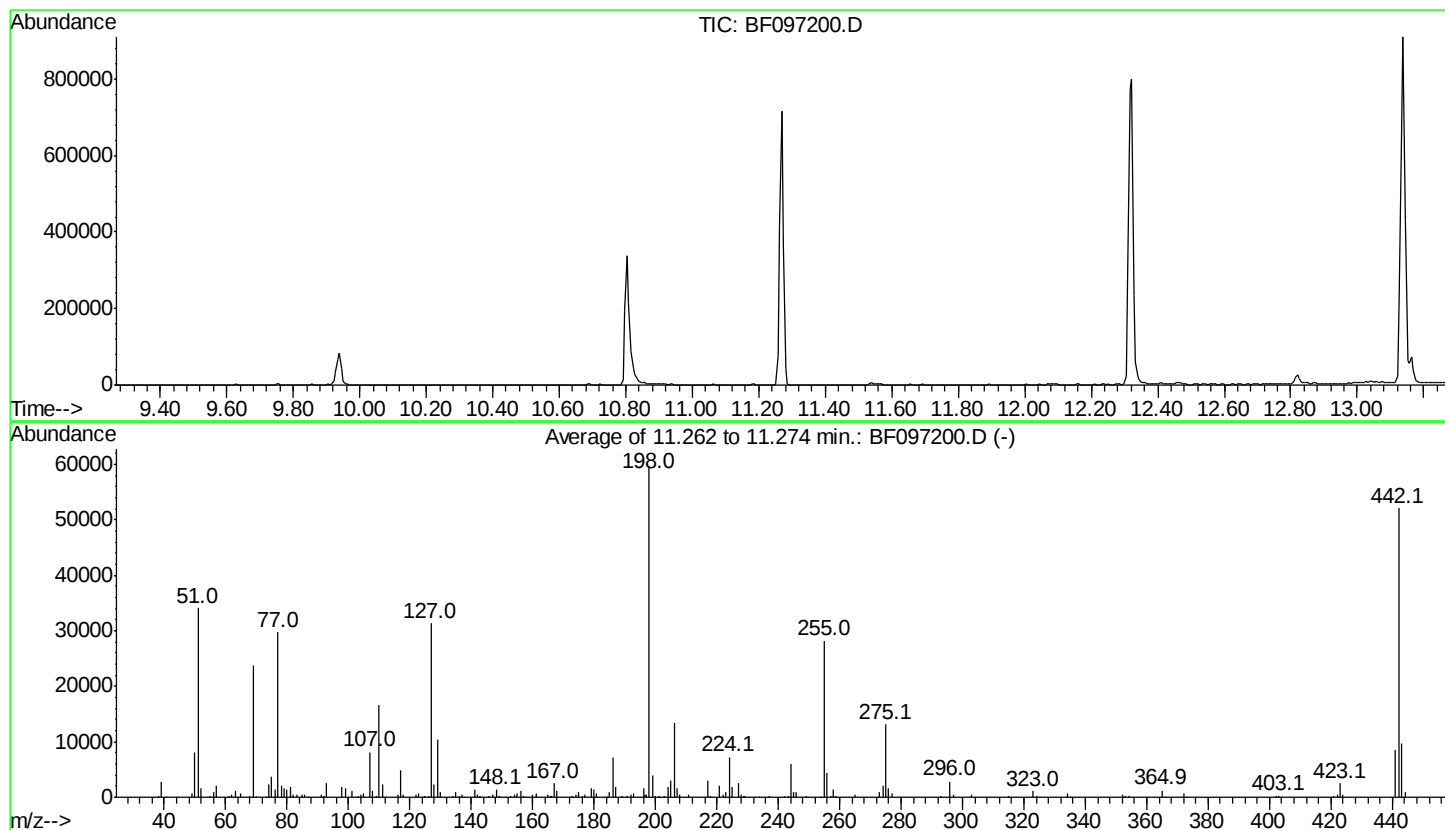

AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	57.1	34096	PASS
68	69	0.00	2	1.5	347	PASS
69	198	0.00	100	39.8	23811	PASS
70	69	0.00	2	0.4	107	PASS
127	198	10	80	52.4	31288	PASS
197	198	0.00	2	0.7	419	PASS
198	198	100	100	100.0	59762	PASS
199	198	5	9	6.6	3917	PASS
275	198	10	60	21.9	13064	PASS
365	198	1	100	2.1	1242	PASS
441	442	0.01	24	16.3	8492	PASS
442	198	50	100	87.1	52040	PASS
443	442	15	24	18.6	9687	PASS