
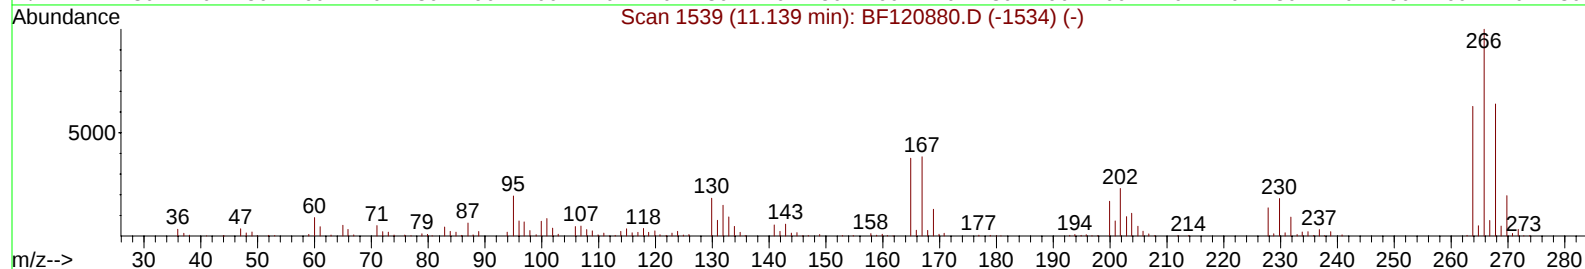
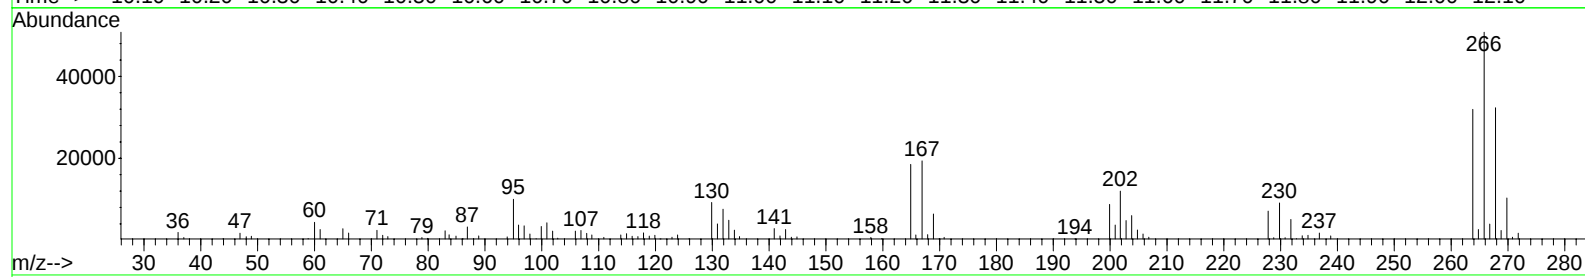


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073120\  
 Data File : BF121147.D  
 Acq On : 31 Jul 2020 9:29  
 Operator : JU/CG  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 17:48:04 2020  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Jul 29 14:55:43 2020  
 Response via : Initial Calibration

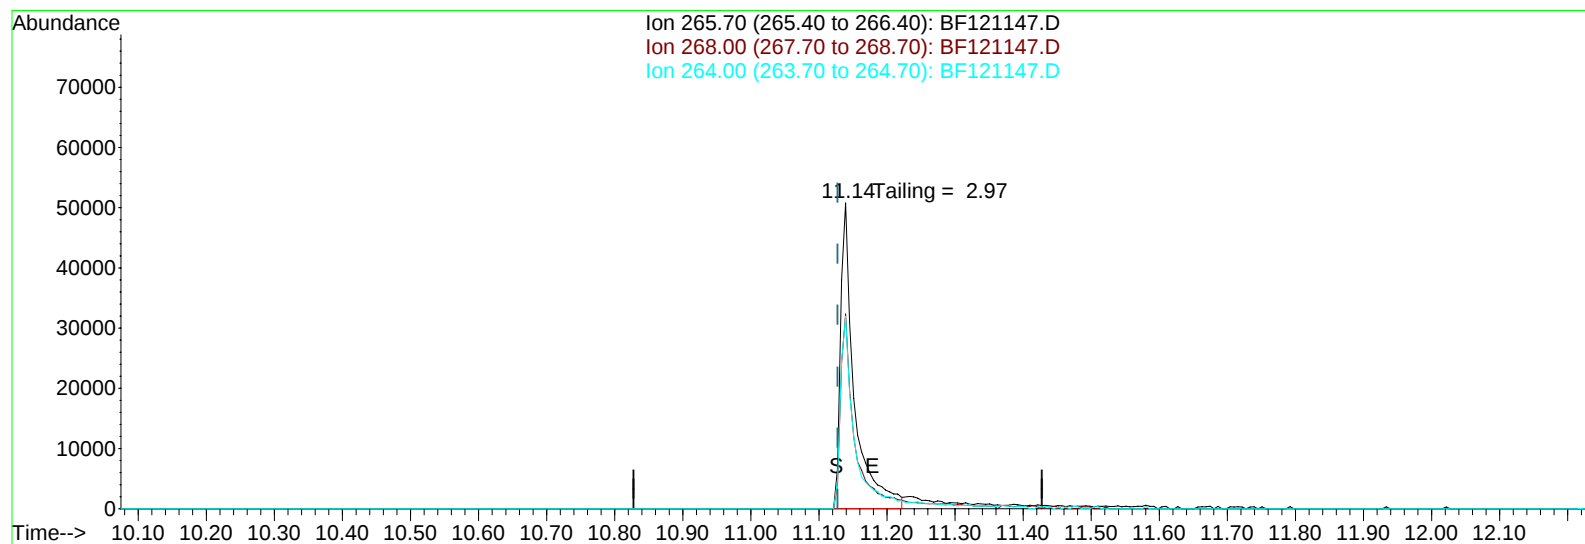

TIC: BF121147.D

(70) Pentachlorophenol (C)




11.139min (+0.012) 43905.01ng

response 73108

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.10 | 63.69 |
| 264.00 | 63.00 | 62.92 |
| 0.00   | 0.00  | 0.00  |

```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073120\  
Data File   : BF121147.D  
Acq On      : 31 Jul 2020    9:29  
Operator    : JU/CG  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Jul 31 17:48:04 2020  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Jul 29 14:55:43 2020  
Response via : Initial Calibration

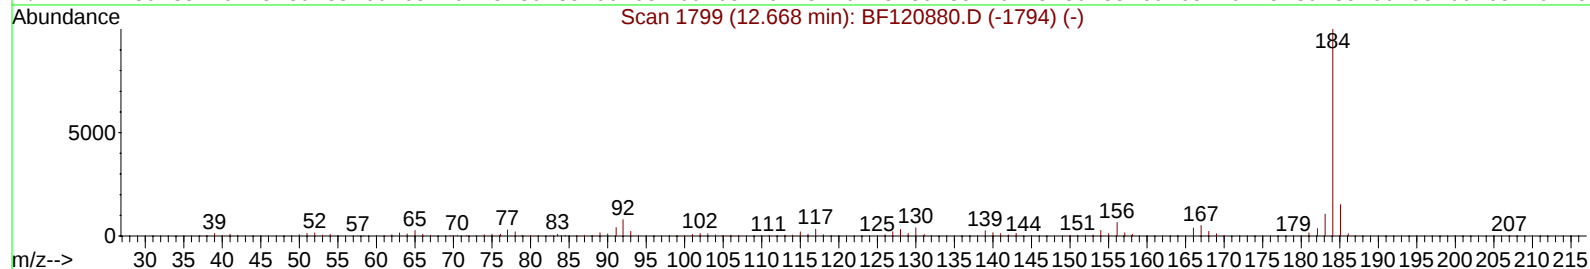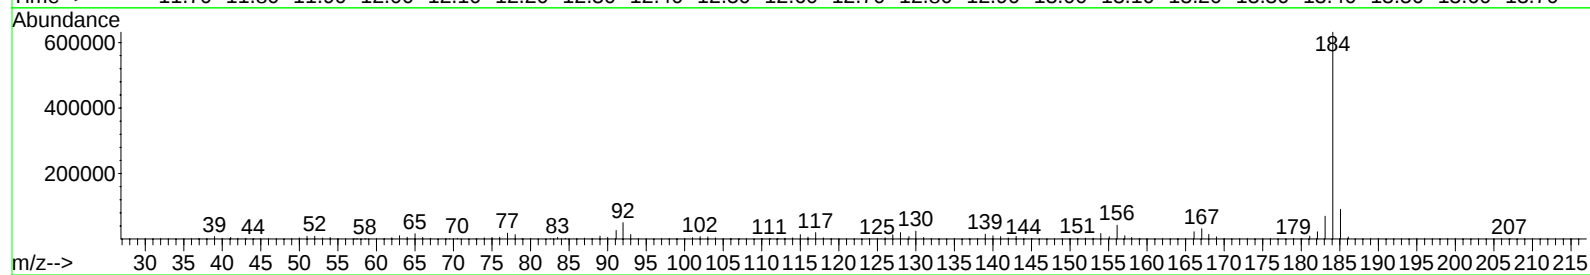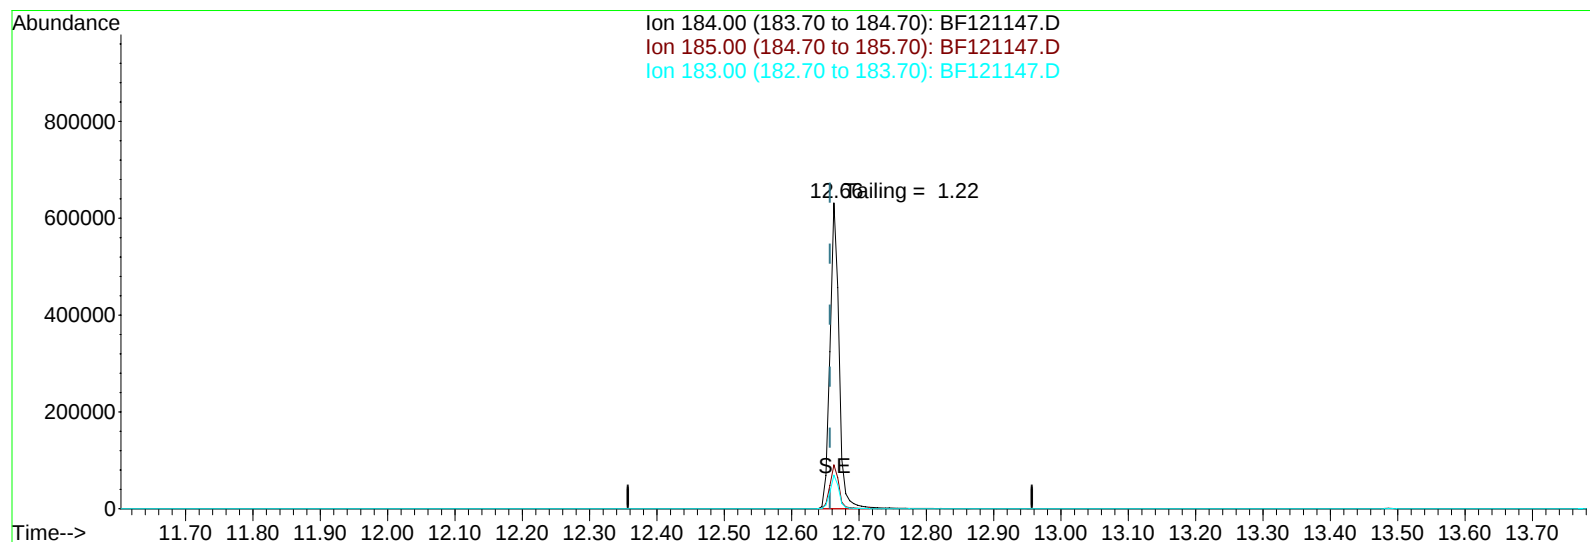

TIC: BF121147.D

(77) Benzidine

12.663min (+0.006) 165955.42ng

response 593404

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.10 | 14.34 |
| 183.00 | 11.20 | 11.01 |
| 0.00   | 0.00  | 0.00  |