

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073120\
 Data File : BF121154.D
 Acq On : 31 Jul 2020 13:22
 Operator : JU/CG
 Sample : L3518-17
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-7

Quant Time: Jul 31 14:33:22 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 29 14:55:43 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	125897	20.00	ng	0.00
21) Naphthalene-d8	8.08	136	479757	20.00	ng	0.00
39) Acenaphthene-d10	9.83	164	247789	20.00	ng	0.00
64) Phenanthrene-d10	11.32	188	464471	20.00	ng	0.00
76) Chrysene-d12	13.96	240	319283	20.00	ng	0.00
86) Perylene-d12	15.42	264	285338	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.42	112	702718	91.50	ng	0.00
7) Phenol-d6	6.43	99	868877	87.59	ng	-0.01
23) Nitrobenzene-d5	7.36	82	577156	69.61	ng	-0.02
42) 2,4,6-Tribromophenol	10.63	330	258782	95.41	ng	0.00
45) 2-Fluorobiphenyl	9.16	172	1039915	62.66	ng	0.00
79) Terphenyl-d14	12.92	244	994865	67.73	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.55	163	103267	5.777	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073120\
Data File : BF121154.D
Acq On : 31 Jul 2020 13:22
Operator : JU/CG
Sample : L3518-17
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-7

Quant Time: Jul 31 14:33:22 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 29 14:55:43 2020
Response via : Initial Calibration

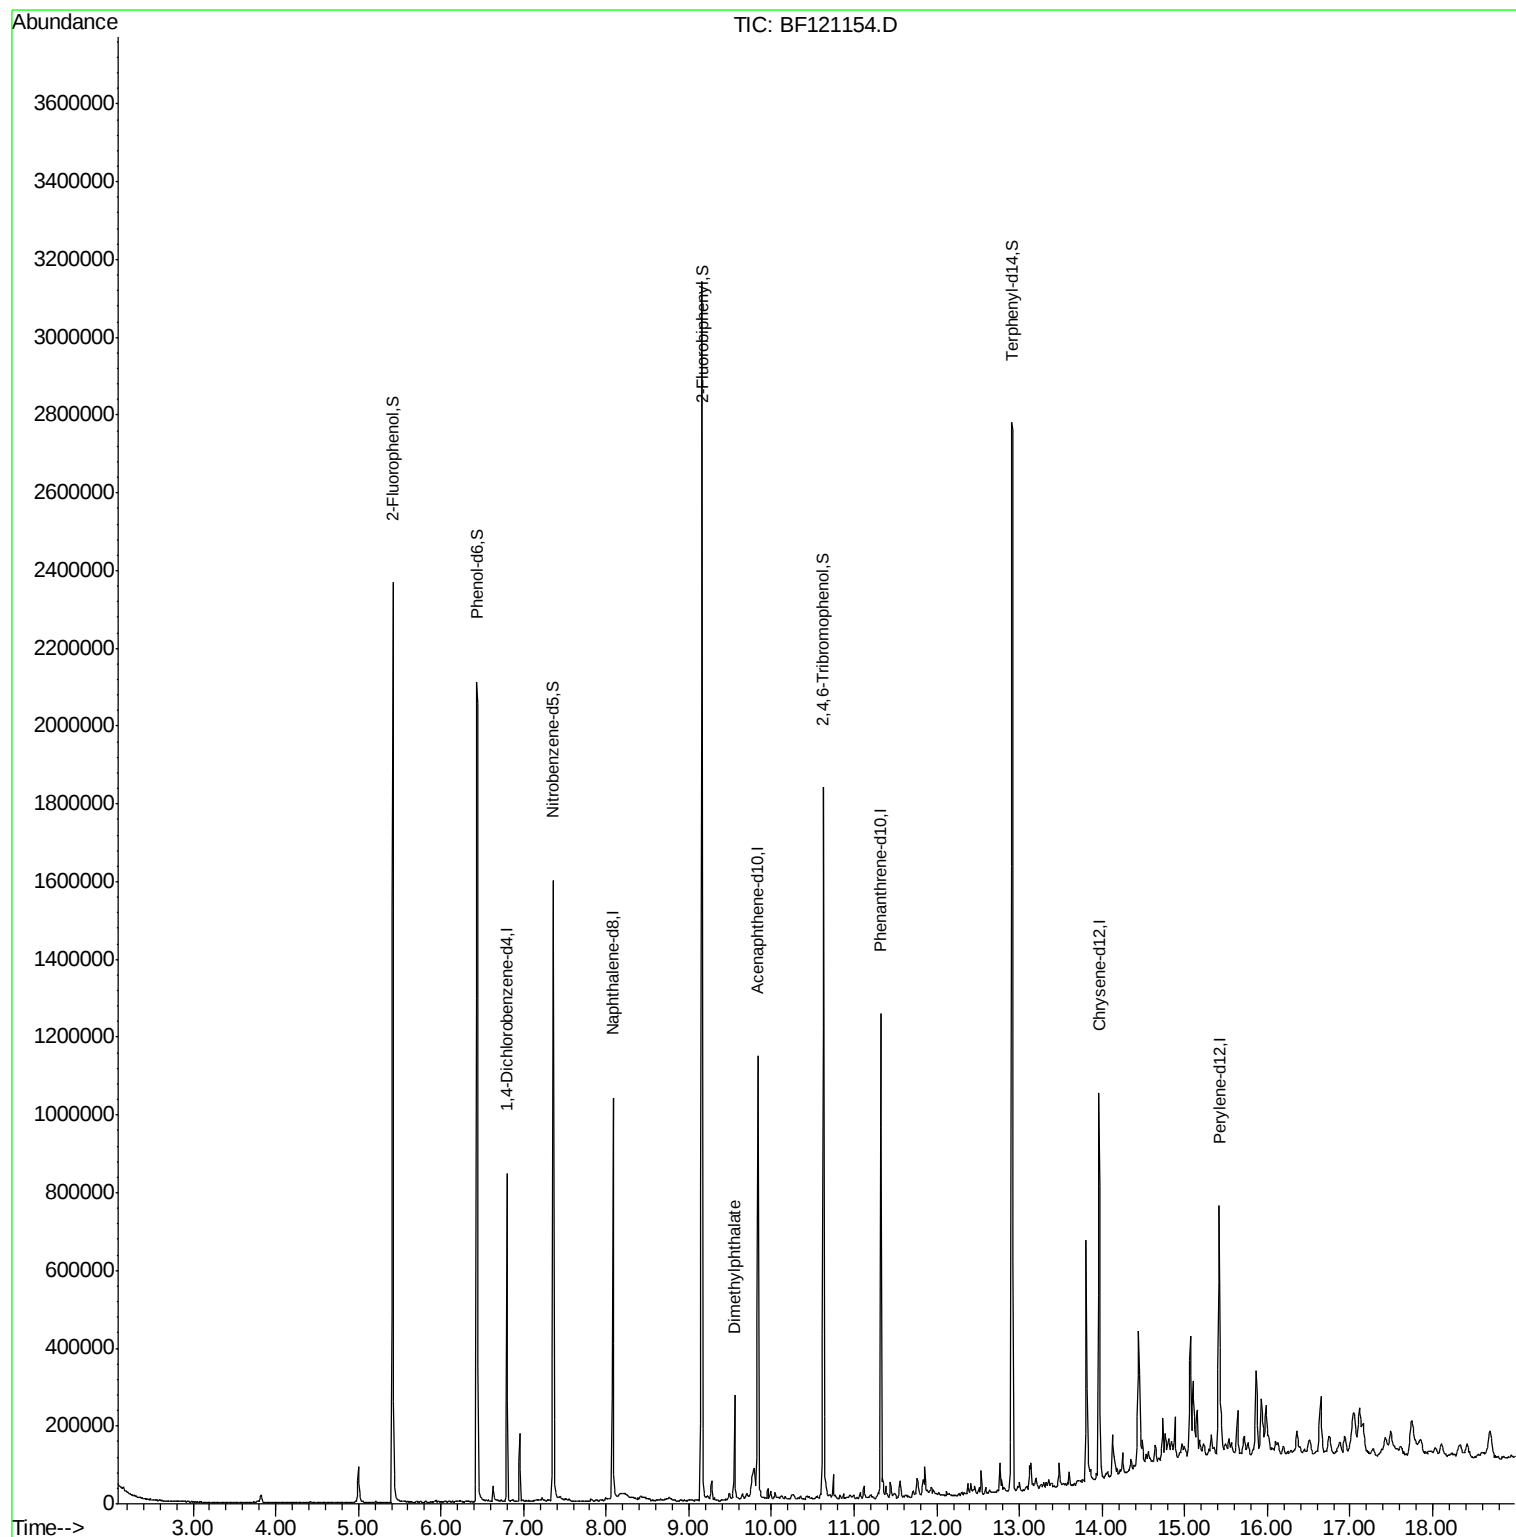

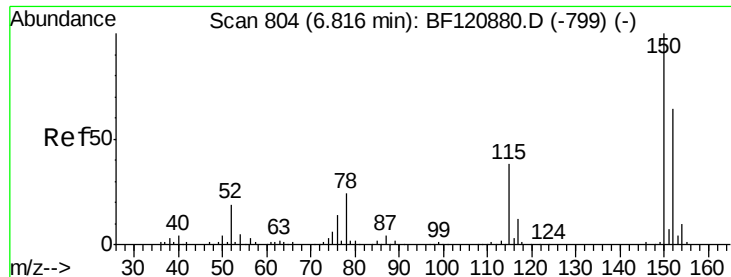


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.80 min Scan# 801
Delta R.T. -0.01 min
Lab File: BF121154.D
Acq: 31 Jul 2020 13:22

Instrument :
BNA_F
ClientSampleId :
TP-7

Tot Ion:152 Resp: 125897
Ion Ratio Lower Upper
152 100
150 156.7 125.6 188.4
115 57.8 46.2 69.2

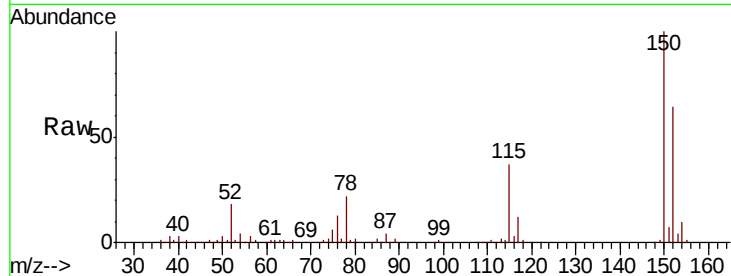


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

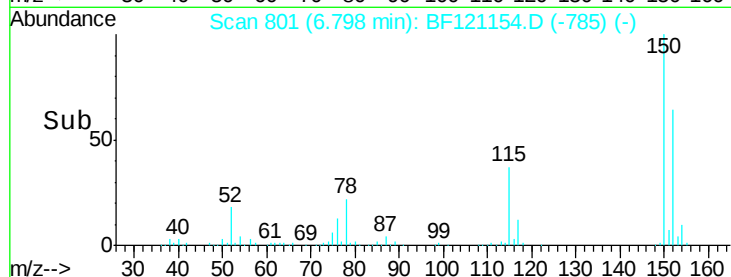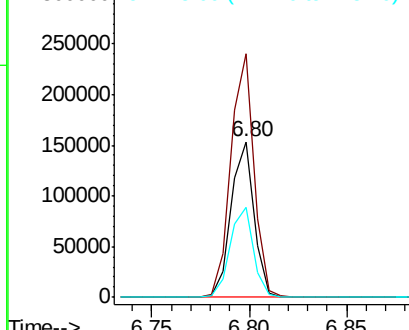



#5



2-Fluorophenol
Concen: 91.504 ng
RT: 5.42 min Scan# 566
Delta R.T. 0.00 min
Lab File: BF121154.D
Acq: 31 Jul 2020 13:22

Tgt Ion:112 Resp: 702718
Ion Ratio Lower Upper
112 100
64 54.4 43.9 65.9
63 27.6 22.7 34.1

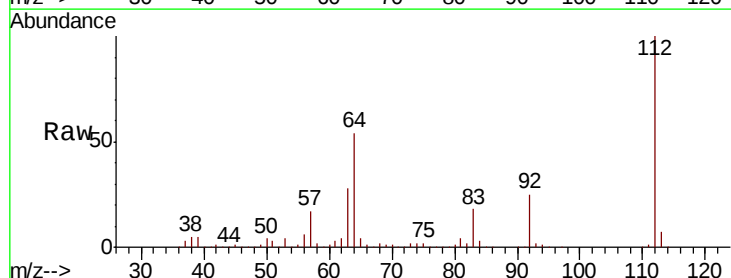

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

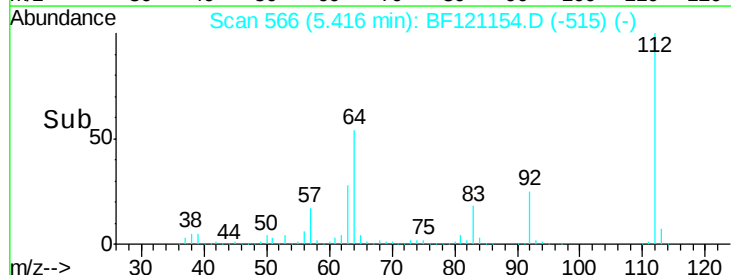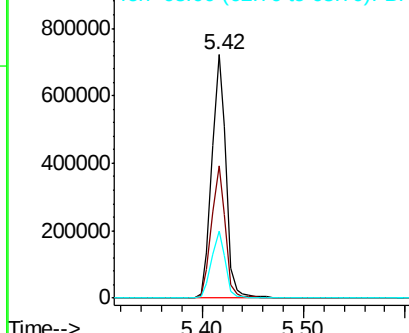

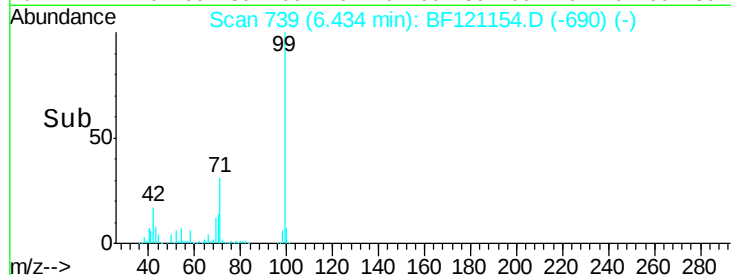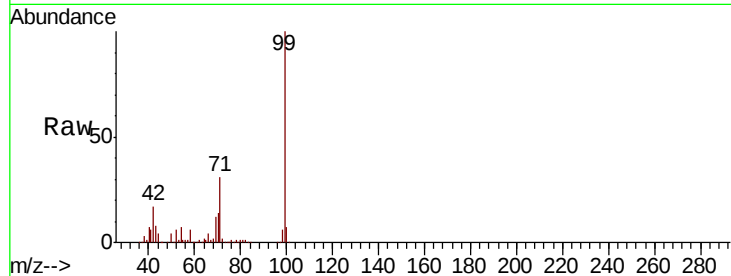

#7

Phenol-d6

Concen: 87.587 ng

RT: 6.43 min Scan# 739

Delta R.T. -0.01 min

Lab File: BF121154.D

Acq: 31 Jul 2020 13:22

Instrument :

BNA_F

ClientSampleId :

TP-7




Tot Ion: 99 Resp: 868877

Ion Ratio Lower Upper

99 100

42 17.0 13.5 20.3

71 31.3 25.0 37.4

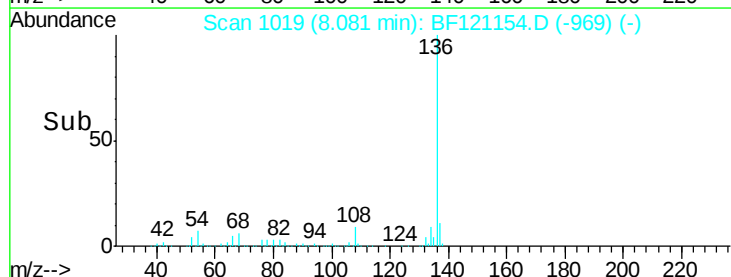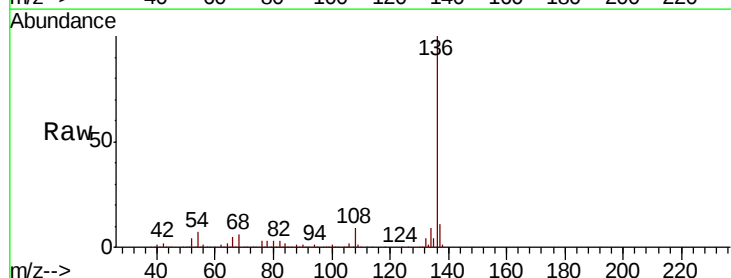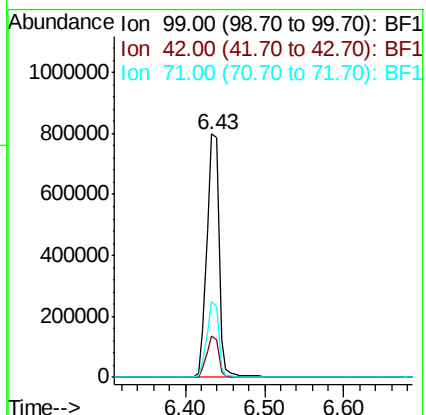

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.08 min Scan# 1019

Delta R.T. -0.01 min

Lab File: BF121154.D

Acq: 31 Jul 2020 13:22

Tgt Ion: 136 Resp: 479757


Ion Ratio Lower Upper


136 100

137 11.0 9.0 13.4

54 6.9 6.1 9.1

68 5.6 5.0 7.6

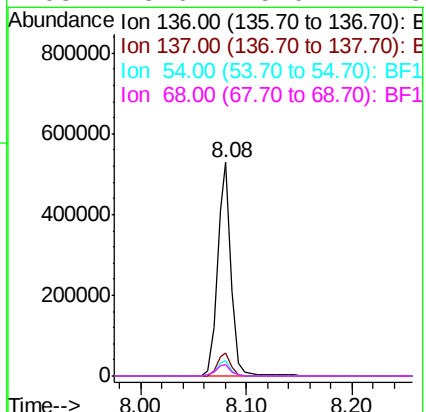

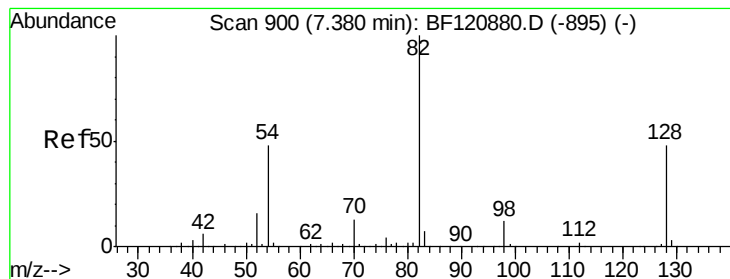

#23

Nitrobenzene-d5

Concen: 69.610 ng

RT: 7.36 min Scan# 896

Delta R.T. -0.02 min

Lab File: BF121154.D

Acq: 31 Jul 2020 13:22

Instrument :

BNA_F

ClientSampleId :

TP-7


Tot Ion: 82 Resp: 577156

Ion Ratio Lower Upper

82 100

128 47.6 39.2 58.8




54 49.2 37.8 56.8

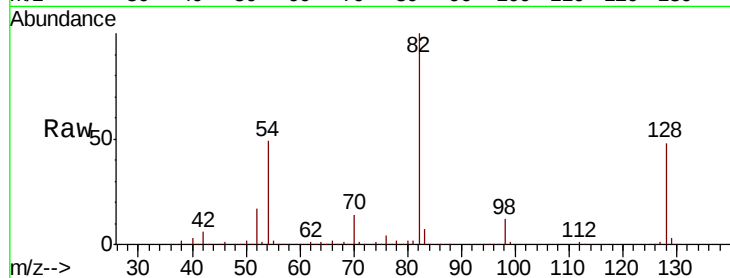

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): BF1

Ion 54.00 (53.70 to 54.70): BF1

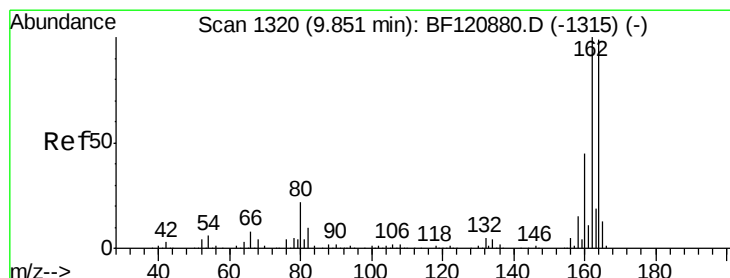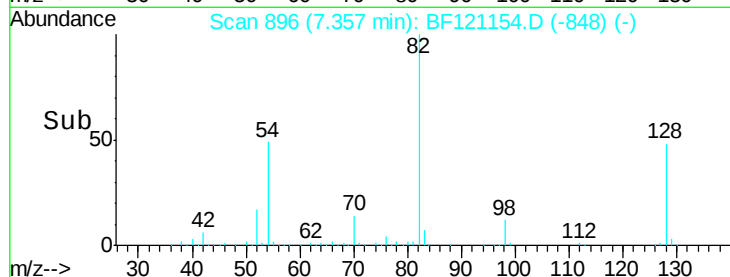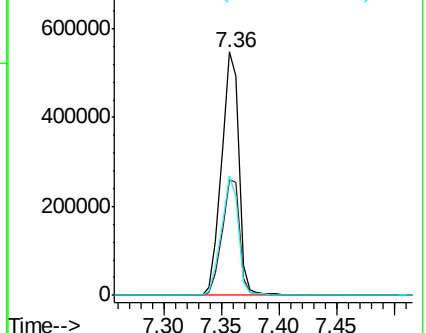

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.83 min Scan# 1317

Delta R.T. -0.01 min

Lab File: BF121154.D

Acq: 31 Jul 2020 13:22


Tgt Ion:164 Resp: 247789

Ion Ratio Lower Upper

164 100

162 100.5 82.2 123.2



160 45.8 37.2 55.8

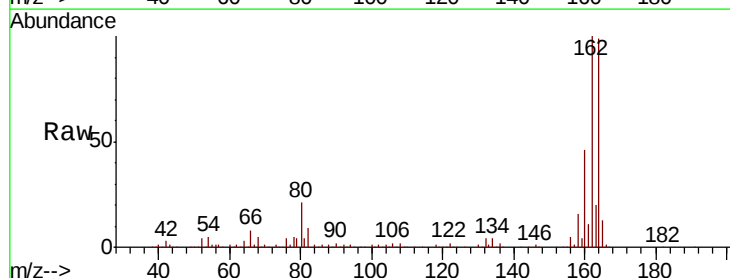

Abundance Ion 164.00 (163.70 to 164.70): BF1

Ion 162.00 (161.70 to 162.70): BF1

Ion 160.00 (159.70 to 160.70): BF1


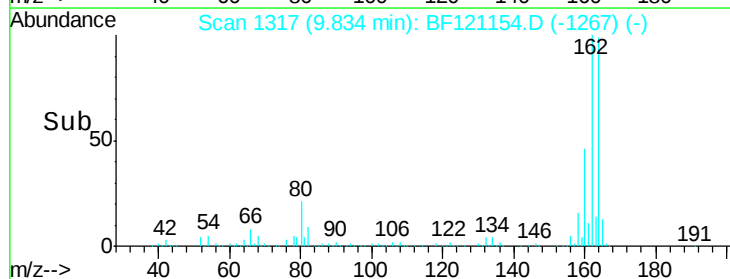
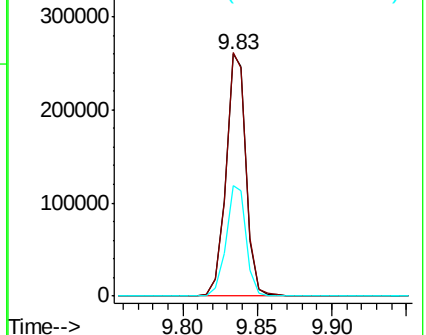




#42
 2,4,6-Tribromophenol
 Concen: 95.411 ng
 RT: 10.63 min Scan# 1452
 Delta R.T. -0.01 min
 Lab File: BF121154.D
 Acq: 31 Jul 2020 13:22




Instrument :
 BNA_F
 ClientSampleId :
 TP-7


Tot Ion:330 Resp: 258782
 Ion Ratio Lower Upper
 330 100
 332 95.9 76.1 114.1
 141 29.7 24.1 36.1

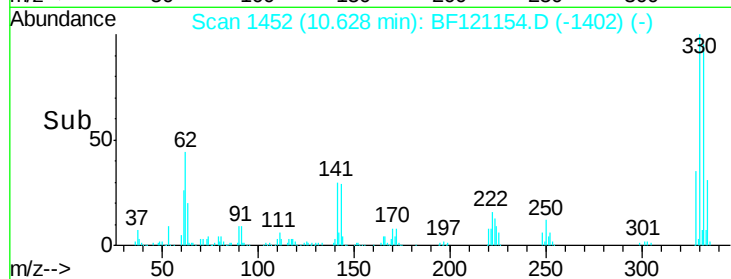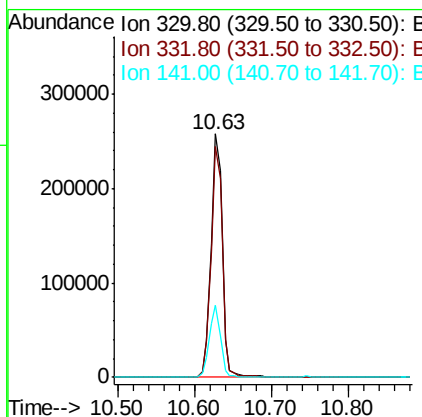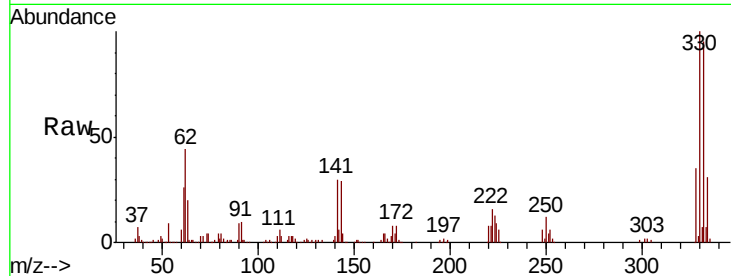

#45
 2-Fluorobiphenyl
 Concen: 62.660 ng
 RT: 9.16 min Scan# 1202
 Delta R.T. -0.01 min
 Lab File: BF121154.D
 Acq: 31 Jul 2020 13:22

Tgt Ion:172 Resp: 1039915
 Ion Ratio Lower Upper
 172 100
 171 35.2 29.0 43.4
 170 24.2 19.6 29.4

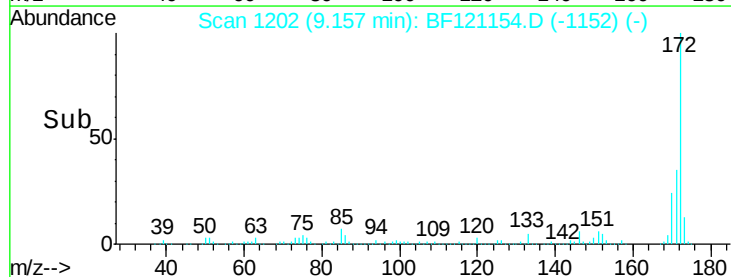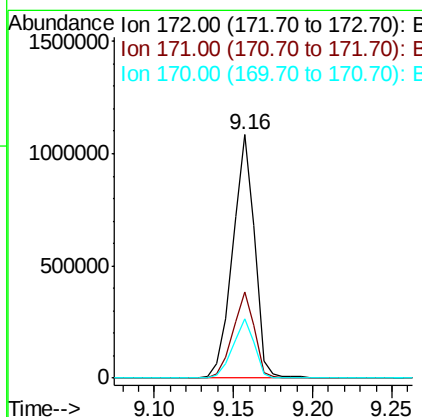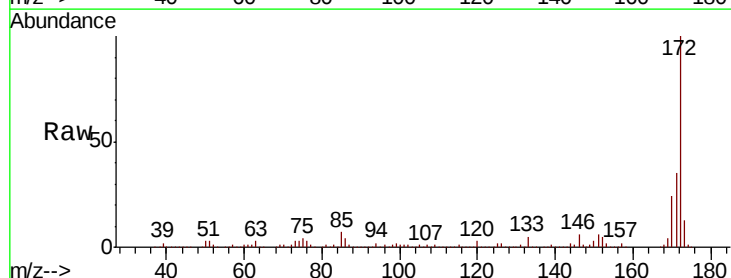


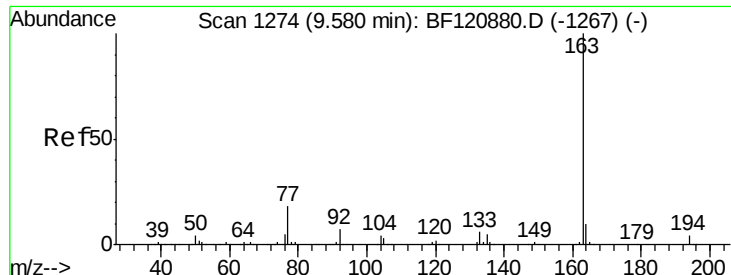




#50
Dimethylphthalate
Concen: 5.777 ng
RT: 9.55 min Scan# 1269
Delta R.T. -0.02 min
Lab File: BF121154.D
Acq: 31 Jul 2020 13:22

Instrument :
BNA_F
ClientSampleId :
TP-7

Tot Ion:163 Resp: 103267
Ion Ratio Lower Upper
163 100
194 3.7 3.0 4.4
164 10.0 8.4 12.6

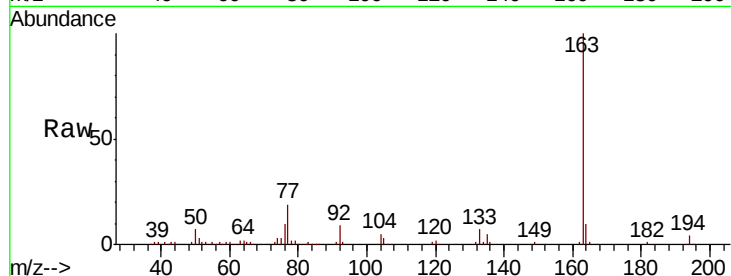


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

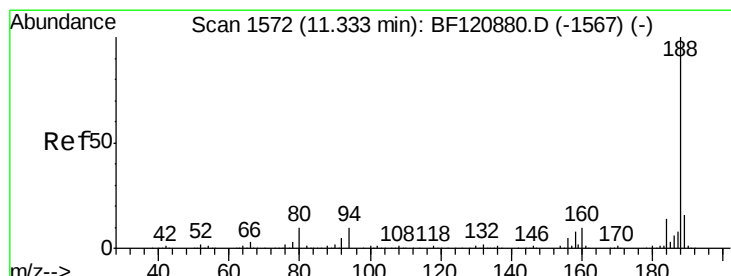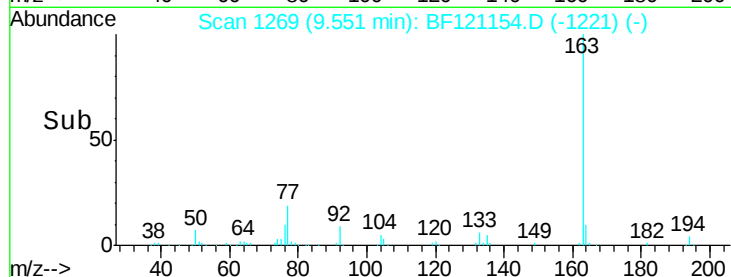
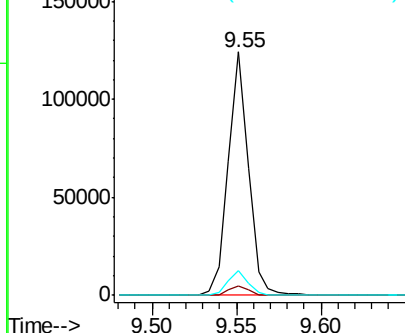



#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.32 min Scan# 1570
Delta R.T. 0.00 min
Lab File: BF121154.D
Acq: 31 Jul 2020 13:22

Tgt Ion:188 Resp: 464471
Ion Ratio Lower Upper
188 100
94 10.1 8.0 12.0
80 10.2 8.3 12.5

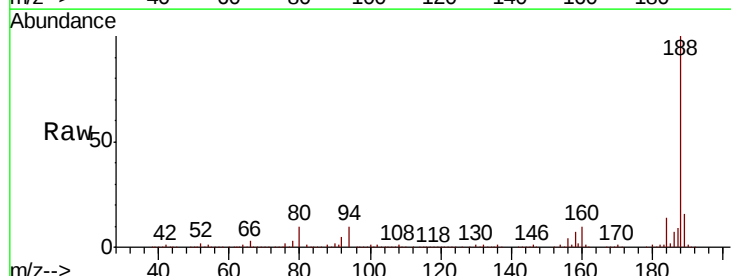

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

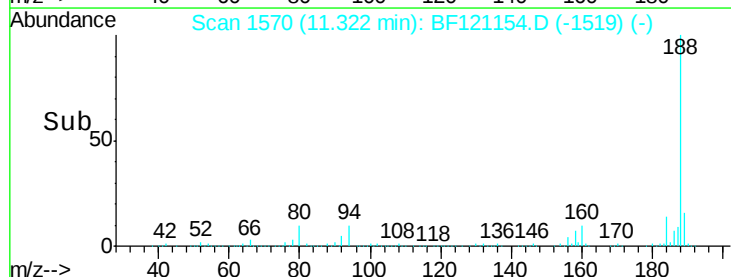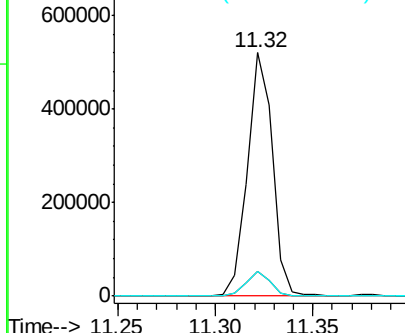

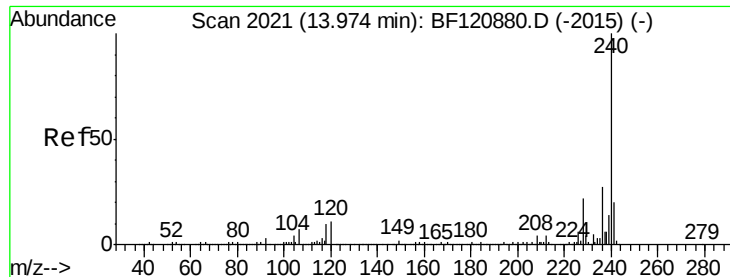

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.96 min Scan# 2019

Delta R.T. 0.00 min

Lab File: BF121154.D

Acq: 31 Jul 2020 13:22

Instrument :

BNA_F

ClientSampleId :

TP-7


Tot Ion:240 Resp: 319283

Ion Ratio Lower Upper

240 100

120 12.1 9.3 13.9




236 26.2 21.1 31.7

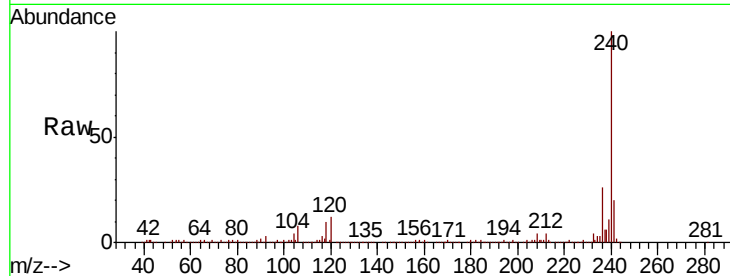

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

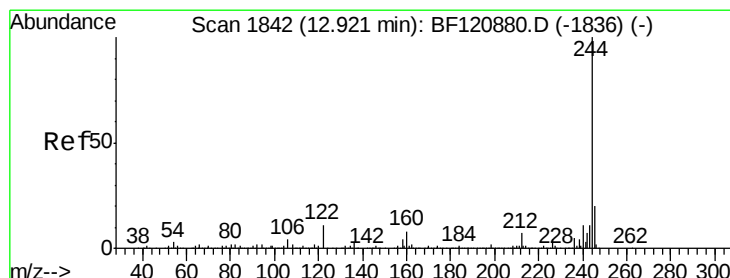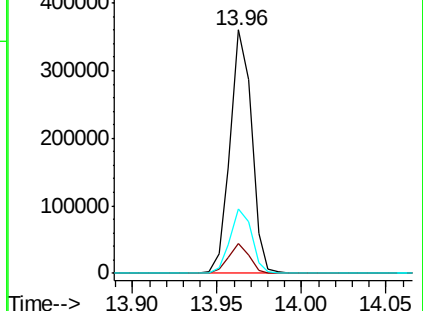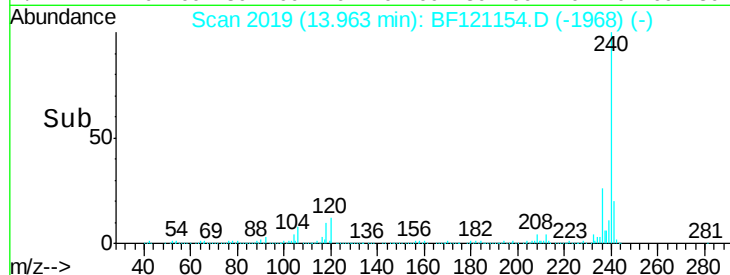

#79

Terphenyl-d14

Concen: 67.734 ng

RT: 12.92 min Scan# 1841

Delta R.T. 0.01 min

Lab File: BF121154.D

Acq: 31 Jul 2020 13:22


Tgt Ion:244 Resp: 994865

Ion Ratio Lower Upper

244 100

212 6.7 5.7 8.5



122 9.9 8.3 12.5

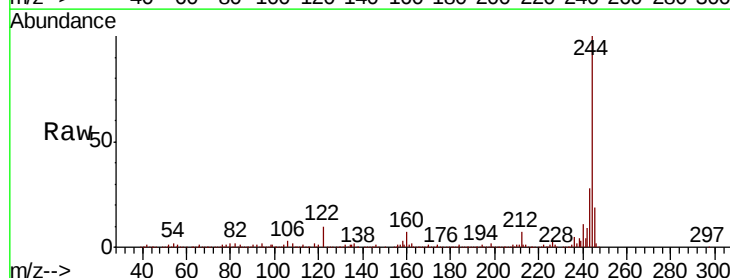


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

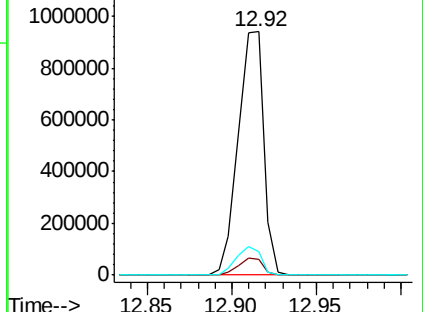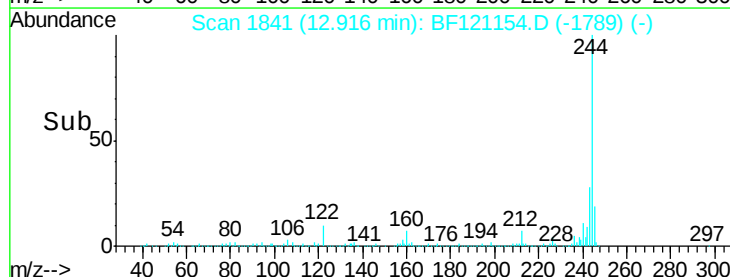

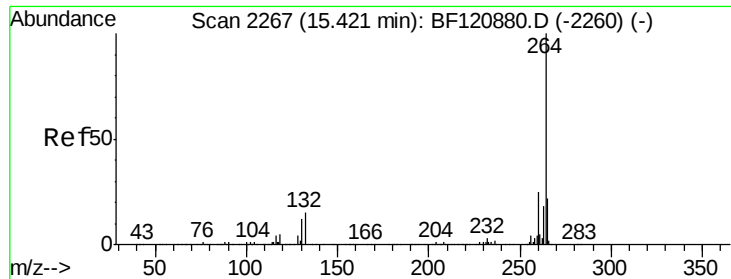

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.42 min Scan# 2266
Delta R.T. 0.01 min
Lab File: BF121154.D
Acq: 31 Jul 2020 13:22

Instrument :
BNA_F
ClientSampleId :
TP-7

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.9	19.9	29.9
265	21.8	17.8	26.8

