

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
 Data File : BF124888.D
 Acq On : 31 Jul 2021 12:25
 Operator : JU/CG
 Sample : PB138079BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB138079BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124888.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	512	515	520	rBB	2523	3224	1.12%	0.204%
2	5.493	574	579	581	rBB	190442	207237	72.21%	13.090%
3	6.487	743	748	751	rBV	187907	211950	73.85%	13.388%
4	6.857	808	811	813	rBB	46551	39258	13.68%	2.480%
5	7.422	901	907	909	rBB	123736	138311	48.19%	8.736%
6	8.139	1024	1029	1032	rBB	53017	54033	18.83%	3.413%
7	9.216	1206	1212	1215	rBV	265146	261374	91.07%	16.509%
8	9.892	1322	1327	1330	rBB	77720	63955	22.28%	4.040%
9	10.680	1456	1461	1464	rBV	177035	160250	55.84%	10.122%
10	11.374	1575	1579	1583	rBB	73481	66662	23.23%	4.211%
11	12.968	1845	1850	1853	rBV	319408	286996	100.00%	18.128%
12	14.015	2024	2028	2031	rBB	66615	50790	17.70%	3.208%
13	15.480	2273	2277	2281	rBB2	33334	39148	13.64%	2.473%




Sum of corrected areas: 1583188

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124888.D
Acq On : 31 Jul 2021 12:25
Operator : JU/CG
Sample : PB138079BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138079BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

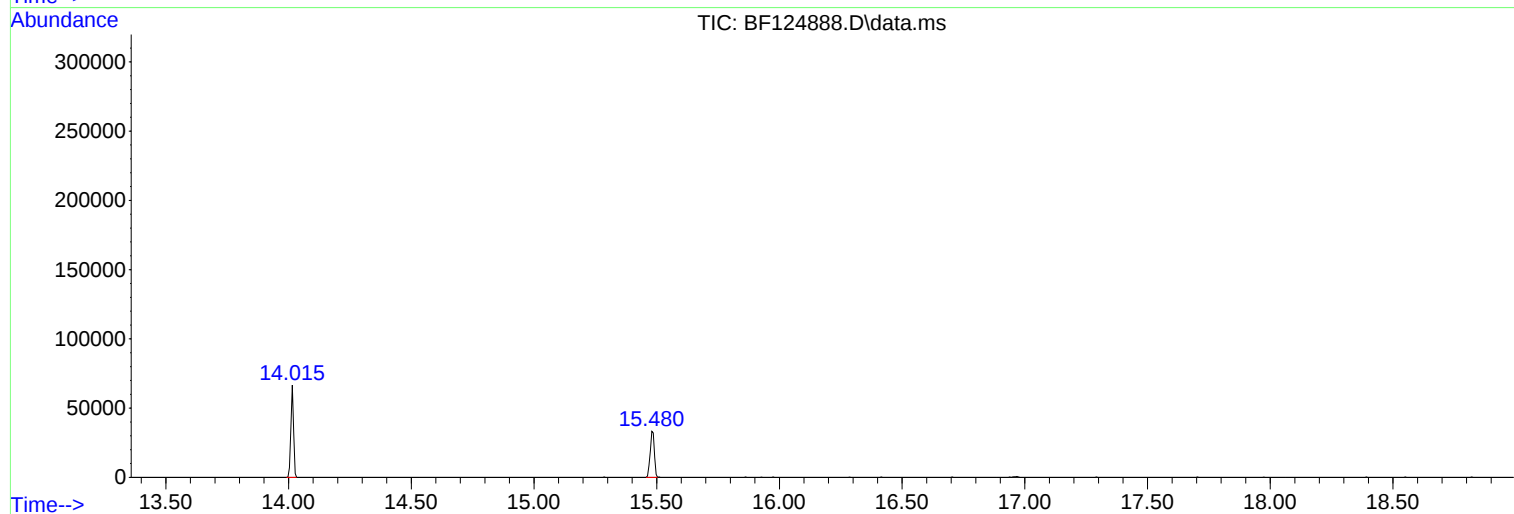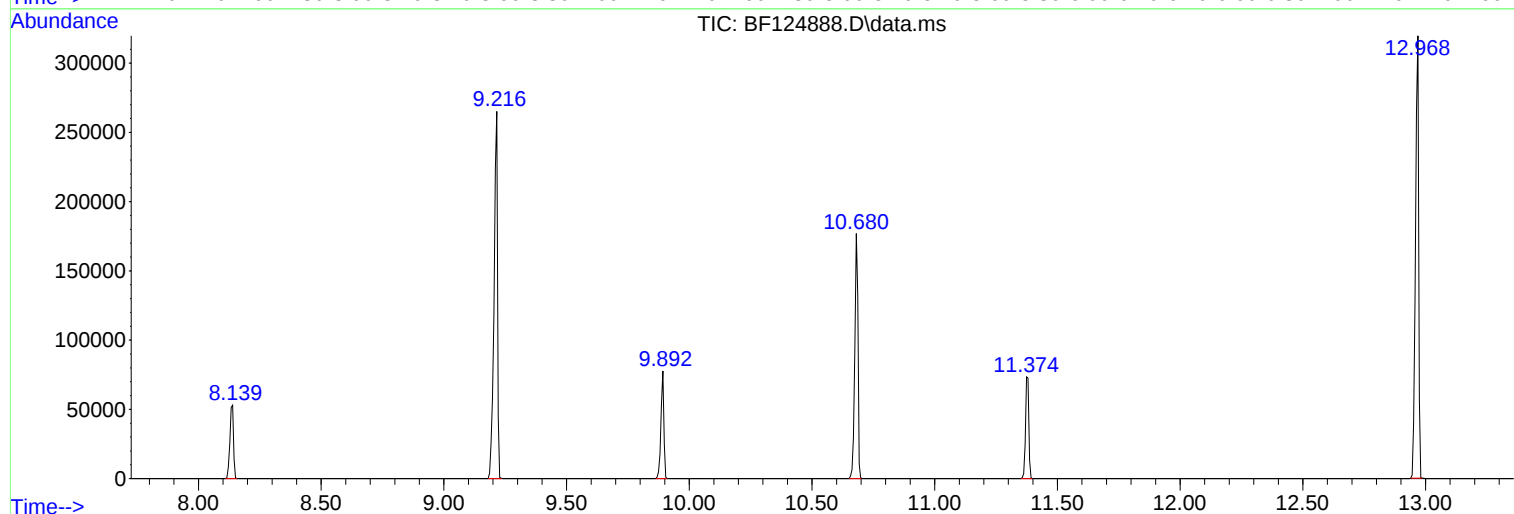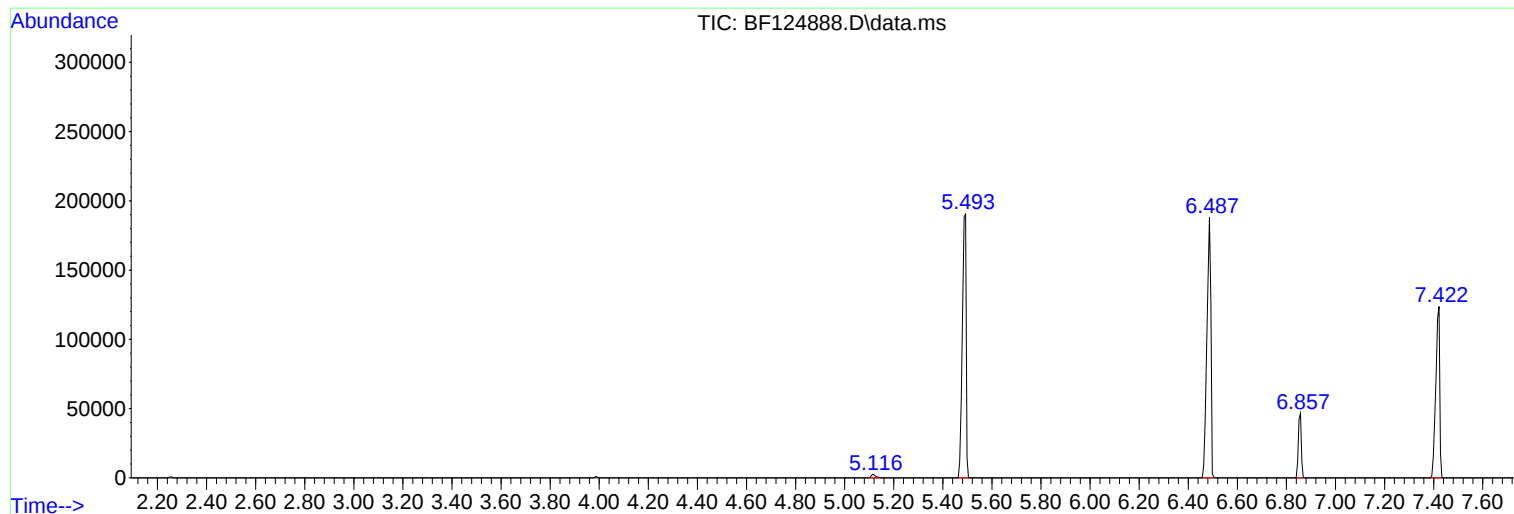

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124888.D
Acq On : 31 Jul 2021 12:25
Operator : JU/CG
Sample : PB138079BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138079BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124888.D
Acq On : 31 Jul 2021 12:25
Operator : JU/CG
Sample : PB138079BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB138079BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------