

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
 Data File : BF124890.D
 Acq On : 31 Jul 2021 13:47
 Operator : JU/CG
 Sample : M3223-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-09

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124890.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.110	3	4	7	rVB	3631	2911	2.30%	0.342%
2	5.469	571	575	578	rBV	107558	95927	75.88%	11.278%
3	6.481	743	747	750	rBV	106976	100335	79.37%	11.796%
4	6.857	808	811	813	rBB	30806	25741	20.36%	3.026%
5	7.416	902	906	909	rBB	77719	64483	51.01%	7.581%
6	8.139	1025	1029	1032	rBB	40926	35012	27.70%	4.116%
7	9.210	1207	1211	1214	rBV	154074	120613	95.41%	14.180%
8	9.892	1323	1327	1329	rBB	50872	40672	32.17%	4.782%
9	10.680	1457	1461	1464	rBB	79836	66441	52.56%	7.811%
10	11.375	1576	1579	1583	rBB	51565	41072	32.49%	4.829%
11	11.892	1664	1667	1670	rBB	3211	3440	2.72%	0.404%
12	12.398	1750	1753	1756	rBV	1039	1551	1.23%	0.182%
13	12.680	1797	1801	1807	rBB	10204	13181	10.43%	1.550%
14	12.927	1839	1843	1845	rBV2	3905	5517	4.36%	0.649%
15	12.963	1845	1849	1852	rVB	153711	126414	100.00%	14.862%
16	13.698	1969	1974	1979	rBB2	5940	9708	7.68%	1.141%
17	13.874	2002	2004	2007	rBV	1756	1811	1.43%	0.213%
18	14.016	2025	2028	2031	rBB	32569	27089	21.43%	3.185%
19	14.292	2071	2075	2080	rBB	6980	9963	7.88%	1.171%
20	14.780	2154	2158	2160	rBV2	3163	3032	2.40%	0.356%
21	14.810	2160	2163	2167	rVB2	6990	9507	7.52%	1.118%
22	15.116	2211	2215	2218	rBB	3593	3350	2.65%	0.394%
23	15.374	2254	2259	2264	rBB2	5340	8334	6.59%	0.980%
24	15.480	2273	2277	2283	rBB2	19775	23363	18.48%	2.747%
25	15.927	2350	2353	2357	rBB	1942	2317	1.83%	0.272%
26	16.015	2364	2368	2373	rBB2	3182	5237	4.14%	0.616%
27	16.757	2489	2494	2500	rBB3	1642	3569	2.82%	0.420%




Sum of corrected areas: 850590

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124890.D
Acq On : 31 Jul 2021 13:47
Operator : JU/CG
Sample : M3223-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BACKFILL-ASHCROFT-REAR-09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

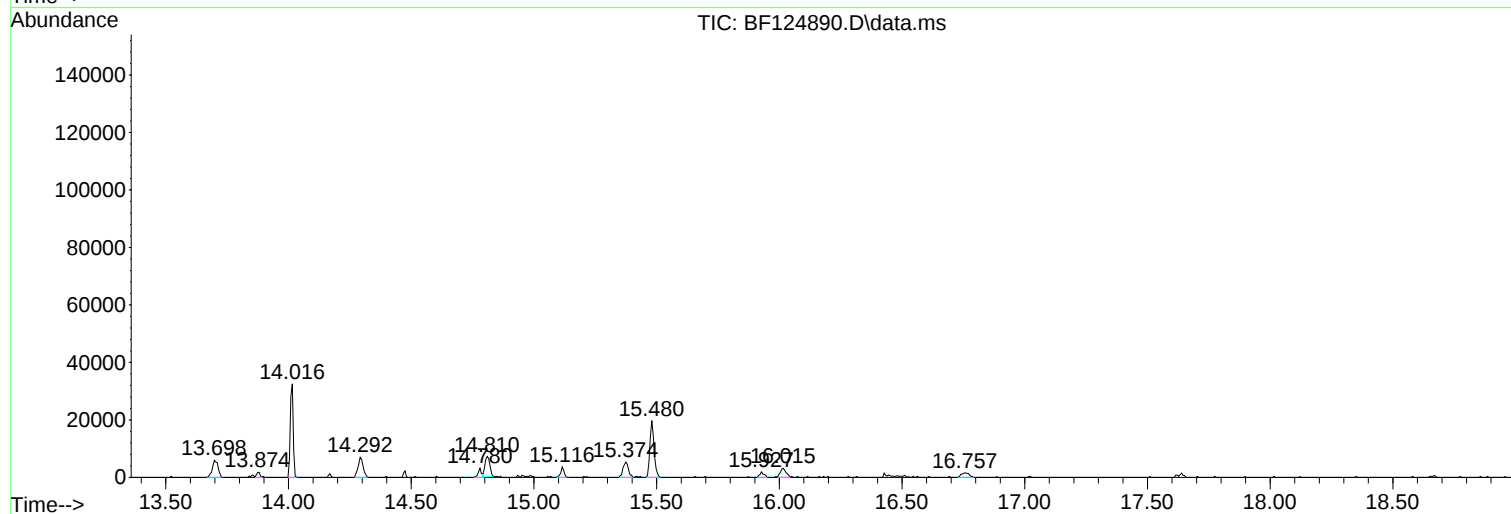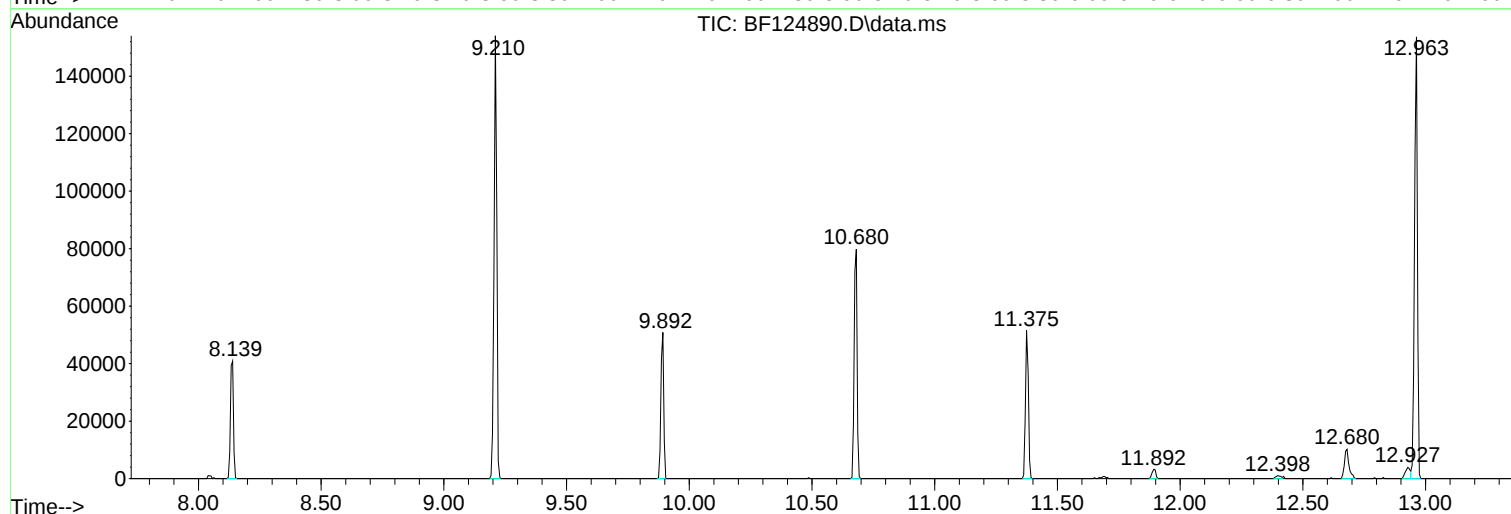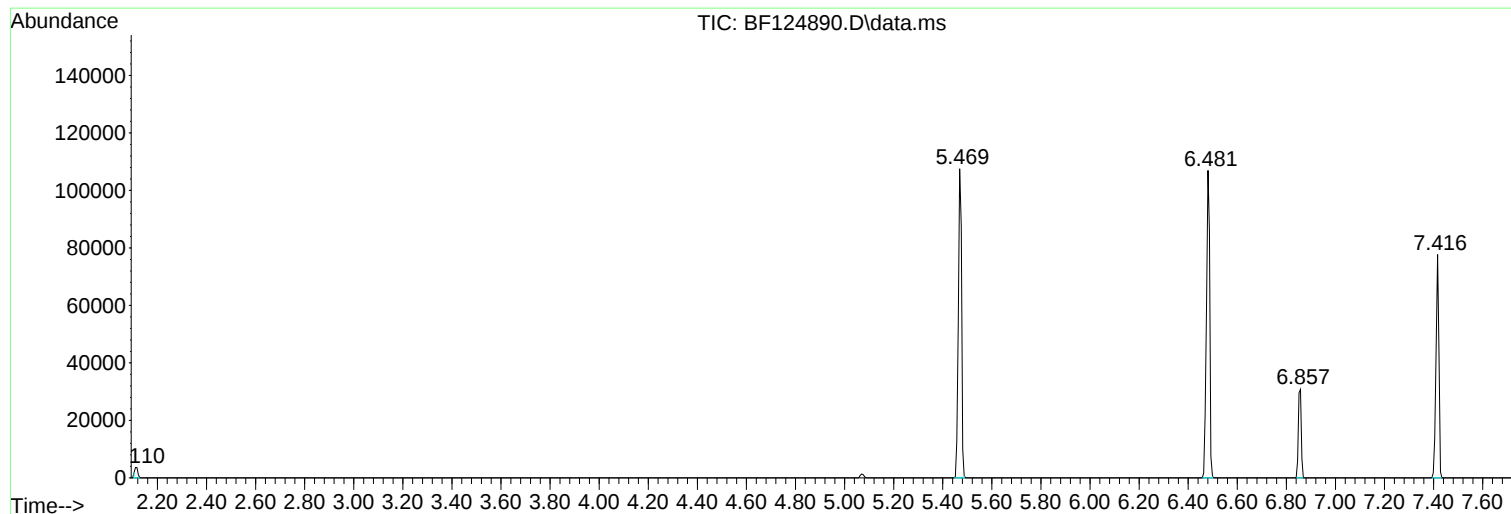

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124890.D
Acq On : 31 Jul 2021 13:47
Operator : JU/CG
Sample : M3223-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BACKFILL-ASHCROFT-REAR-09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124890.D
Acq On : 31 Jul 2021 13:47
Operator : JU/CG
Sample : M3223-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BACKFILL-ASHCROFT-REAR-09

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------