

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
 Data File : BF124891.D
 Acq On : 31 Jul 2021 14:19
 Operator : JU/CG
 Sample : M3223-03
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BACKFILL-ASHCROFT-REAR-10

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124891.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.140	5	9	13	rBB	8196	8780	4.38%	0.782%
2	5.087	508	510	514	rBB	1818	2142	1.07%	0.191%
3	5.475	572	576	579	rBV	157423	161099	80.30%	14.347%
4	6.487	743	748	751	rBB	159611	160882	80.20%	14.328%
5	6.857	808	811	813	rBB	34753	28470	14.19%	2.535%
6	7.422	902	907	909	rBB	110873	105626	52.65%	9.407%
7	8.033	1009	1011	1016	rBB	4214	4243	2.12%	0.378%
8	8.139	1025	1029	1032	rBB	43595	38204	19.04%	3.402%
9	9.216	1207	1212	1214	rBV	213144	200613	100.00%	17.866%
10	9.892	1323	1327	1330	rBB	53891	43498	21.68%	3.874%
11	10.680	1457	1461	1464	rBB	141398	107463	53.57%	9.570%
12	11.374	1576	1579	1582	rBV	54255	42039	20.96%	3.744%
13	12.963	1845	1849	1852	rBV	211124	174123	86.80%	15.507%
14	14.015	2024	2028	2031	rBB	27606	23487	11.71%	2.092%
15	15.480	2273	2277	2281	rBB	20406	22204	11.07%	1.977%




Sum of corrected areas: 1122873

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124891.D
Acq On : 31 Jul 2021 14:19
Operator : JU/CG
Sample : M3223-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BACKFILL-ASHCROFT-REAR-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

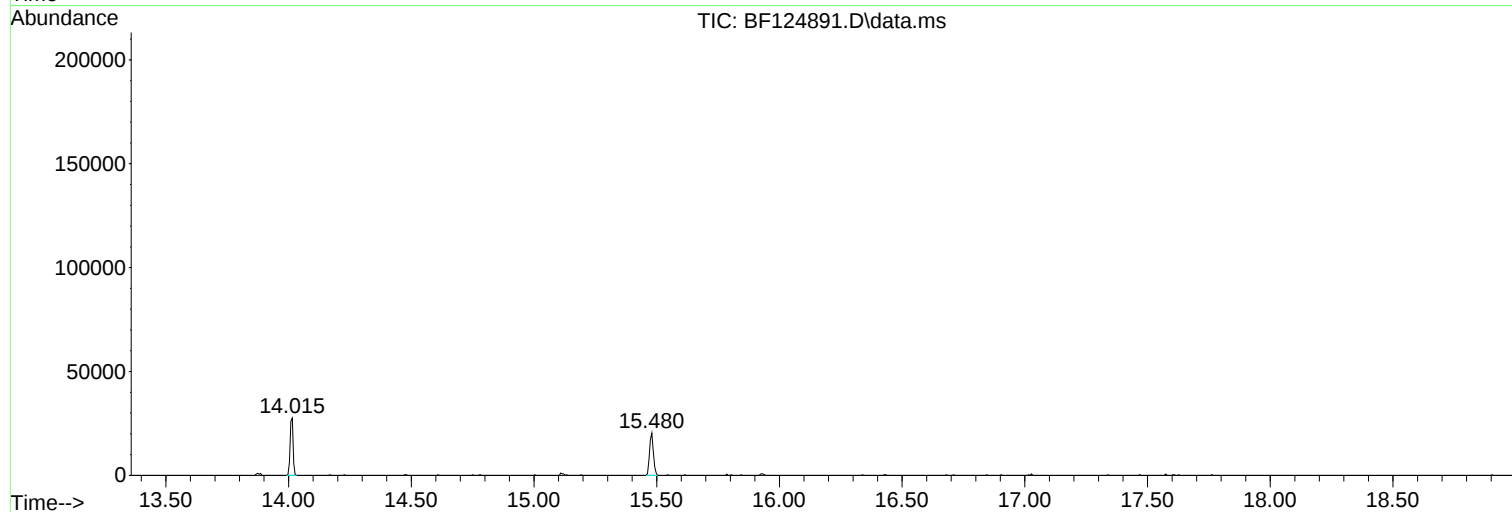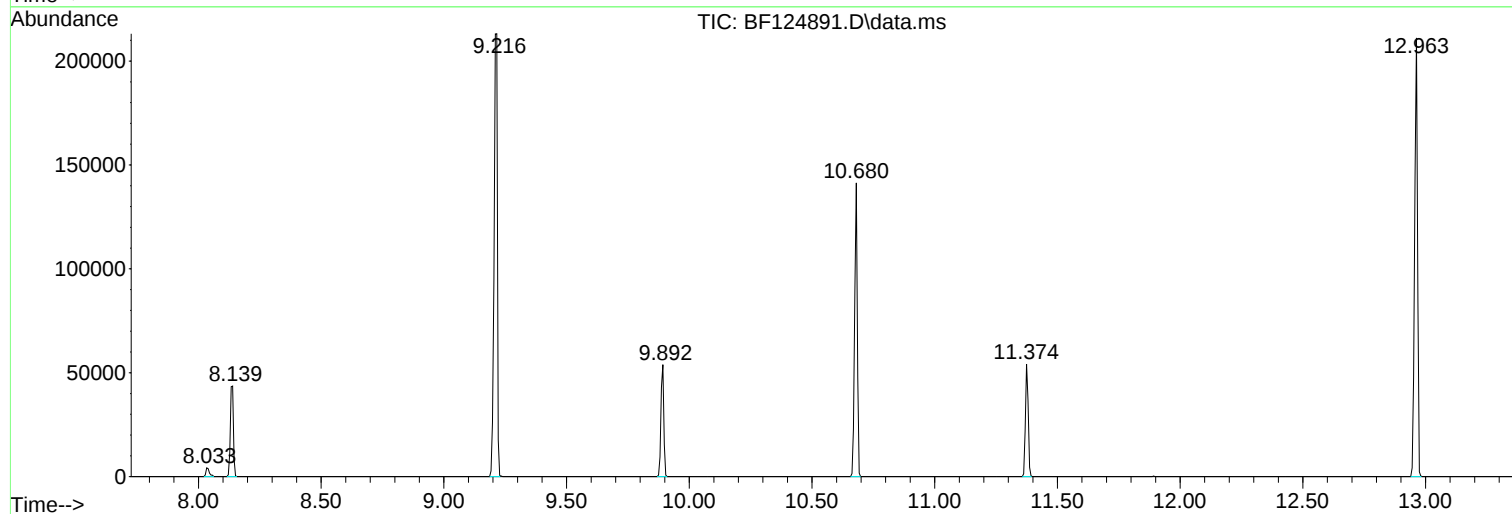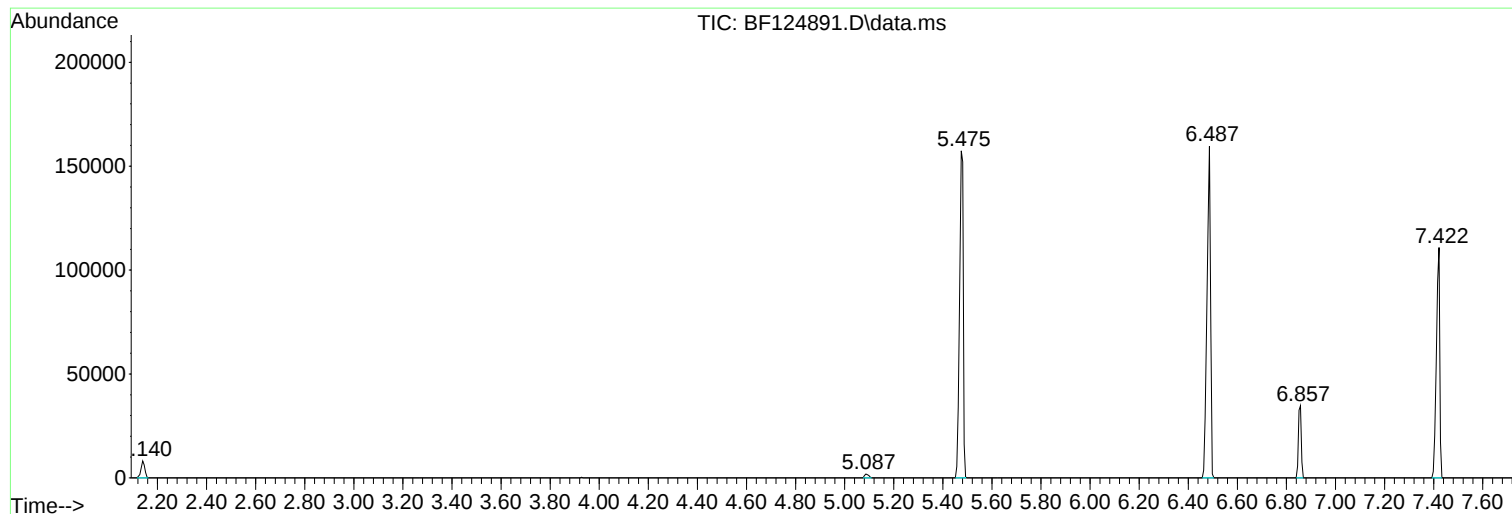

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124891.D
Acq On : 31 Jul 2021 14:19
Operator : JU/CG
Sample : M3223-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BACKFILL-ASHCROFT-REAR-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
Data File : BF124891.D
Acq On : 31 Jul 2021 14:19
Operator : JU/CG
Sample : M3223-03
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BACKFILL-ASHCROFT-REAR-10

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------