


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
 Data File : BF124886.D
 Acq On : 31 Jul 2021 10:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 02 11:15:51 2021

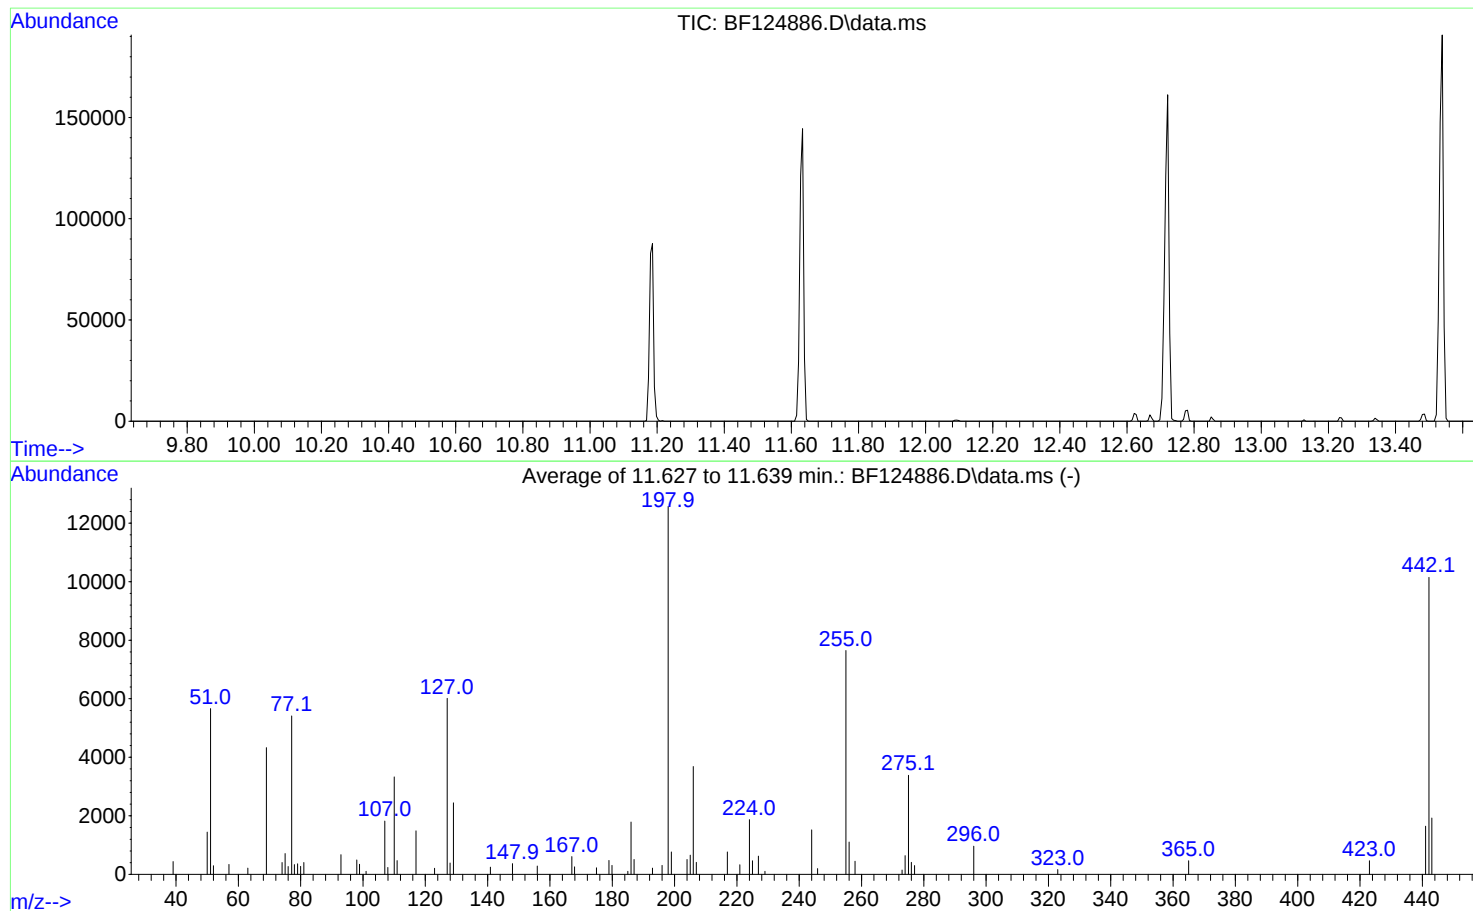




AutoFind: Scans 1622, 1623, 1624; Background Corrected with Scan 1617

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	5663	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	34.5	4331	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.8	6012	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	12568	PASS
199	198	5	9	6.1	763	PASS
275	198	10	60	26.9	3386	PASS
365	198	1	100	3.7	465	PASS
441	198	0.01	100	13.1	1644	PASS
442	442	50	100	100.0	10146	PASS
443	442	15	24	19.0	1923	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\  
Data File : BF124886.D  
Acq On    : 31 Jul 2021  10:46  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 02 03:18:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 02 02:31:45 2021
Response via : Initial Calibration

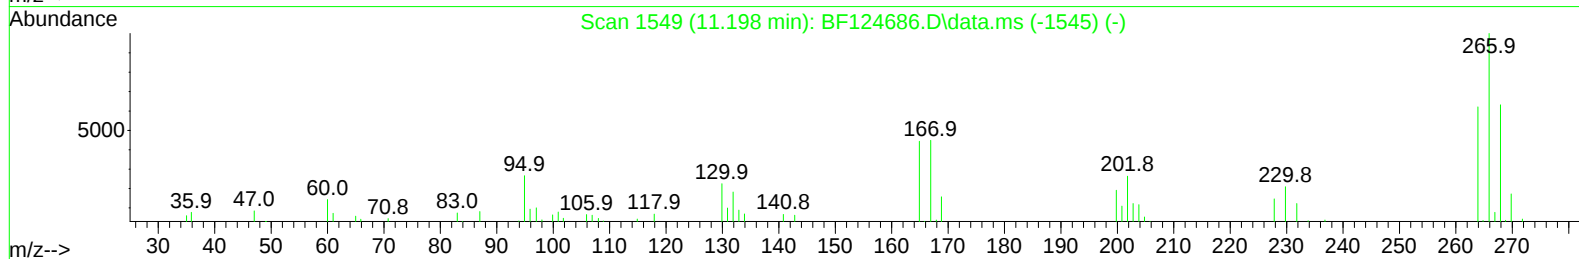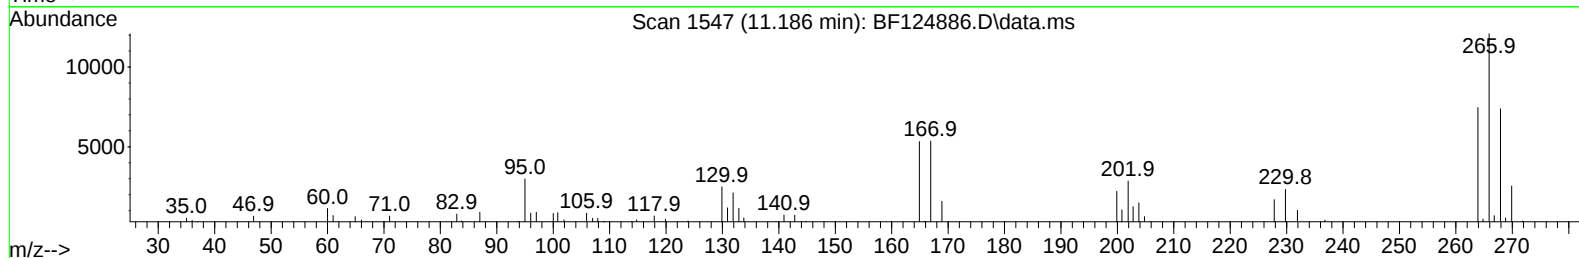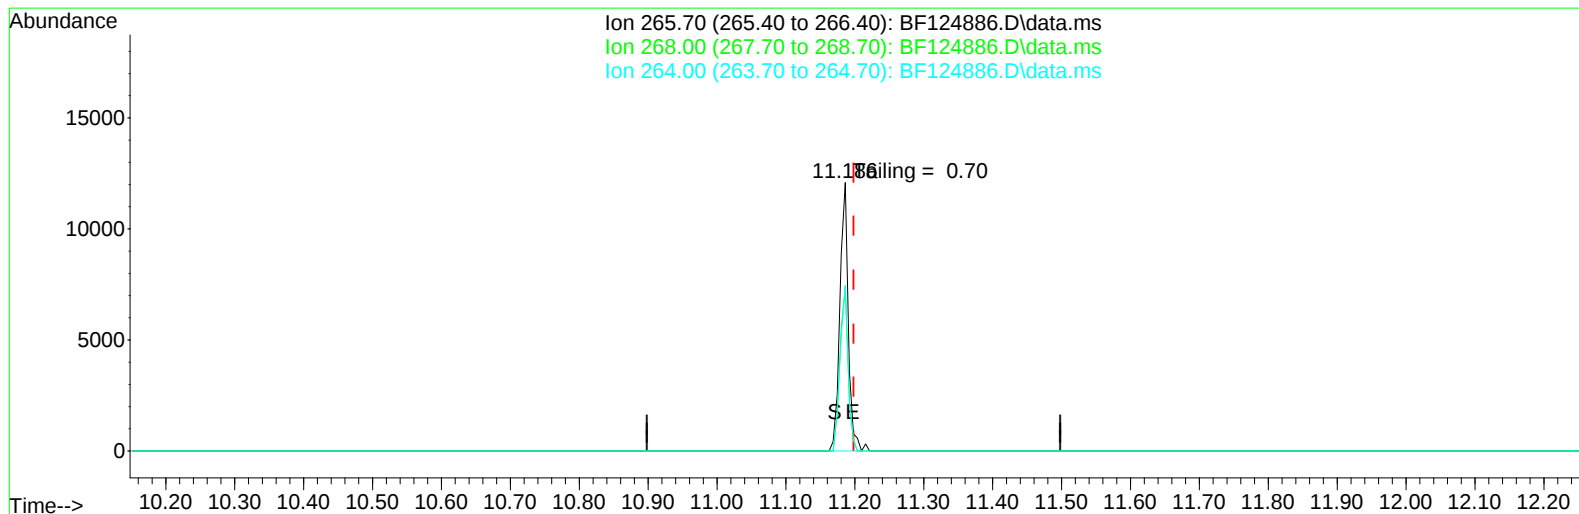

TIC: BF124886.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.012) 0.00 ng




response **10308**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	61.11
264.00	69.90	61.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073121\
 Data File : BF124886.D
 Acq On : 31 Jul 2021 10:46
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Aug 02 03:18:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 02 02:31:45 2021
 Response via : Initial Calibration

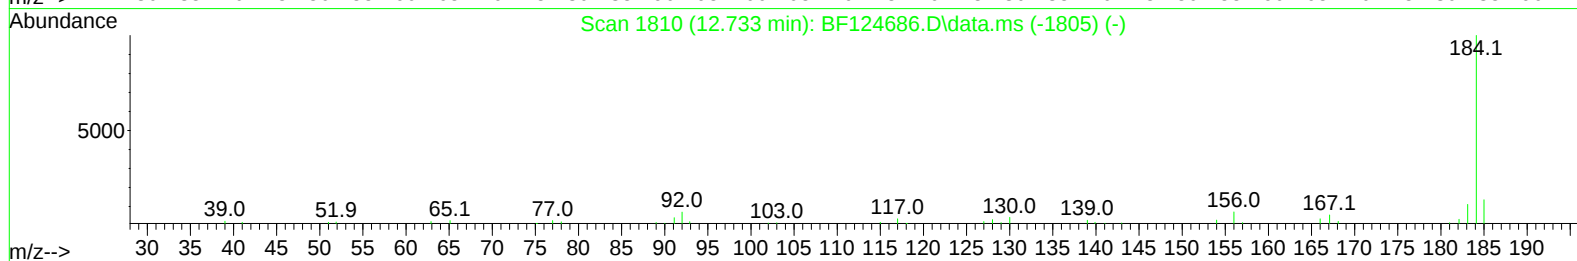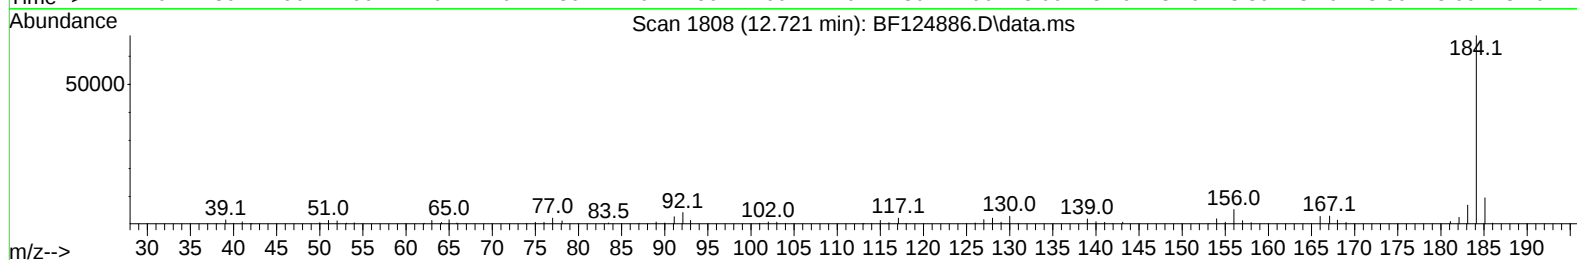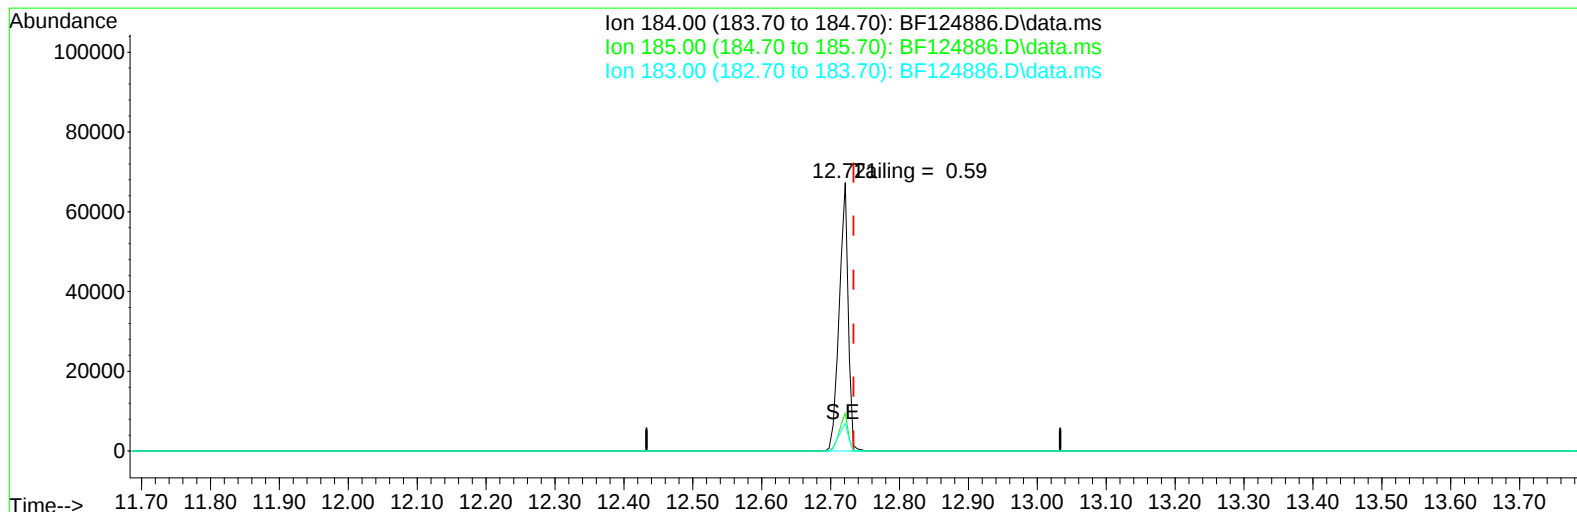

TIC: BF124886.D\data.ms

(77) Benzidine

12.721min (-0.012) 0.00 ng

response 60691

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.17
183.00	10.10	10.29
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/31/2021	BNA_F	<u>BF124886.D</u>
Compound Name	Response	Retention Time
DDT	31052	13.53
DDD	492	13.23
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
492	31544	1.56

Instrument :
BNA_F
ClientSampleId :
DFTPP