
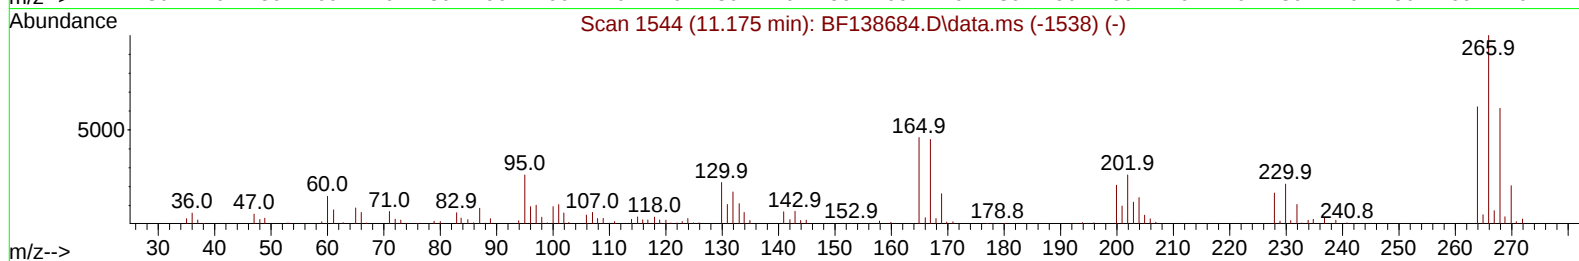
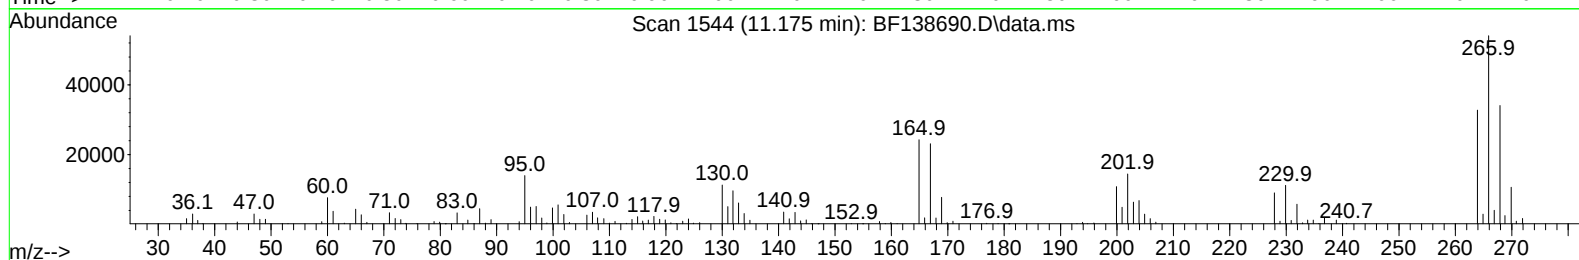


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073124\
Data File : BF138690.D
Acq On : 31 Jul 2024 08:31
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 11:03:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

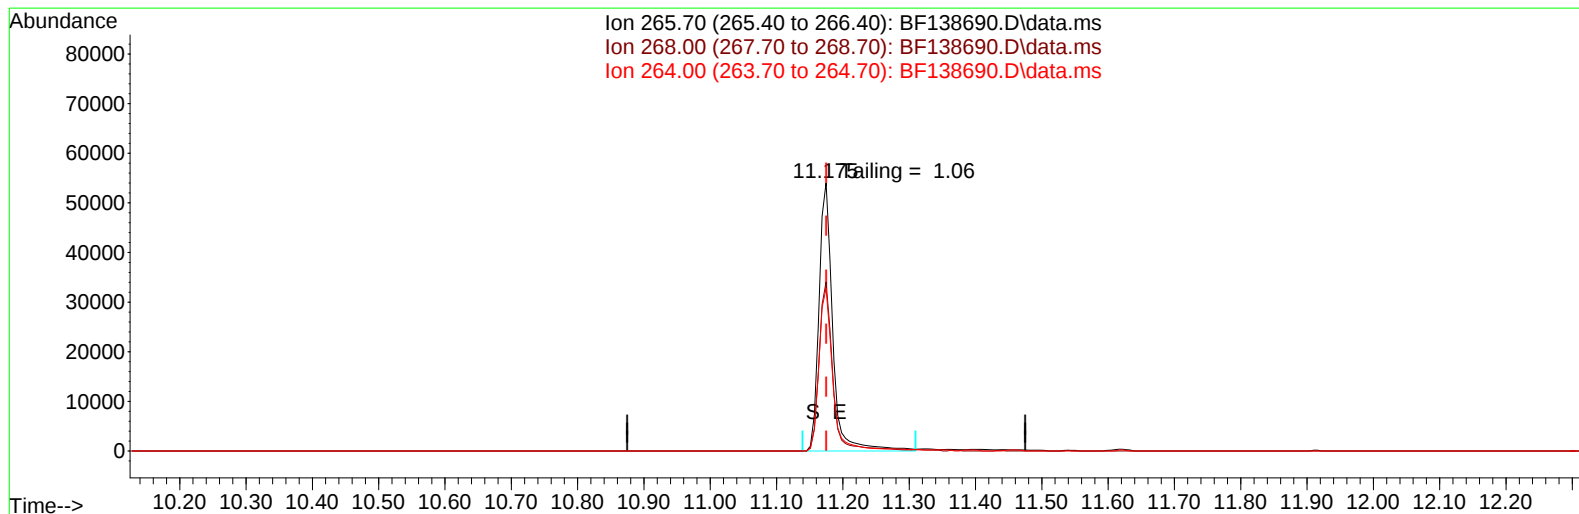

TIC: BF138690.D\data.ms




(70) Pentachlorophenol (C)

11.175min (-0.000) 281854.08 ng

response 78111

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.97
264.00	62.20	60.56
0.00	0.00	0.00

Quant Time: Jul 31 11:03:11 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

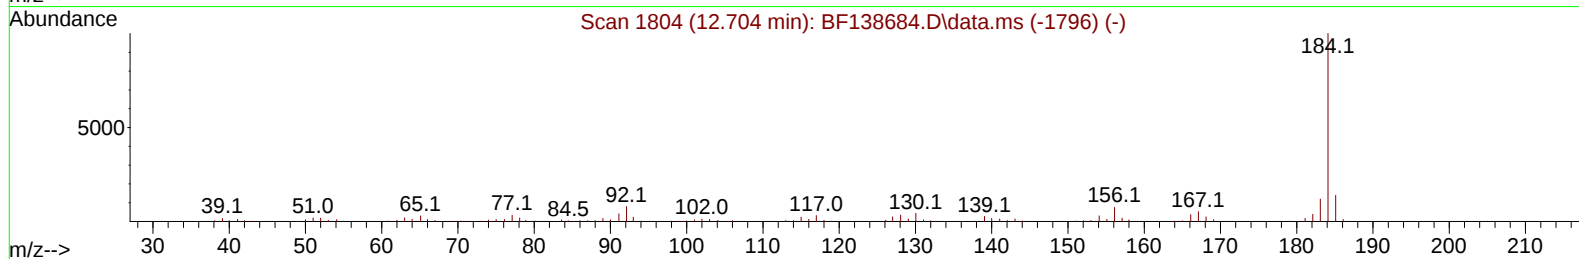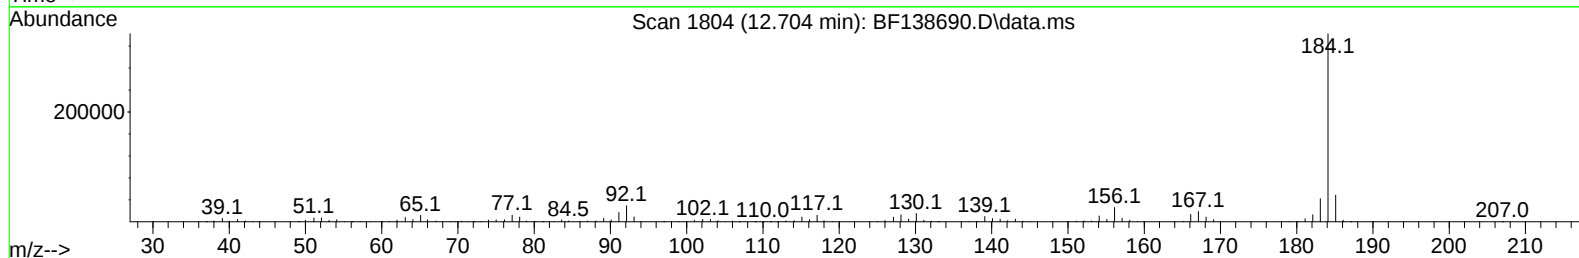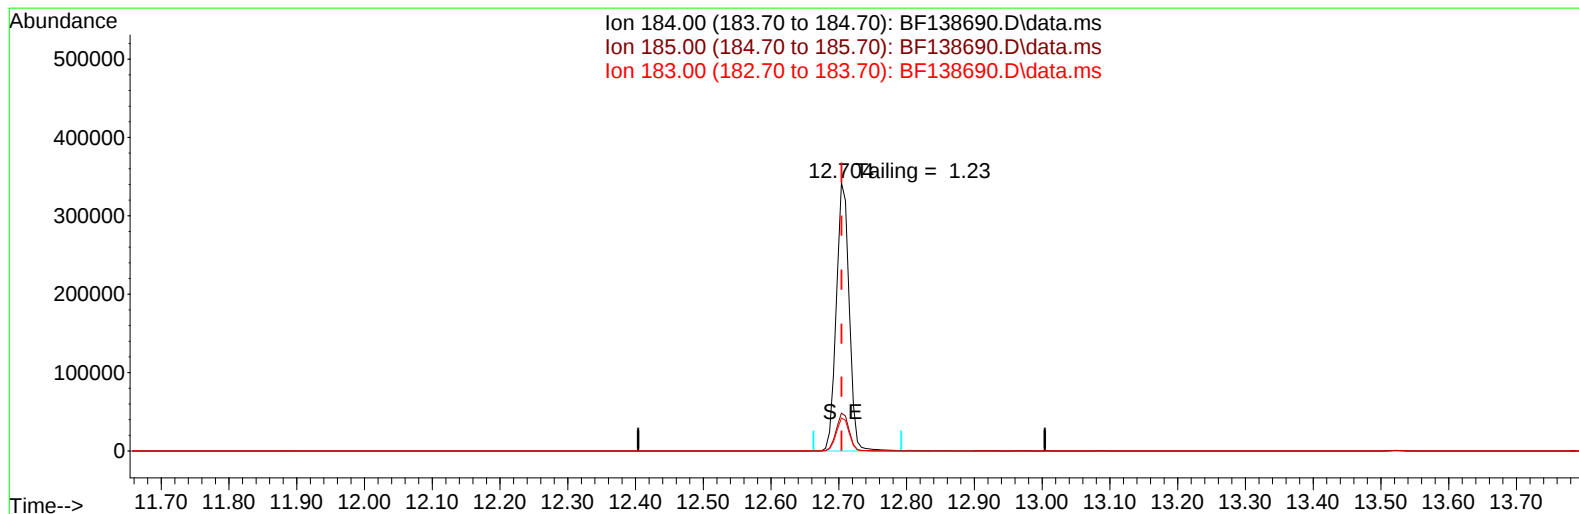

TIC: BF138690.D\data.ms

(77) Benzidine

12.704min (-0.000) 80204.41 ng

response **454649**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.18
183.00	12.00	12.30
0.00	0.00	0.00