
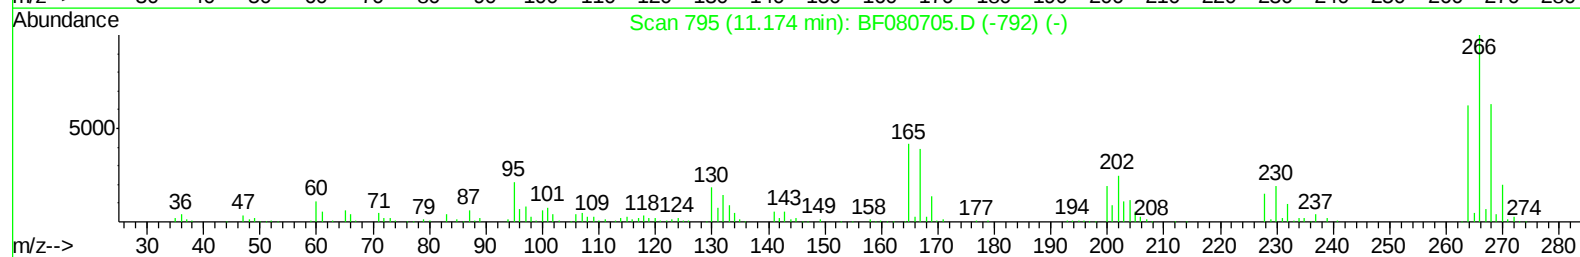
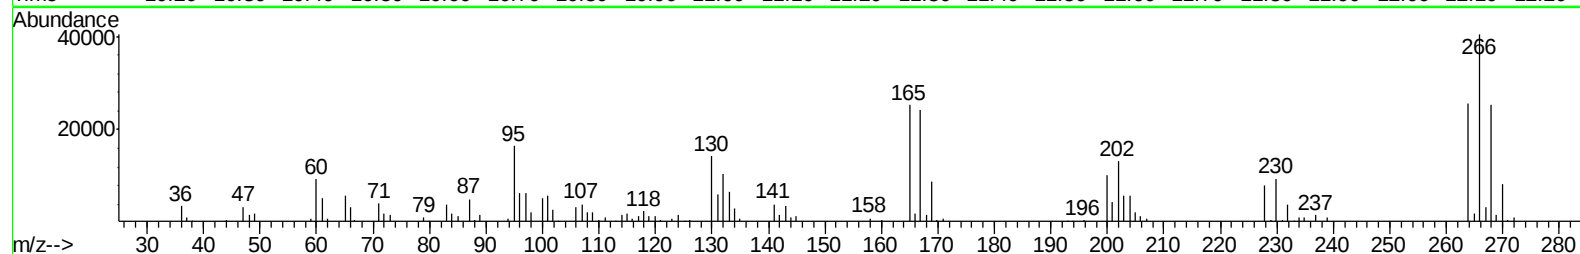


Data Path : Z:\HPCHEM1\BNA F\Data\BF080115\
Data File : BF080781.D
Acq On : 1 Aug 2015 15:23
Operator : TP/UM
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 04:02:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 31 01:45:22 2015
Response via : Initial Calibration

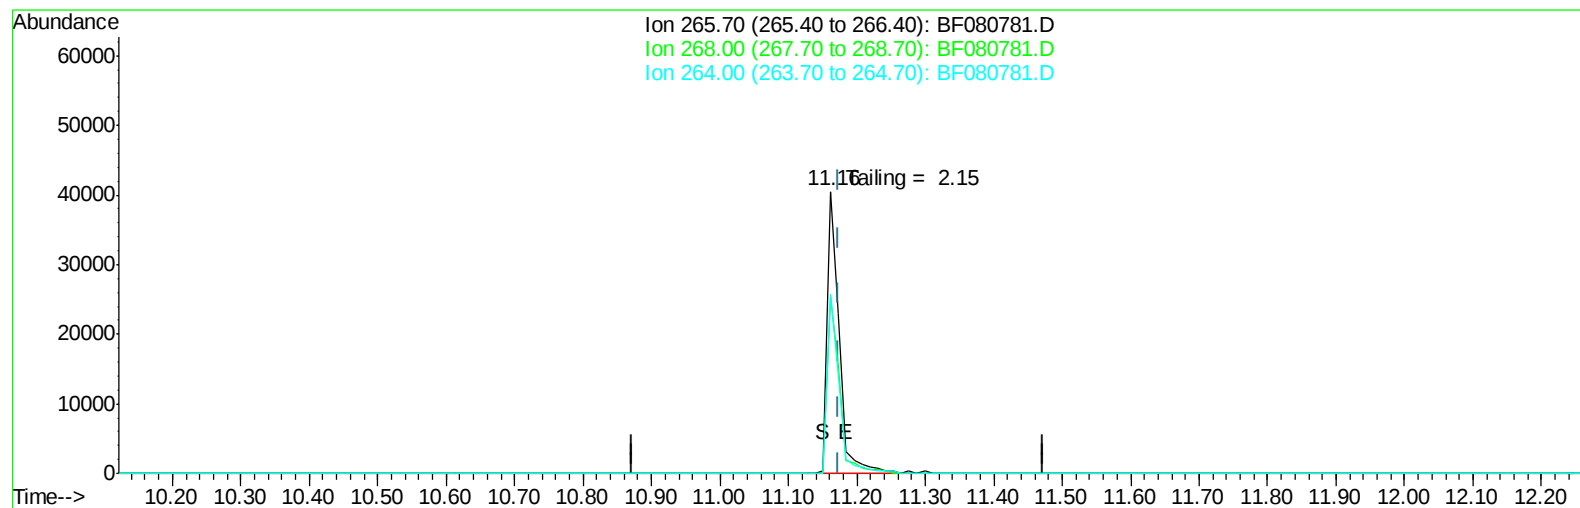

TIC: BF080781.D

(69) Pentachlorophenol (C)




11.162min (-0.011) 25820.35ng

response 49605

Ion	Exp%	Act%
265.70	100	100
268.00	63.10	62.82
264.00	62.50	63.63
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF080115\
Data File : BF080781.D
Acq On : 1 Aug 2015 15:23
Operator : TP/UM
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 04:02:04 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF073015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 31 01:45:22 2015
Response via : Initial Calibration

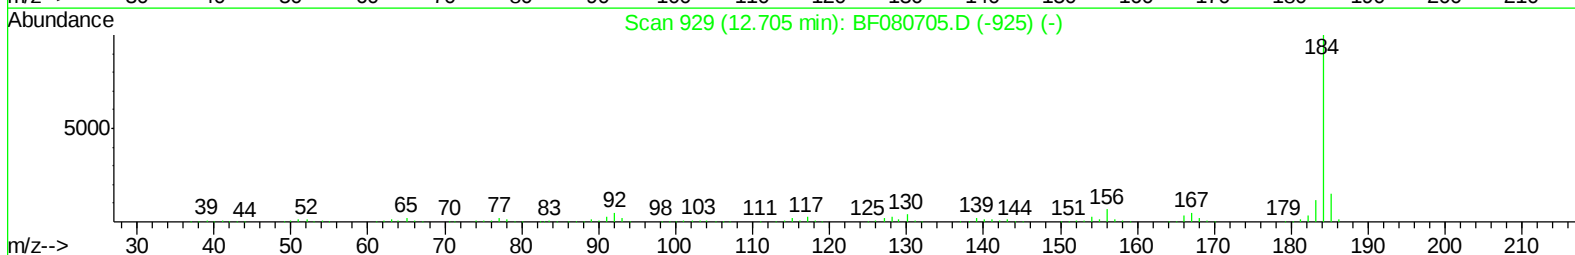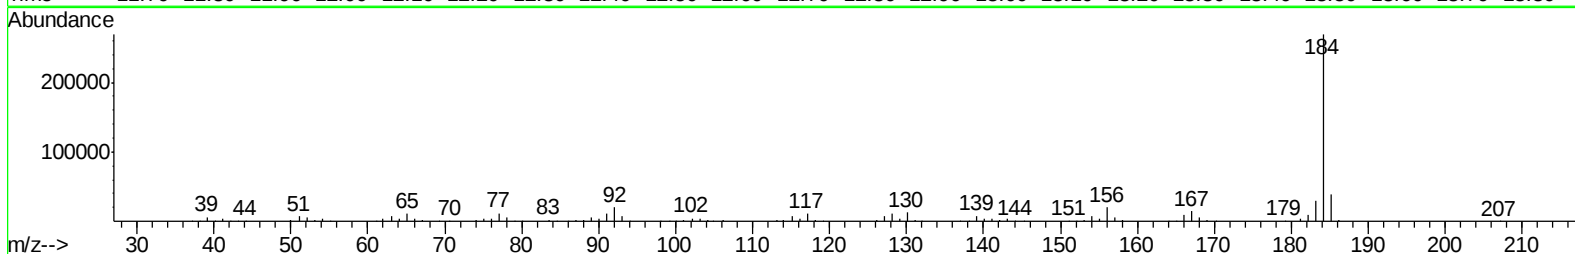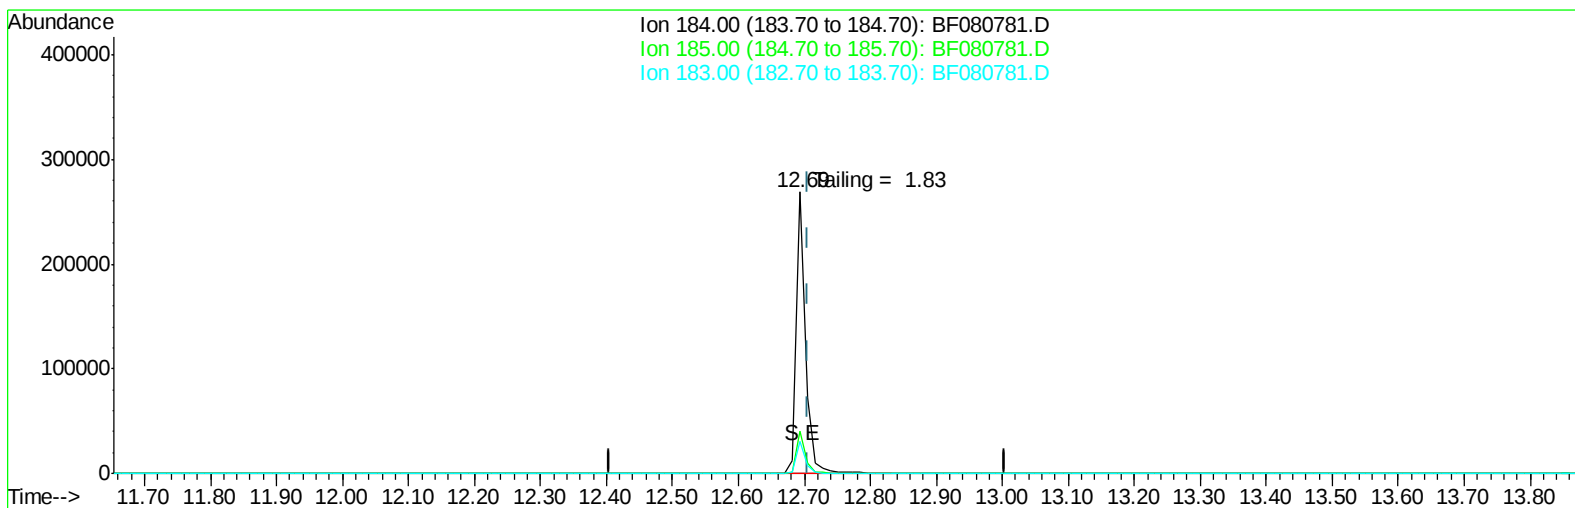

TIC: BF080781.D

(76) Benzidine

12.694min (-0.011) 0.00ng

response 257989

Ion	Exp%	Act%
184.00	100	100
185.00	15.00	14.84
183.00	11.40	11.26
0.00	0.00	0.00