


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080115\
 Data File : BF080761.D
 Acq On : 1 Aug 2015 5:07
 Operator : TP/UM
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 03 14:00:36 2015

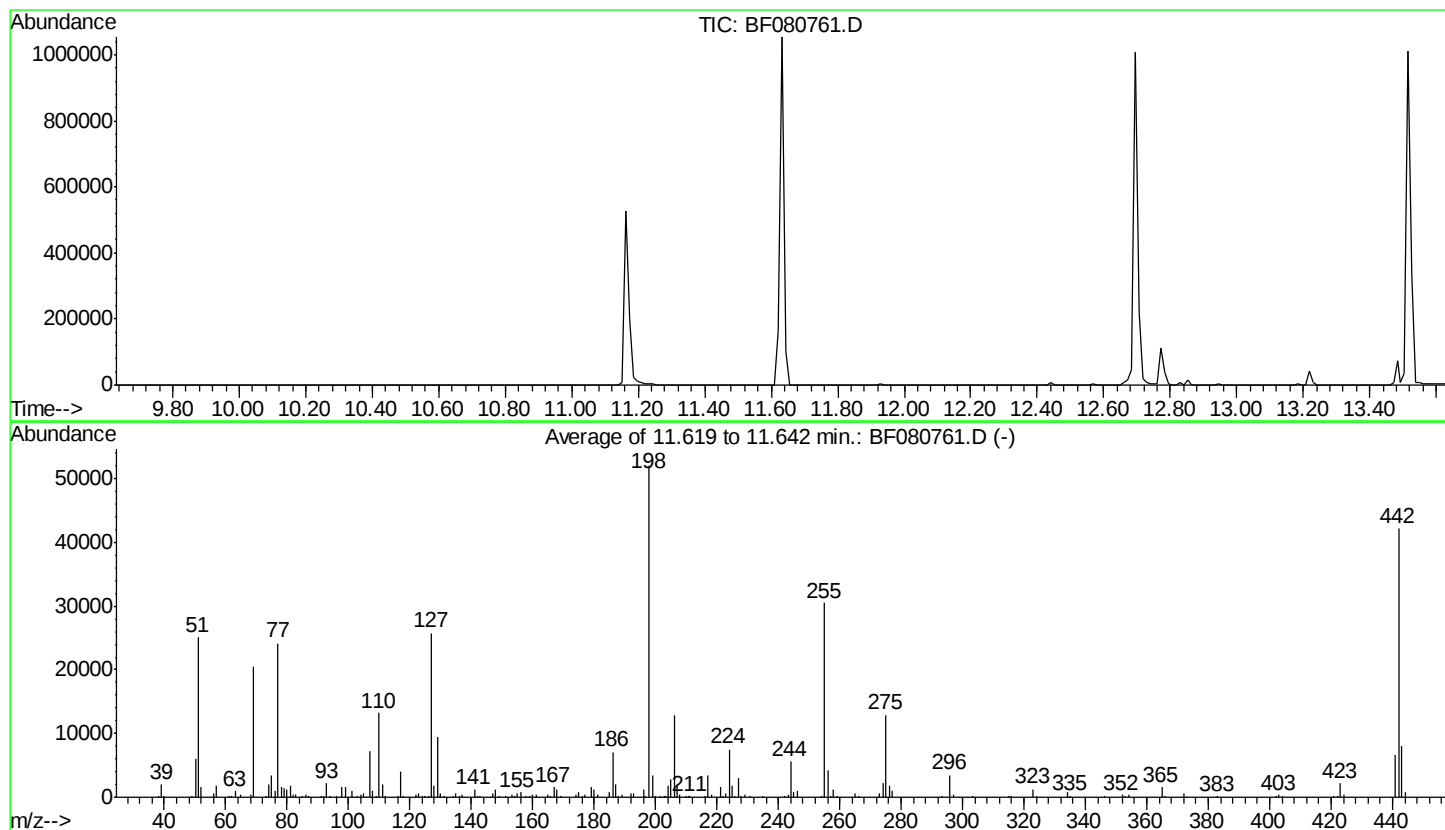

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.2	25073	PASS
68	69	0.00	2	1.7	341	PASS
69	198	0.00	100	39.3	20481	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	25820	PASS
197	198	0.00	2	0.6	304	PASS
198	198	100	100	100.0	52052	PASS
199	198	5	9	6.8	3519	PASS
275	198	10	60	24.9	12951	PASS
365	198	1	100	3.1	1590	PASS
441	442	0.01	24	15.8	6679	PASS
442	198	50	100	81.0	42147	PASS
443	442	15	24	18.9	7963	PASS