
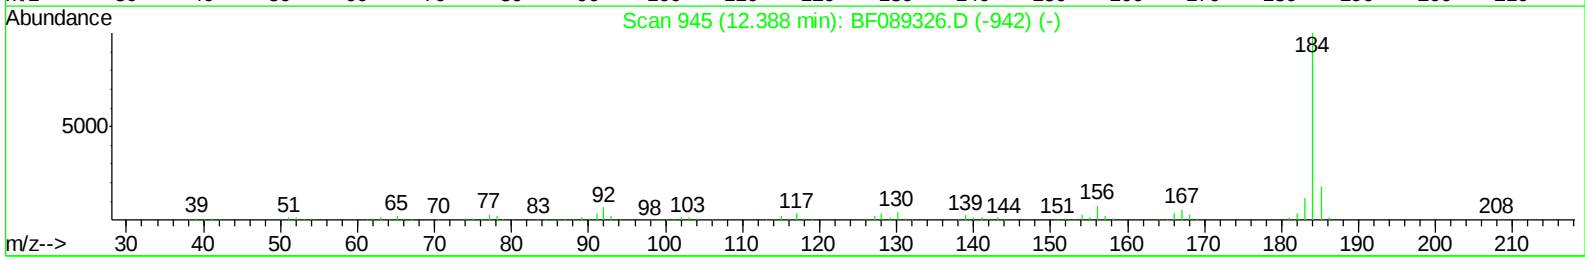
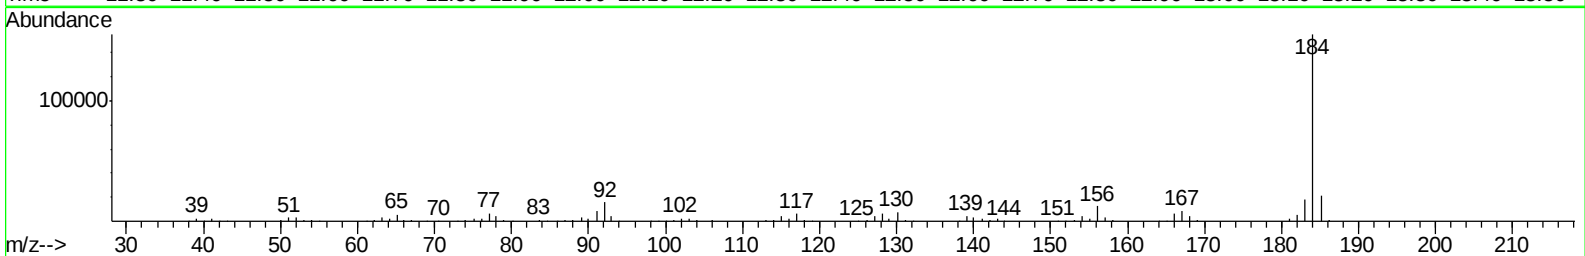


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080116\
Data File : BF089504.D
Acq On : 1 Aug 2016 11:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 05:37:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 02:21:57 2016
Response via : Initial Calibration

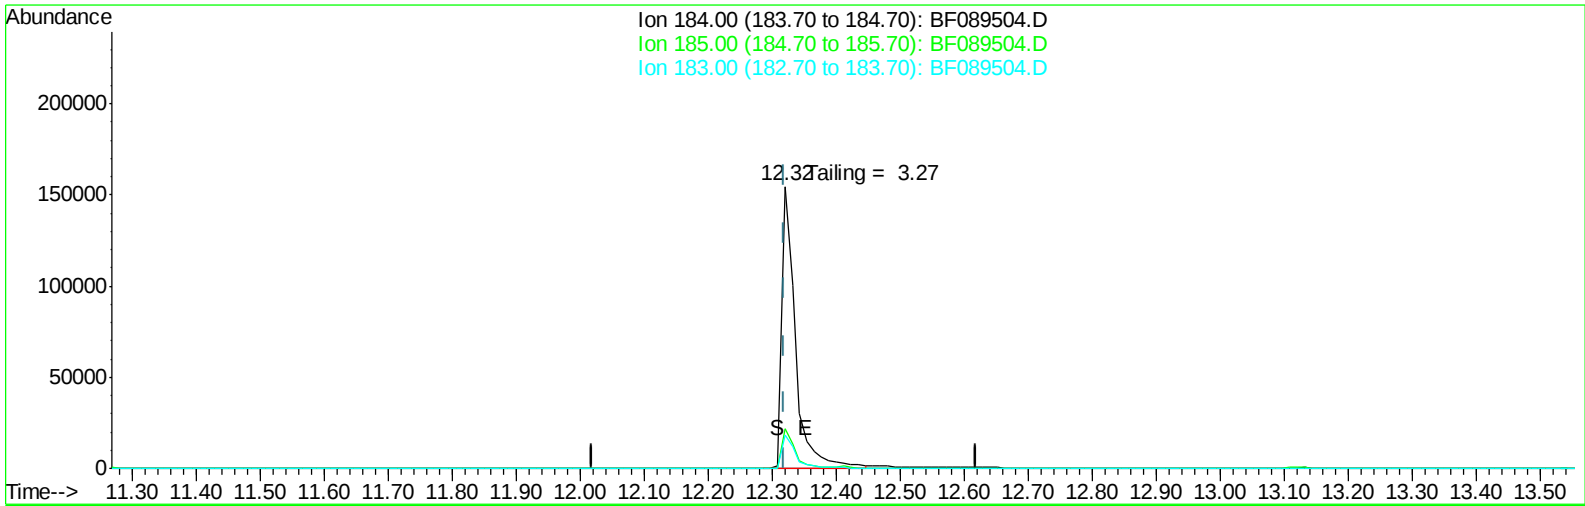

TIC: BF089504.D

(76) Benzidine




12.319min (+0.000) 0.00ng

response 236379

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	14.19
183.00	12.20	11.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080116\
Data File : BF089504.D
Acq On : 1 Aug 2016 11:41
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 05:37:21 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 02:21:57 2016
Response via : Initial Calibration

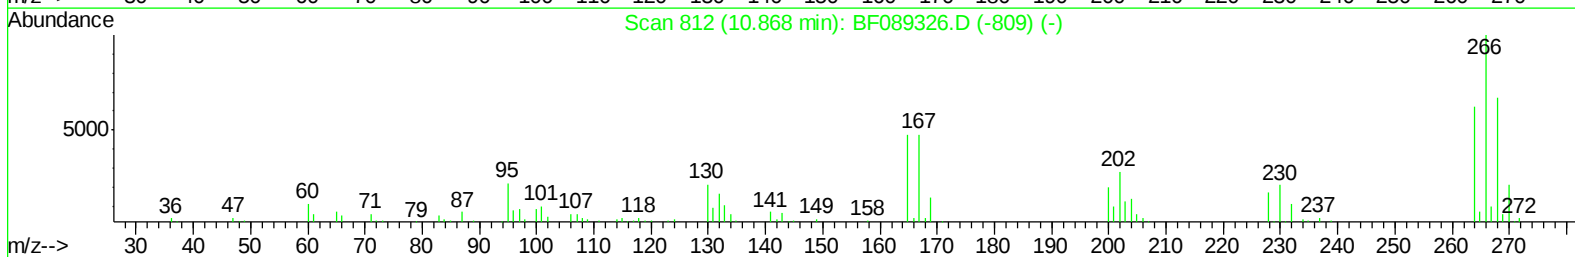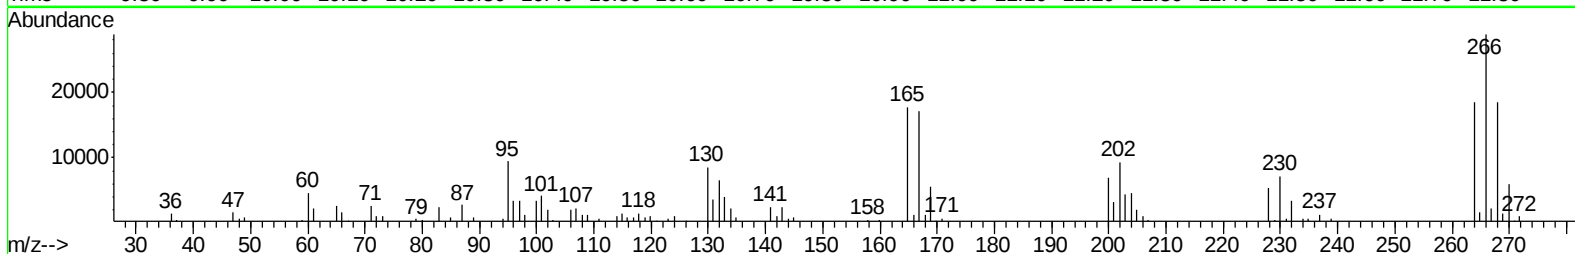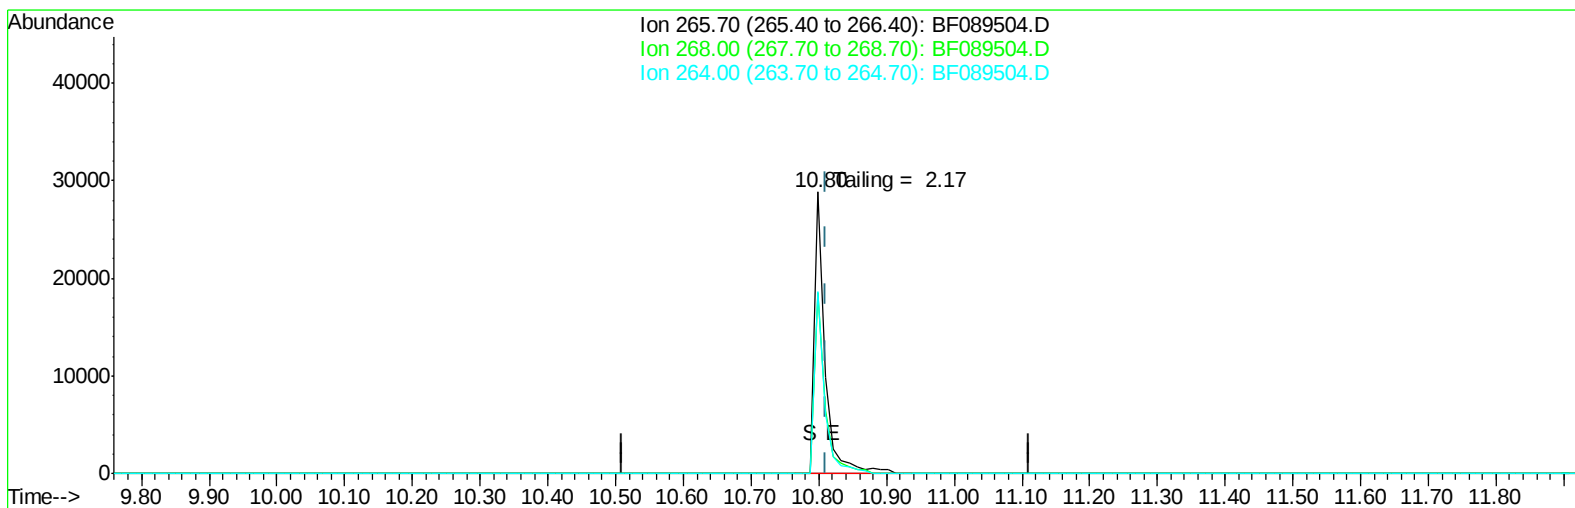

TIC: BF089504.D

(69) Pentachlorophenol (C)

10.799min (-0.011) 0.00ng

response 31456

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	64.09
264.00	62.70	64.34
0.00	0.00	0.00