

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080116\
 Data File : BF089518.D
 Acq On : 1 Aug 2016 18:56
 Operator : UM/SJ
 Sample : H4256-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MH-6

Quant Time: Aug 02 03:16:02 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Aug 02 02:21:57 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.48	152	39635	20.00	ng	0.00
21) Naphthalene-d8	7.76	136	163127	20.00	ng	-0.01
38) Acenaphthene-d10	9.51	164	74382	20.00	ng	-0.01
63) Phenanthrene-d10	10.98	188	124584	20.00	ng	0.00
75) Chrysene-d12	13.60	240	75361	20.00	ng	-0.01
86) Perylene-d12	14.93	264	78420	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.04	112	85710	34.53	ng	0.00
7) Phenol-d6	6.14	99	74613	22.74	ng	-0.01
23) Nitrobenzene-d5	7.05	82	234256	84.76	ng	-0.01
41) 2,4,6-Tribromophenol	10.30	330	53005	86.04	ng	-0.01
44) 2-Fluorobiphenyl	8.84	172	446615	88.12	ng	-0.01
78) Terphenyl-d14	12.56	244	229909	71.40	ng	-0.01
Target Compounds						
49) Dimethylphthalate	9.24	163	59653	10.54	ng	Qvalue 100
83) Bis(2-ethylhexyl)phthalate	13.61	149	15731	4.19	ng	# 94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080116\
Data File : BF089518.D
Acq On : 1 Aug 2016 18:56
Operator : UM/SJ
Sample : H4256-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MH-6

Quant Time: Aug 02 03:16:02 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Aug 02 02:21:57 2016
Response via : Initial Calibration

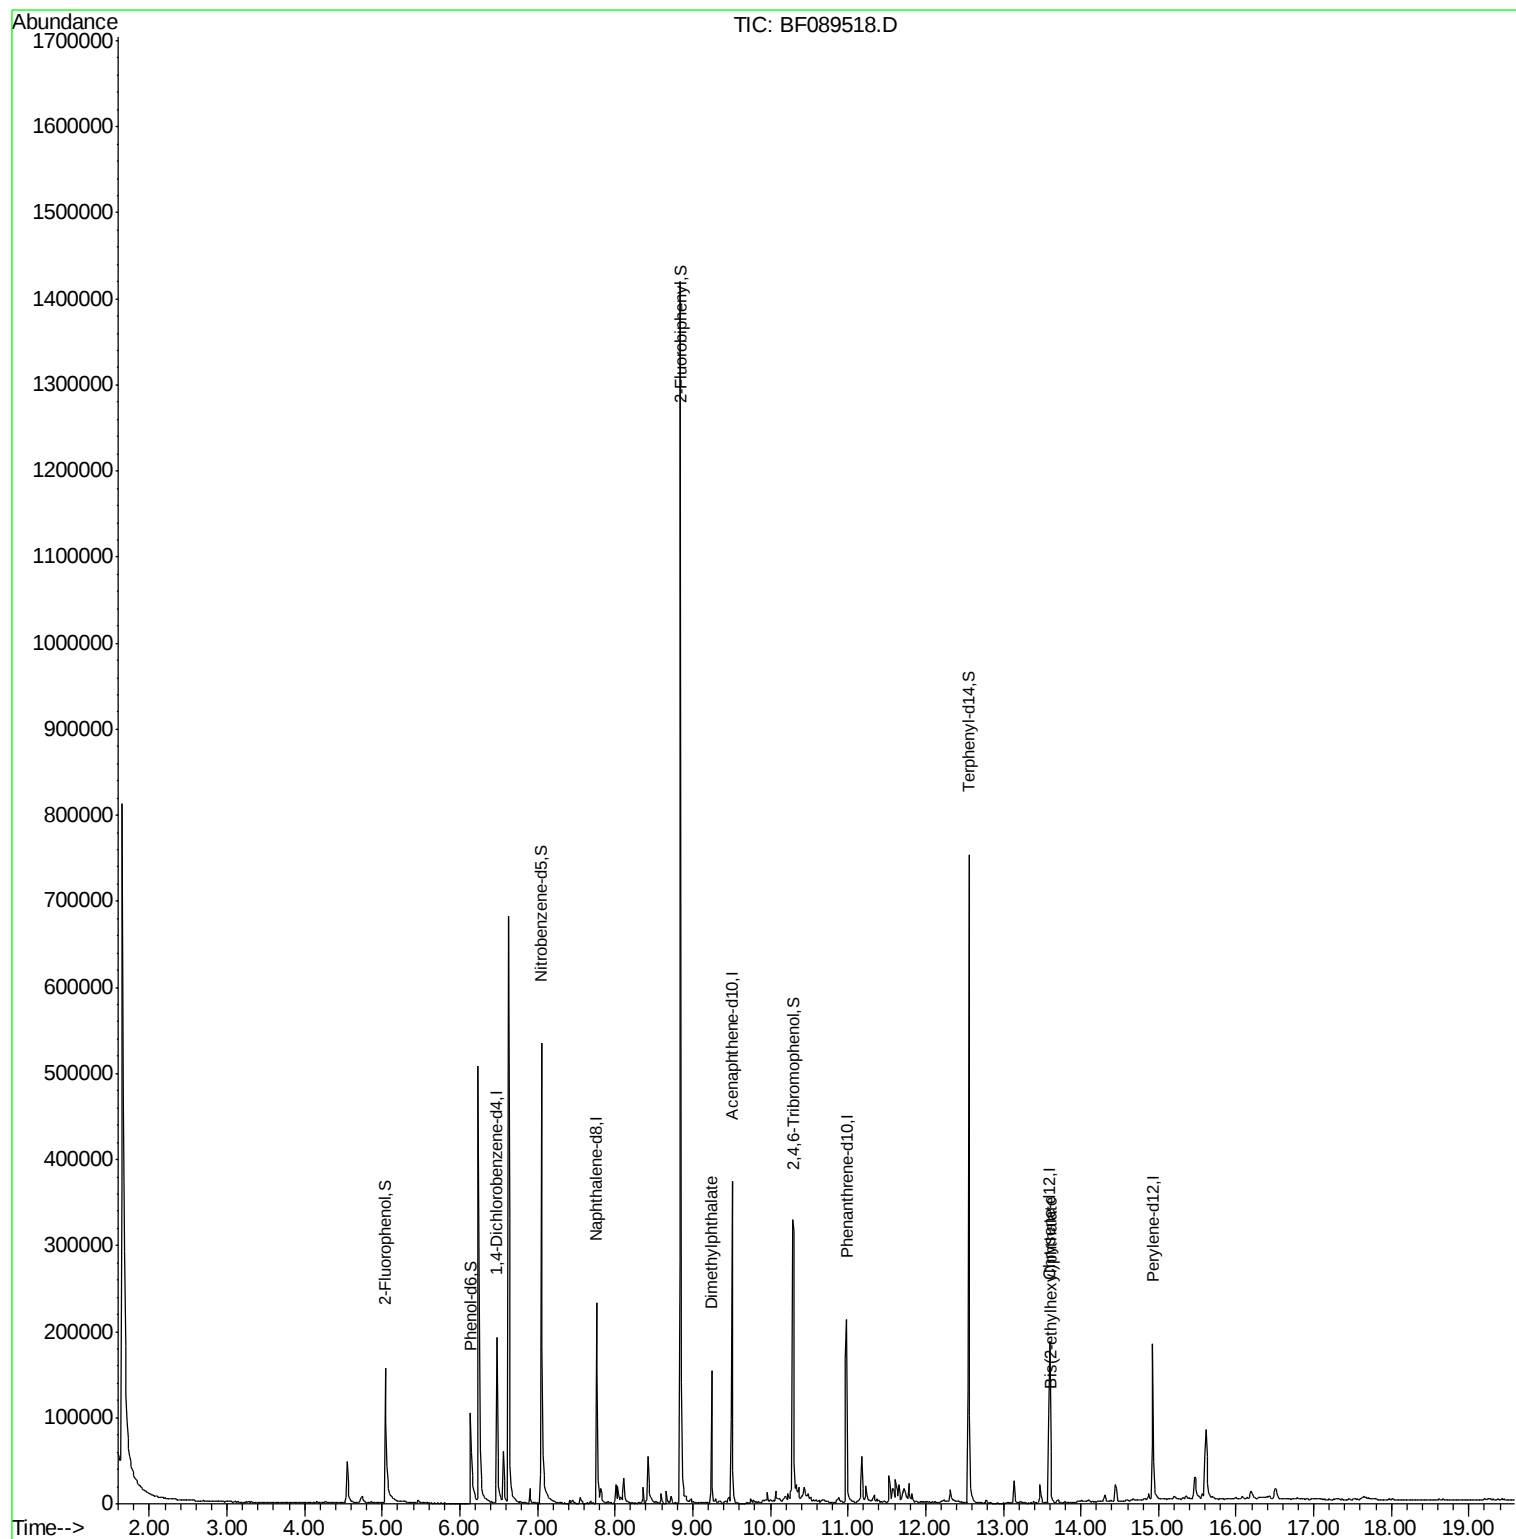

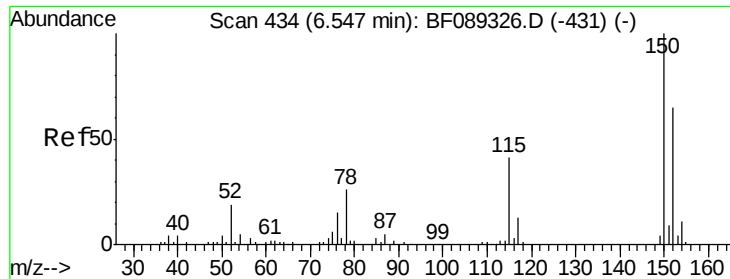

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.48 min Scan# 428

Delta R.T. -0.00 min

Lab File: BF089518.D

Acq: 1 Aug 2016 18:56

Instrument :

BNA_F

ClientSampleId :

MH-6


Tot Ion:152 Resp: 39635

Ion Ratio Lower Upper

152 100

150 153.6 129.5 194.3




115 63.3 51.4 77.2

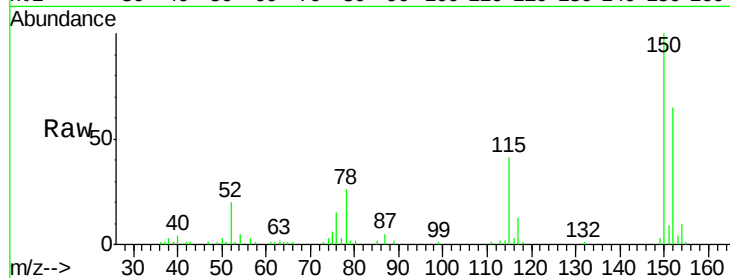

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

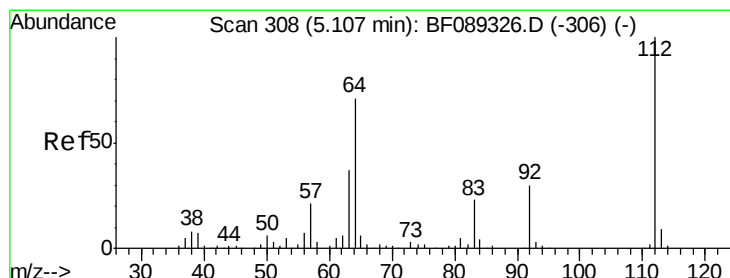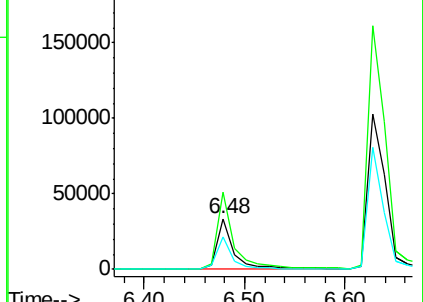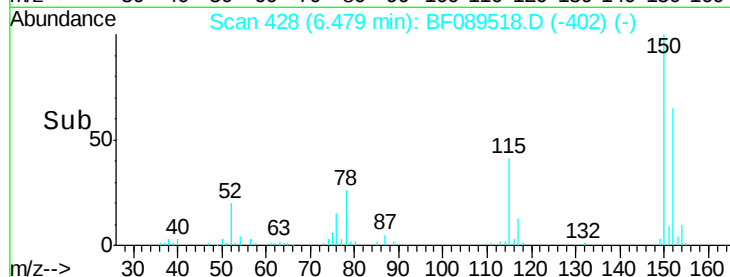

#5

2-Fluorophenol

Concen: 34.53 ng

RT: 5.04 min Scan# 302

Delta R.T. -0.00 min

Lab File: BF089518.D

Acq: 1 Aug 2016 18:56


Tgt Ion:112 Resp: 85710

Ion Ratio Lower Upper

112 100

64 62.1 55.0 82.6



63 32.8 29.4 44.2

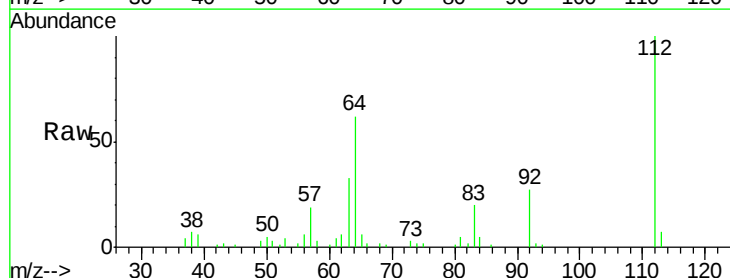

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

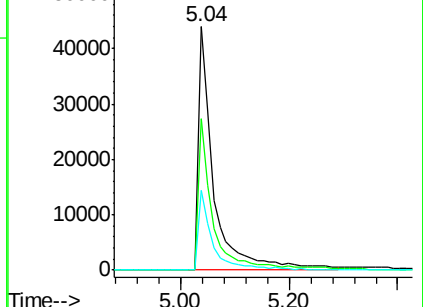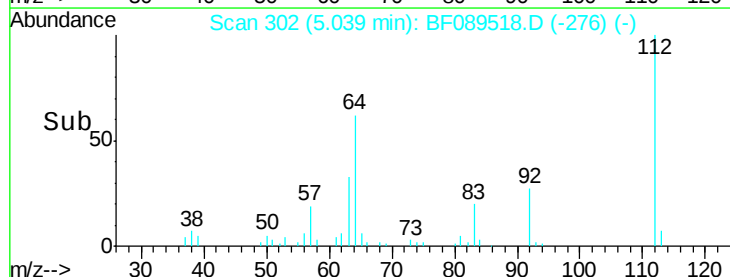



#7

Phenol-d6

Concen: 22.74 ng

RT: 6.14 min Scan# 398

Delta R.T. -0.01 min

Lab File: BF089518.D

Acq: 1 Aug 2016 18:56

Instrument :

BNA_F

ClientSampled :

MH-6


Tot Ion: 99 Resp: 74613

Ion Ratio Lower Upper

99 100

42 18.3 13.6 20.4




71 37.2 29.4 44.2

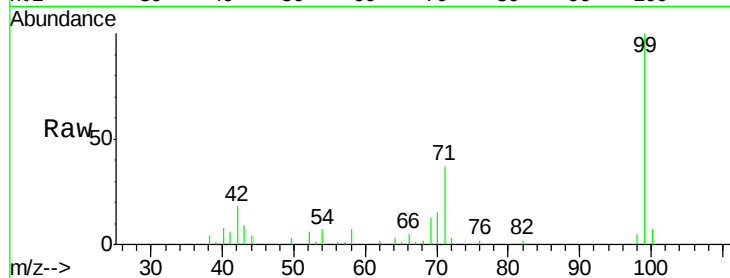

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

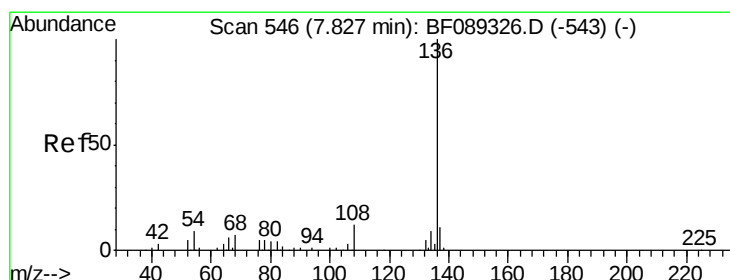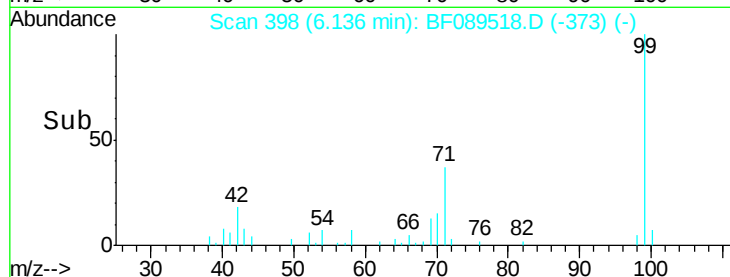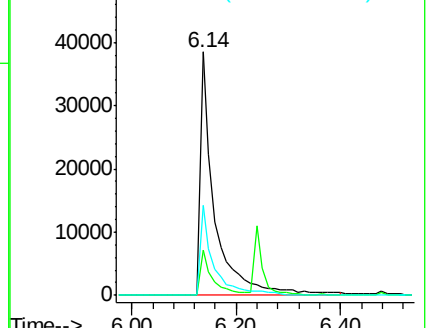

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.76 min Scan# 540

Delta R.T. -0.01 min

Lab File: BF089518.D

Acq: 1 Aug 2016 18:56

Tgt Ion: 136 Resp: 163127


Ion Ratio Lower Upper

136 100

137 11.1 8.6 13.0

54 10.2 7.0 10.4

68 7.9 4.9 7.3#


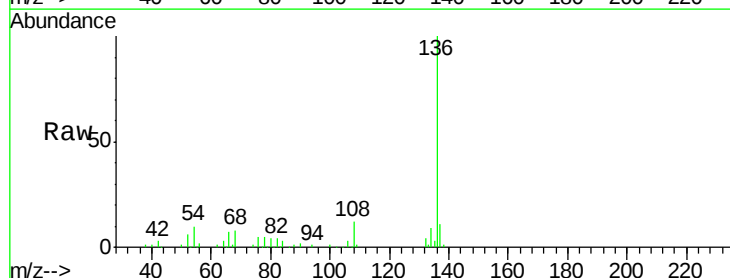



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

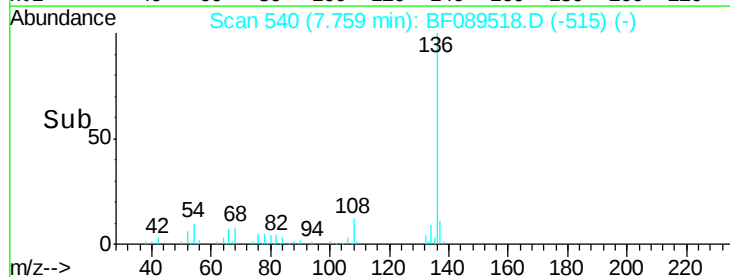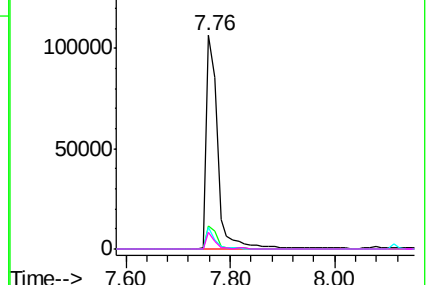


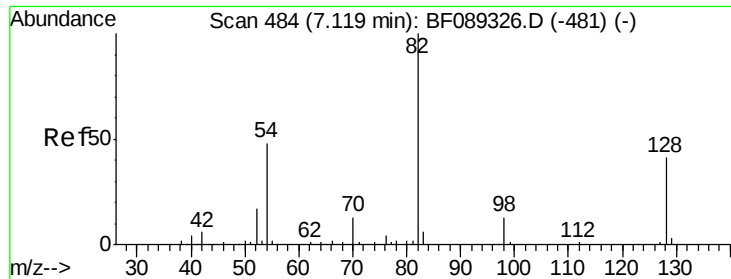




#23
 Nitrobenzene-d5
 Concen: 84.76 ng
 RT: 7.05 min Scan# 478
 Delta R.T. -0.01 min
 Lab File: BF089518.D
 Acq: 1 Aug 2016 18:56

Instrument :
 BNA_F
 ClientSampled :
 MH-6

Tot Ion	82	Resp	234256
Ion Ratio	100	Lower	Upper
128	39.4	32.5	48.7
54	48.9	38.8	58.2

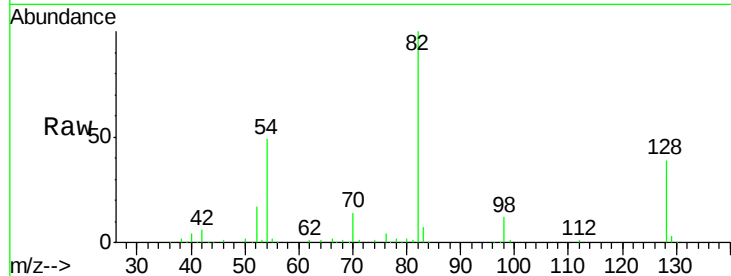


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

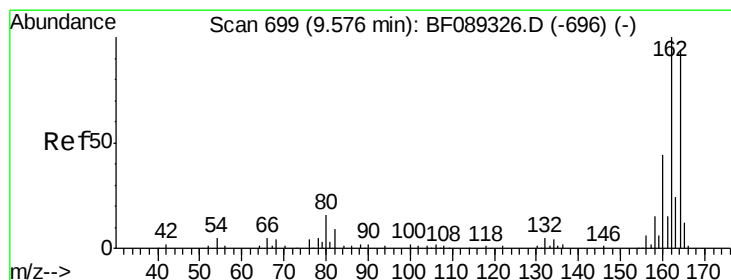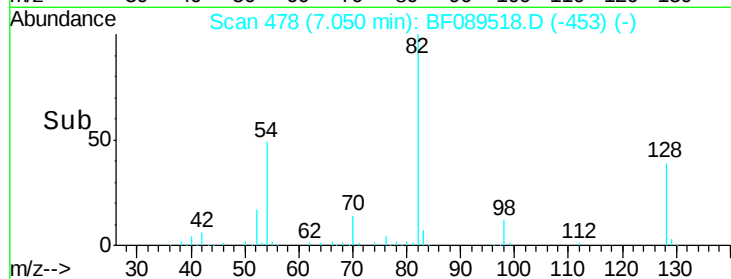
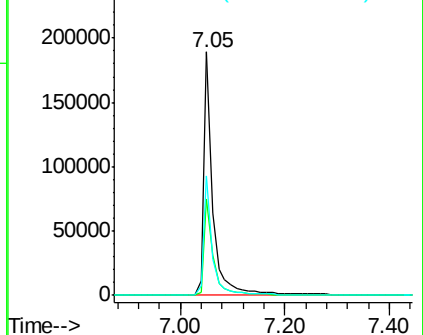



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.51 min Scan# 693
 Delta R.T. -0.01 min
 Lab File: BF089518.D
 Acq: 1 Aug 2016 18:56

Tgt Ion	164	Resp	74382
Ion Ratio	100	Lower	Upper
162	108.6	83.7	125.5
160	47.6	37.8	56.6

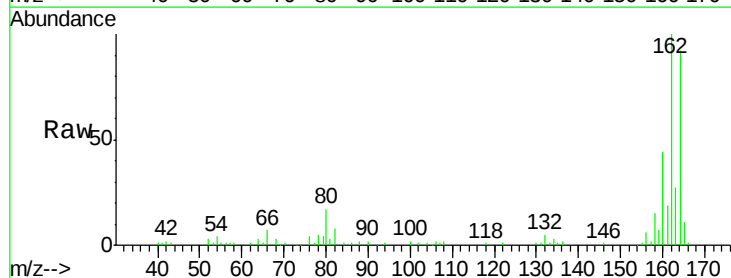

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



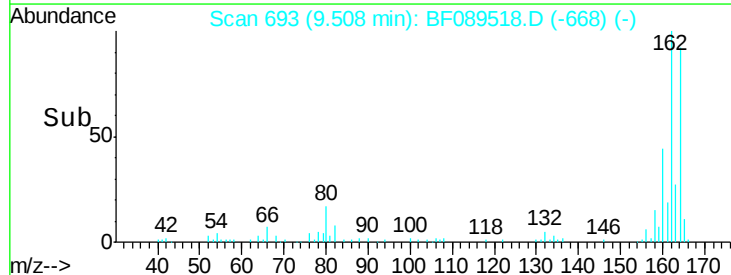
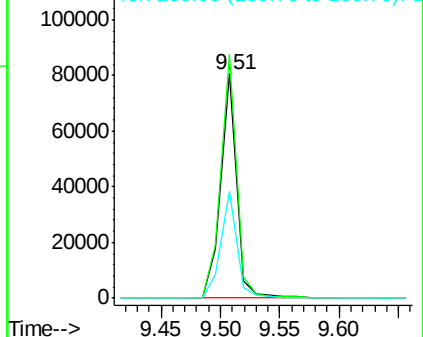


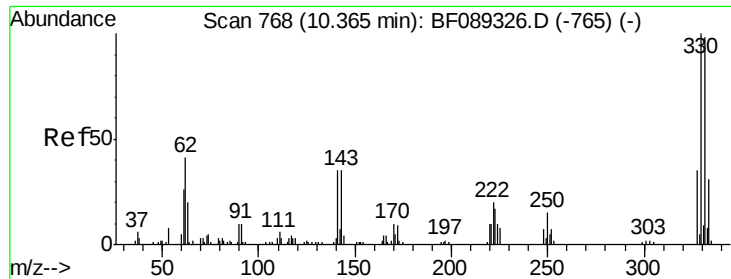

#41
 2,4,6-Tribromophenol
 Concen: 86.04 ng
 RT: 10.30 min Scan# 762
 Delta R.T. -0.01 min
 Lab File: BF089518.D
 Acq: 1 Aug 2016 18:56




Instrument :
 BNA_F
 ClientSampleId :
 MH-6


Tot Ion	Ratio	Lower	Upper
330	100		
332	94.5	76.8	115.2
141	45.8	37.3	55.9

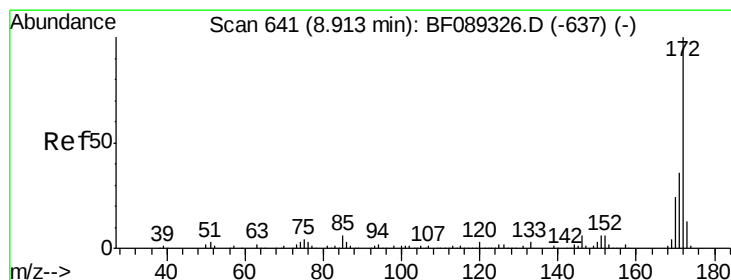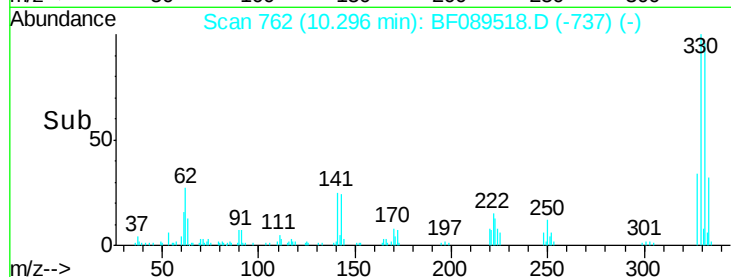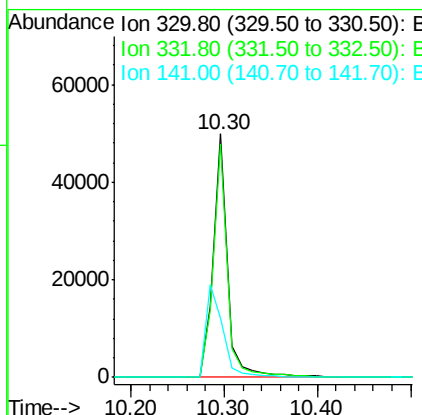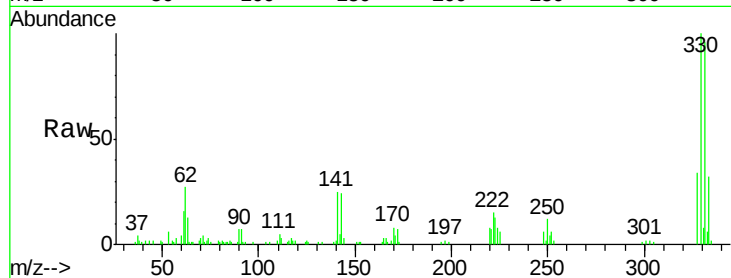

#44
 2-Fluorobiphenyl
 Concen: 88.12 ng
 RT: 8.84 min Scan# 635
 Delta R.T. -0.01 min
 Lab File: BF089518.D
 Acq: 1 Aug 2016 18:56

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.4	29.2	43.8
170	23.6	19.2	28.8


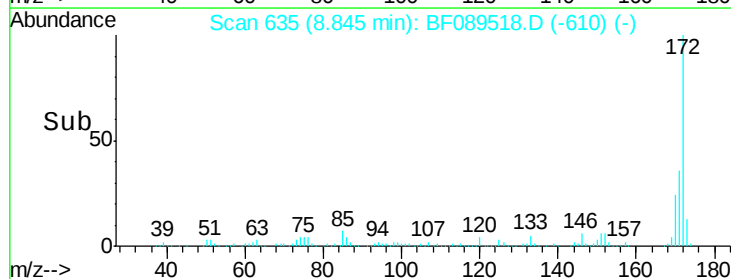
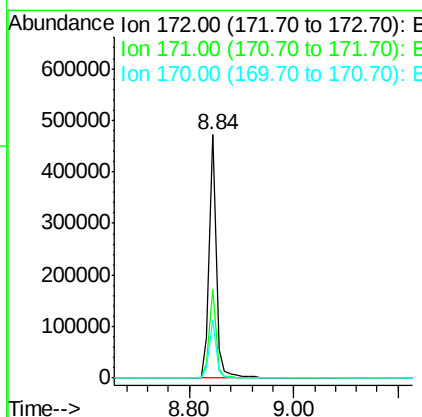
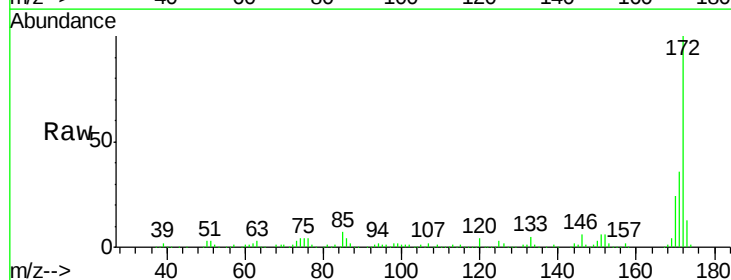


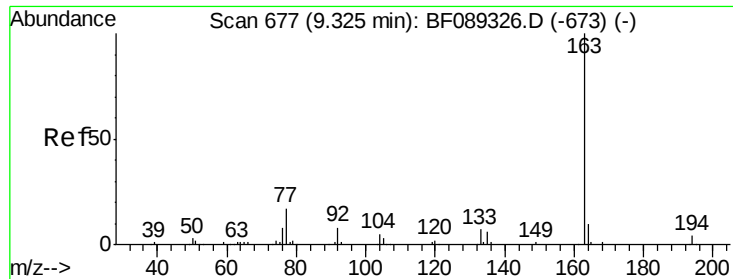

#49
Dimethylphthalate
Concen: 10.54 ng
RT: 9.24 min Scan# 670
Delta R.T. -0.02 min
Lab File: BF089518.D
Acq: 1 Aug 2016 18:56




Instrument :
BNA_F
ClientSampled :
MH-6


Tot Ion:163 Resp: 59653
Ion Ratio Lower Upper
163 100
194 3.5 2.8 4.2
164 10.0 7.8 11.8

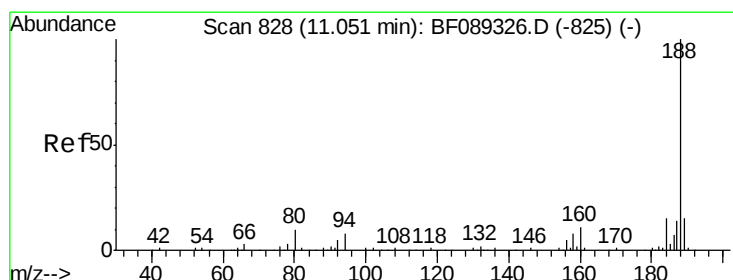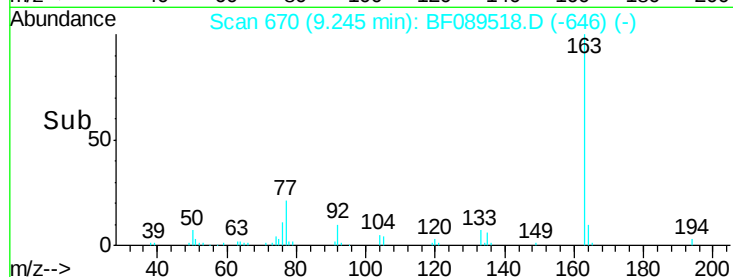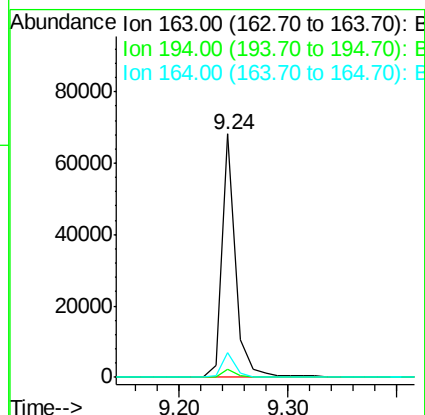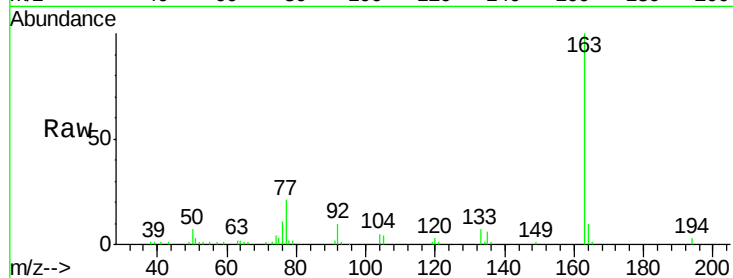

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.98 min Scan# 822
Delta R.T. -0.00 min
Lab File: BF089518.D
Acq: 1 Aug 2016 18:56

Tgt Ion:188 Resp: 124584
Ion Ratio Lower Upper
188 100
94 7.2 6.5 9.7
80 7.5 7.2 10.8

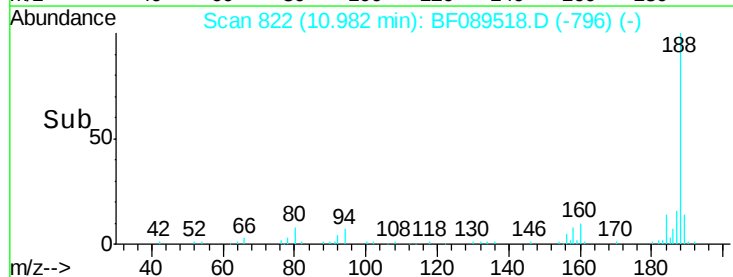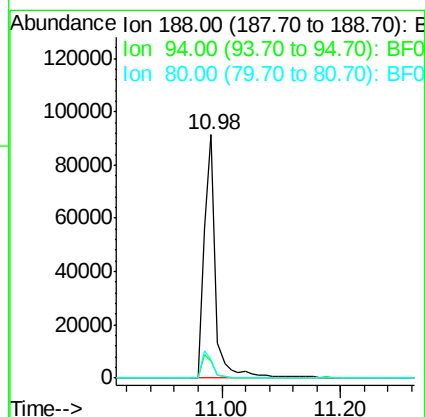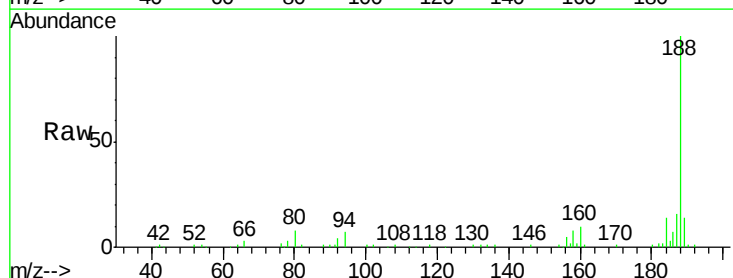

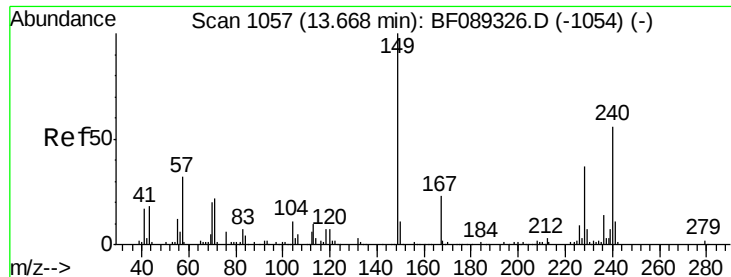

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.60 min Scan# 1051

Delta R.T. -0.01 min

Lab File: BF089518.D

Acq: 1 Aug 2016 18:56

Instrument :

BNA_F

ClientSampleId :

MH-6


Tot Ion:240 Resp: 75361

Ion Ratio Lower Upper

240 100

120 9.8 9.1 13.7




236 25.1 20.6 30.8

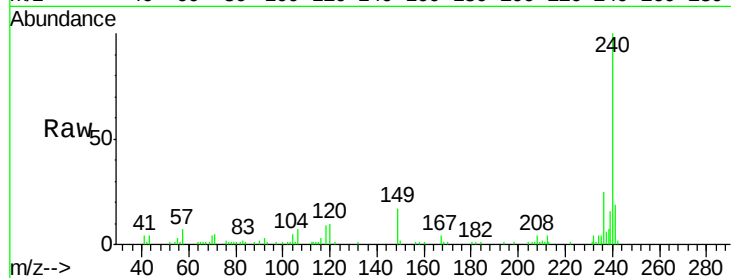

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

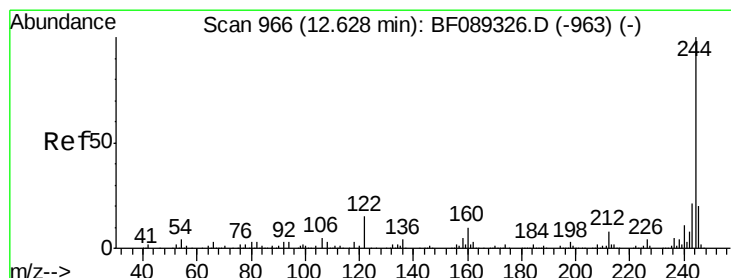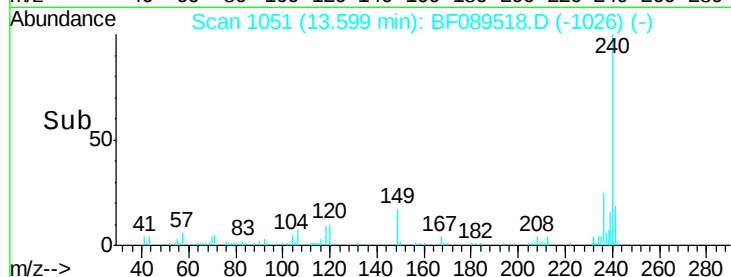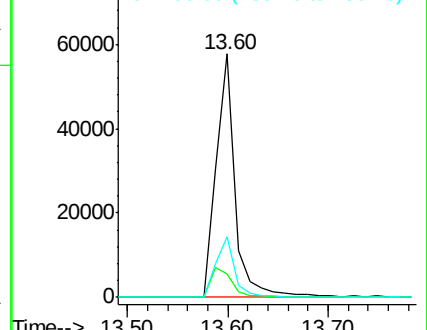

#78

Terphenyl-d14

Concen: 71.40 ng

RT: 12.56 min Scan# 960

Delta R.T. -0.01 min

Lab File: BF089518.D

Acq: 1 Aug 2016 18:56


Tgt Ion:244 Resp: 229909

Ion Ratio Lower Upper

244 100

212 7.8 6.5 9.7



122 12.5 11.4 17.0

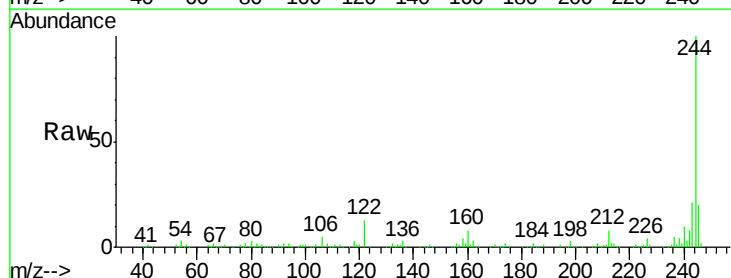


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

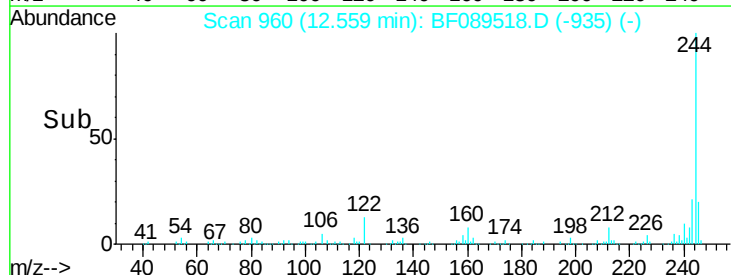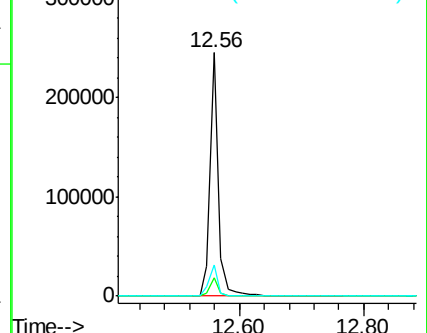


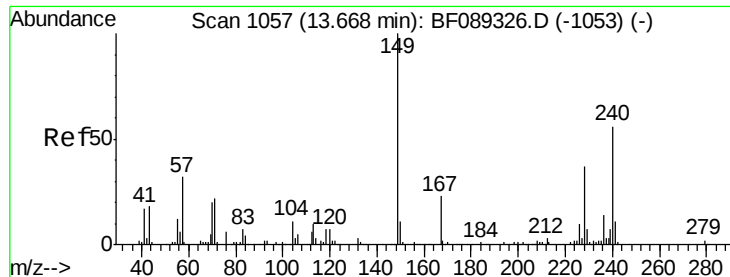




#83
 Bis(2-ethylhexyl)phthalate
 Concen: 4.19 ng
 RT: 13.61 min Scan# 1052
 Delta R.T. -0.00 min
 Lab File: BF089518.D
 Acq: 1 Aug 2016 18:56

Instrument :
 BNA_F
 ClientSampleId :
 MH-6

Tot Ion:149 Resp: 15731
 Ion Ratio Lower Upper
 149 100
 167 26.5 18.8 28.2
 279 3.9 1.4 2.0#

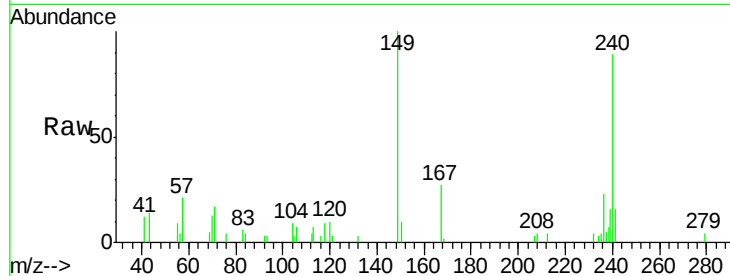


Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 167.00 (166.70 to 167.70): E
 Ion 279.00 (278.70 to 279.70): E

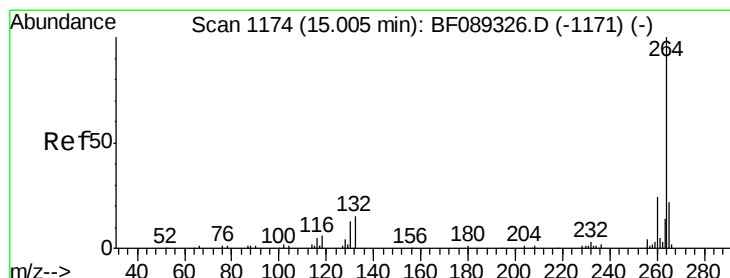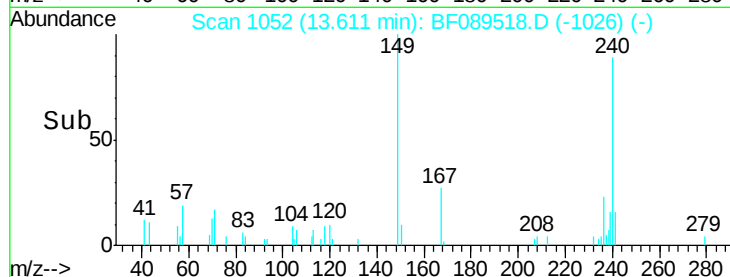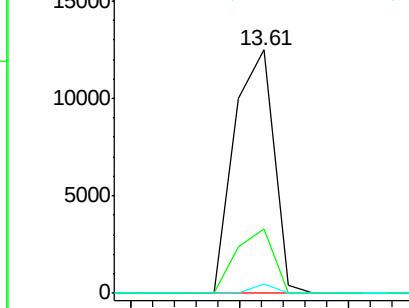

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 14.93 min Scan# 1167
 Delta R.T. -0.01 min
 Lab File: BF089518.D
 Acq: 1 Aug 2016 18:56

Tgt Ion:264 Resp: 78420
 Ion Ratio Lower Upper
 264 100
 260 23.8 19.0 28.4
 265 21.3 17.5 26.3

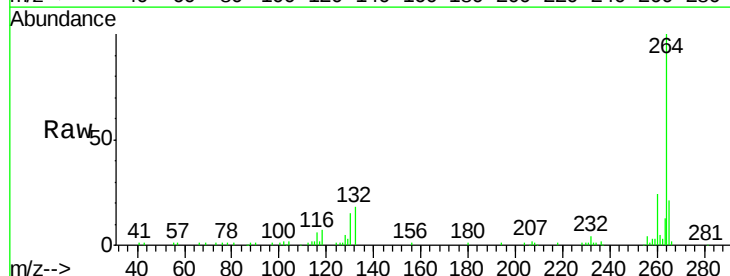

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

