


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080116\
 Data File : BF089504.D
 Acq On : 1 Aug 2016 11:41
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 28 16:02:32 2016

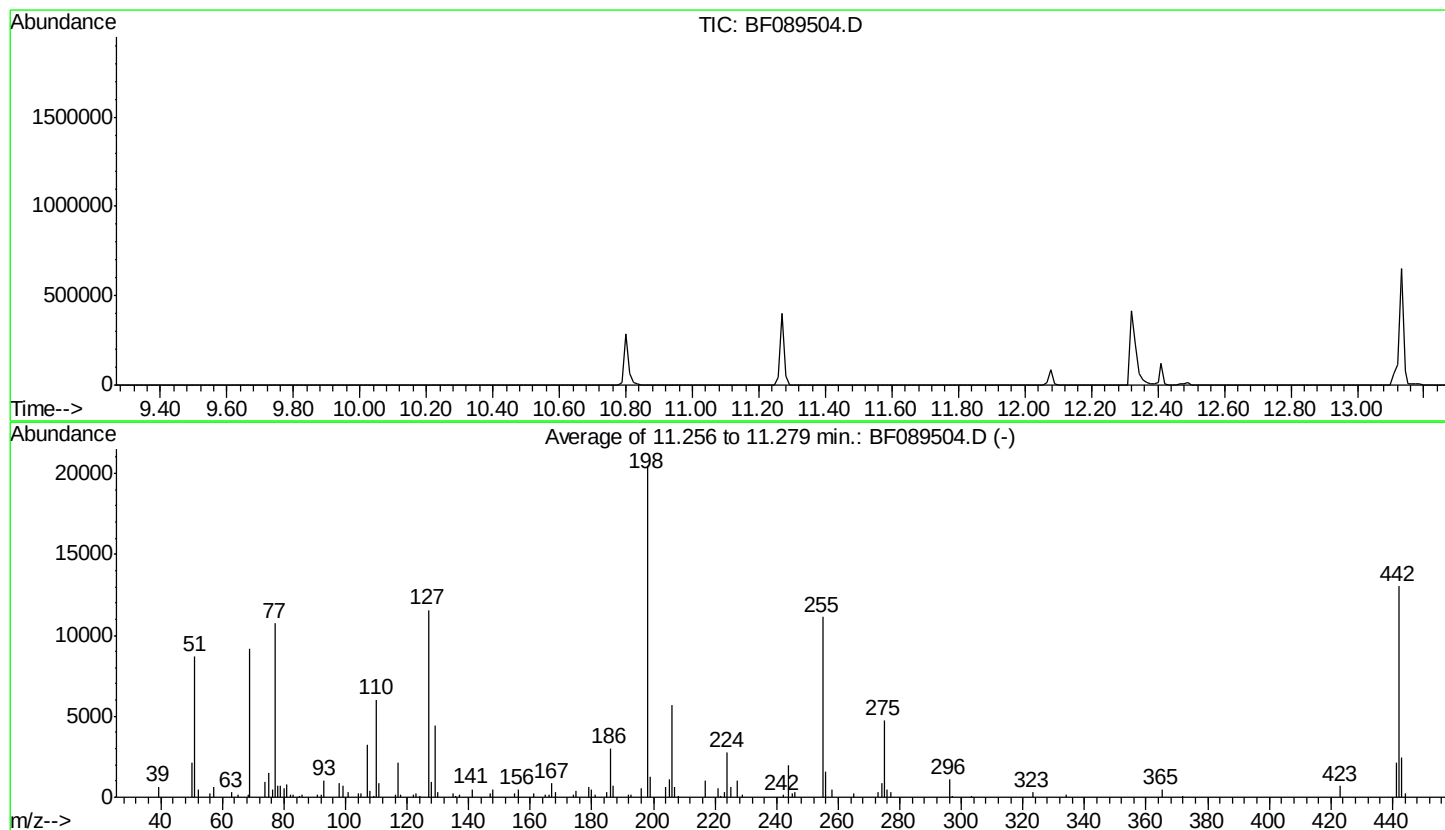

AutoFind: Scans 846, 847, 848; Background Corrected with Scan 843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	8681	PASS
68	69	0.00	2	1.6	147	PASS
69	198	0.00	100	44.9	9204	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	56.4	11554	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20480	PASS
199	198	5	9	6.4	1301	PASS
275	198	10	60	23.1	4721	PASS
365	198	1	100	2.2	444	PASS
441	442	0.01	24	16.6	2161	PASS
442	198	50	100	63.7	13040	PASS
443	442	15	24	18.9	2460	PASS