
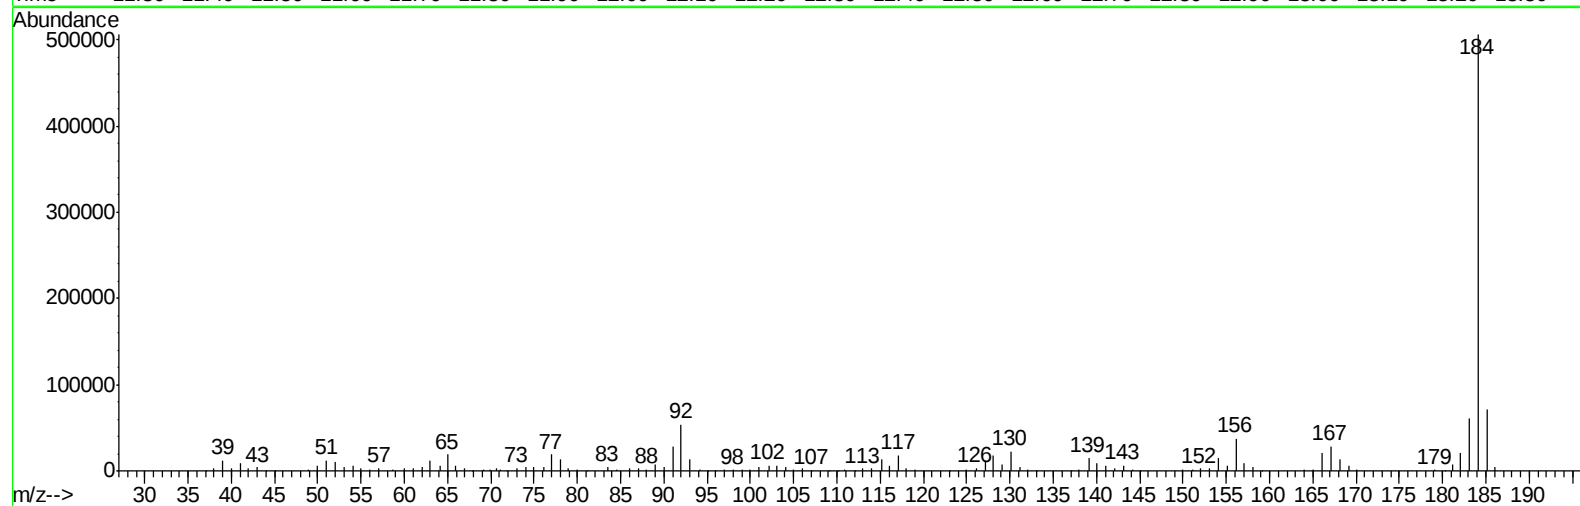


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
Data File : BF097223.D
Acq On : 1 Aug 2017 10:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 09:24:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

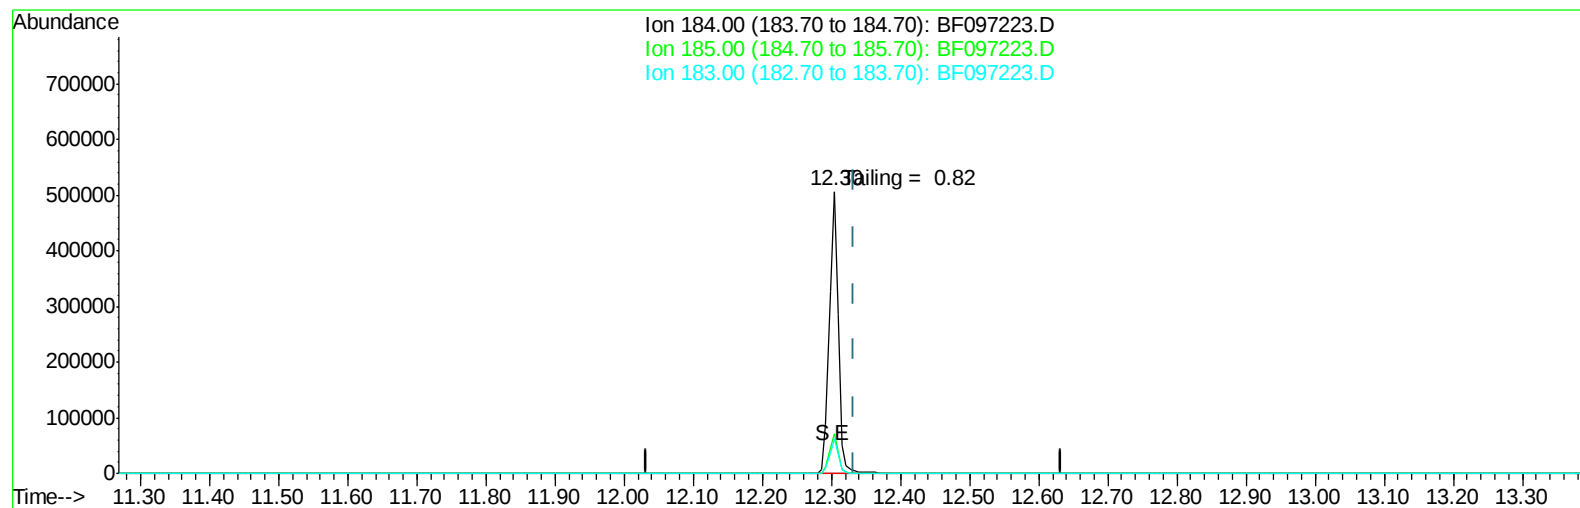

TIC: BF097223.D

(76) Benzidine



12.304min (-0.030) 79027.97ng

response 460374

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.12#
183.00	12.20	12.07
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
Data File : BF097223.D
Acq On : 1 Aug 2017 10:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 09:24:13 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

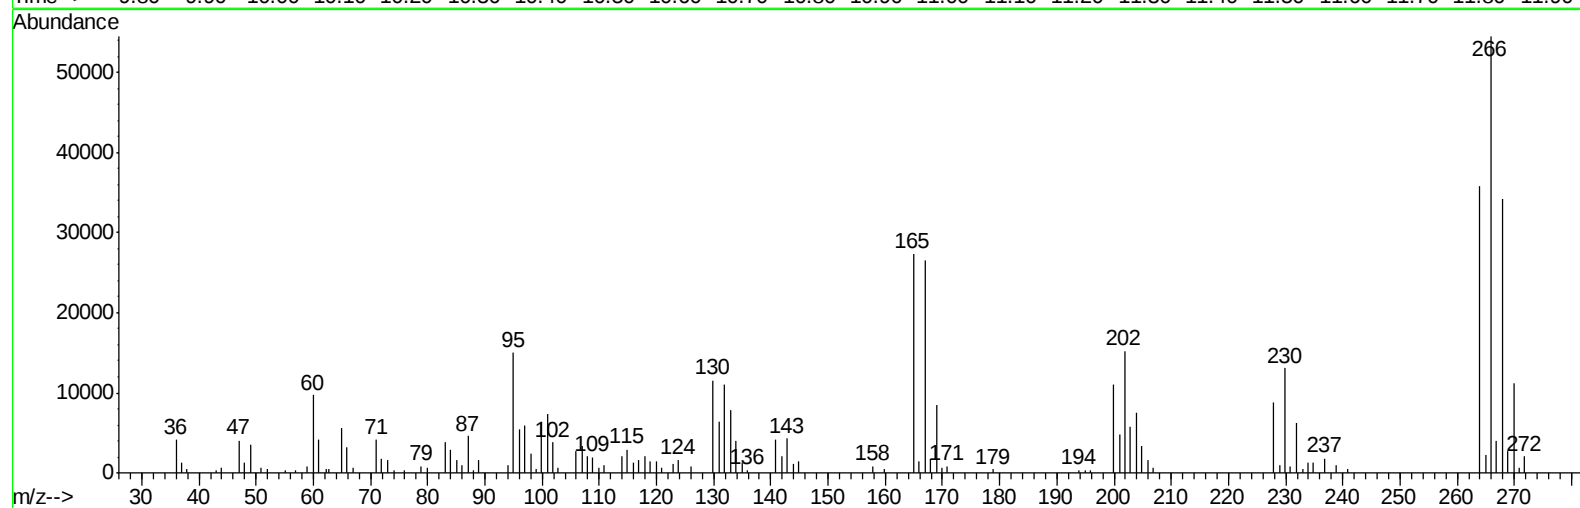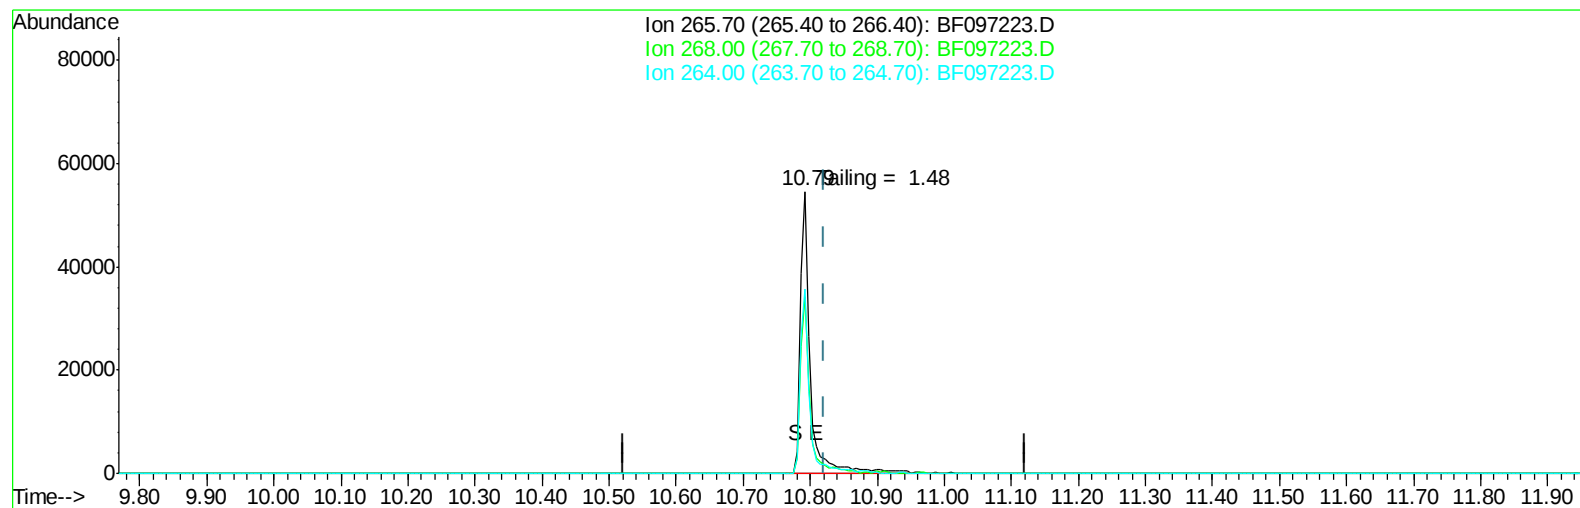

TIC: BF097223.D

(69) Pentachlorophenol (C)

10.792min (-0.029) 40622.31ng

response 57182

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.80
264.00	64.60	65.57
0.00	0.00	0.00