

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
 Data File : BF097258.D
 Acq On : 2 Aug 2017 7:00
 Operator : SJ/JU
 Sample : I4527-03 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-HS7-ESW

Quant Time: Aug 02 07:57:45 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 14:11:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.46	152	104125	20.00	ng	-0.04
21) Naphthalene-d8	7.75	136	391140	20.00	ng	-0.04
38) Acenaphthene-d10	9.49	164	159361	20.00	ng	-0.04
63) Phenanthrene-d10	10.96	188	209430	20.00	ng	-0.04
75) Chrysene-d12	13.59	240	210198	20.00	ng	-0.04
86) Perylene-d12	14.93	264	152368	20.00	ng	-0.04
System Monitoring Compounds						
5) 2-Fluorophenol	5.07	112	142091	20.57	ng	-0.03
7) Phenol-d6	6.13	99	165934	21.04	ng	-0.04
23) Nitrobenzene-d5	7.03	82	78211	11.73	ng	-0.05
41) 2,4,6-Tribromophenol	10.28	330	21268	16.89	ng	-0.04
44) 2-Fluorobiphenyl	8.82	172	156384	16.65	ng	-0.05
78) Terphenyl-d14	12.54	244	95759	9.29	ng	-0.04
Target Compounds						Qvalue
49) Dimethylphthalate	9.23	163	29983	2.478	ng	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
Data File : BF097258.D
Acq On : 2 Aug 2017 7:00
Operator : SJ/JU
Sample : I4527-03 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-HS7-ESW

Quant Time: Aug 02 07:57:45 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

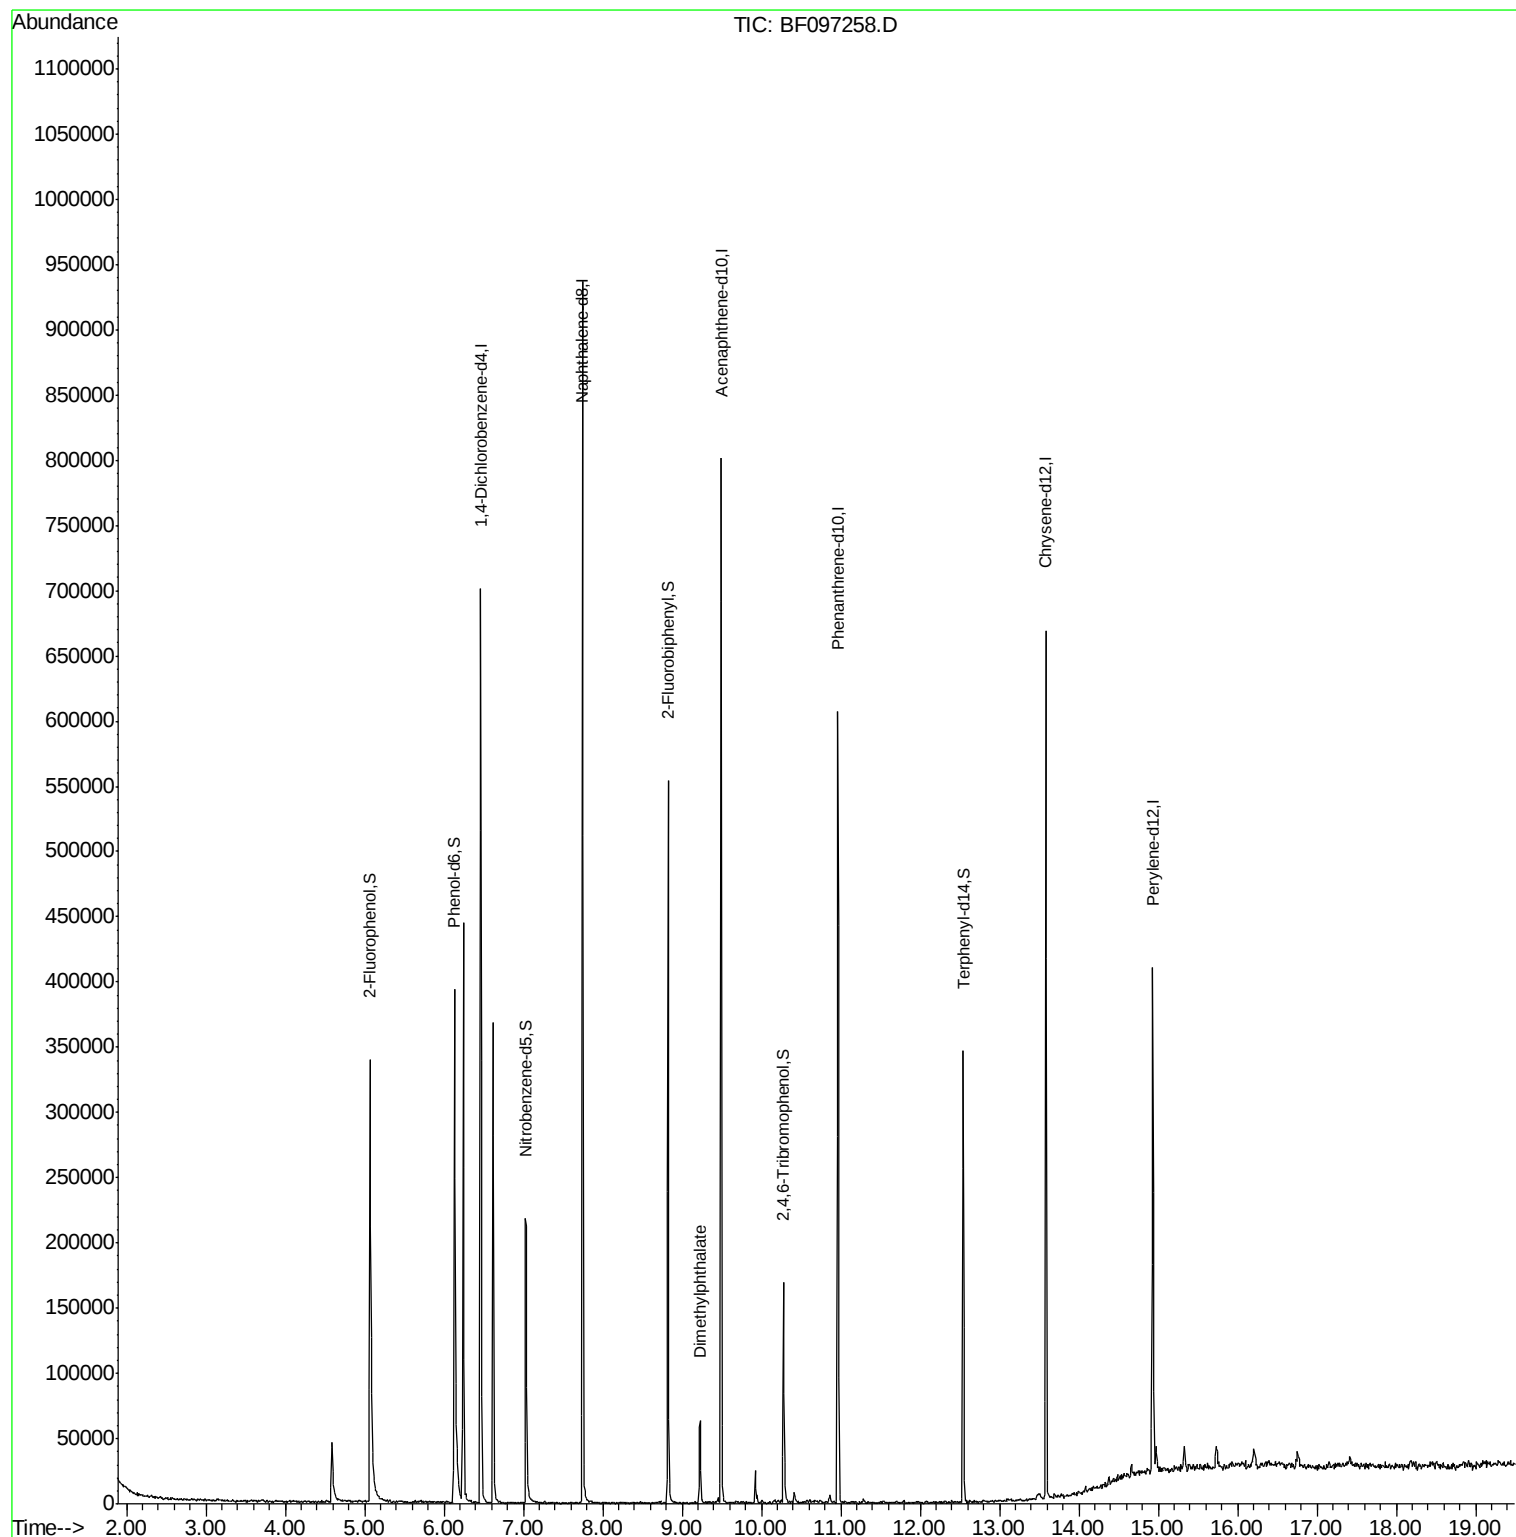

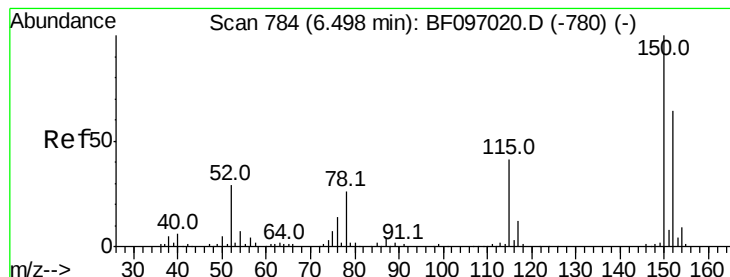

#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.46 min Scan# 778

Delta R.T. -0.04 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00

Instrument :

BNA_F

ClientSampleId :

E2-HS7-ESW


Tot Ion:152 Resp: 104125

Ion Ratio Lower Upper

152 100

150 150.5 126.2 189.2




115 61.6 52.2 78.2

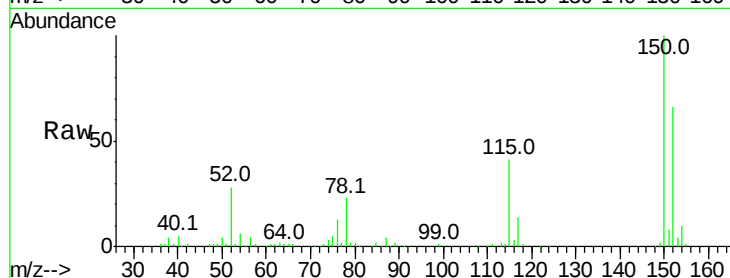

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

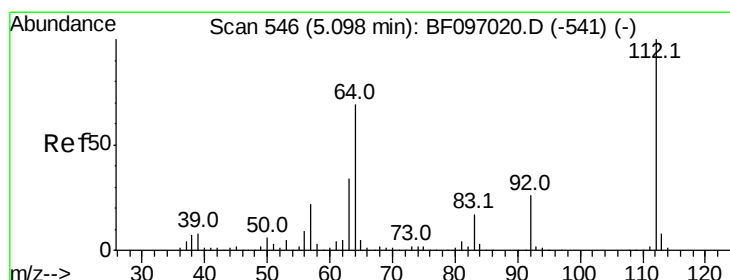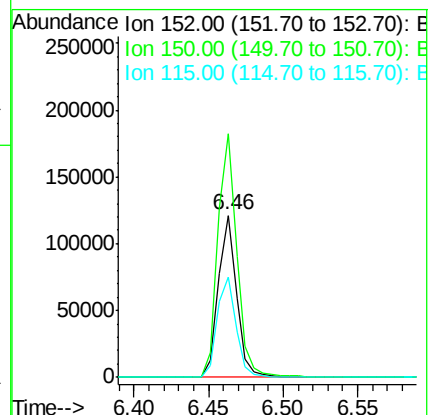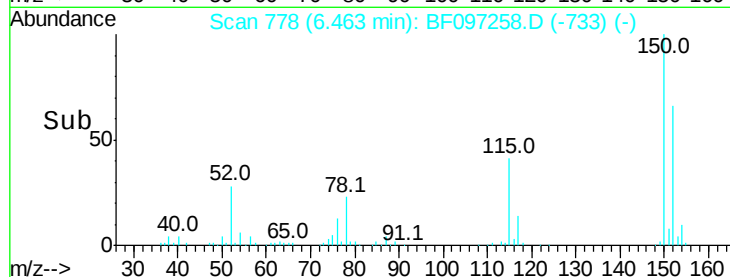

#5

2-Fluorophenol

Concen: 20.571 ng

RT: 5.07 min Scan# 541

Delta R.T. -0.03 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00


Tgt Ion:112 Resp: 142091

Ion Ratio Lower Upper

112 100

64 62.2 46.0 69.0



63 30.4 23.4 35.0

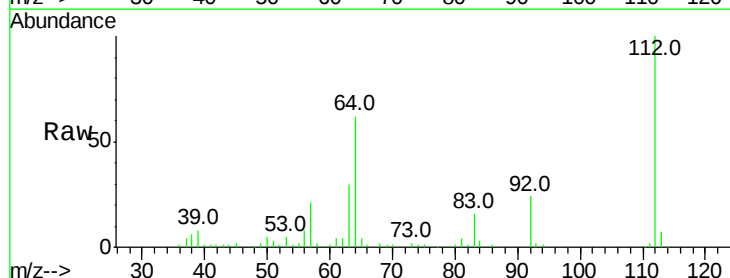


Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

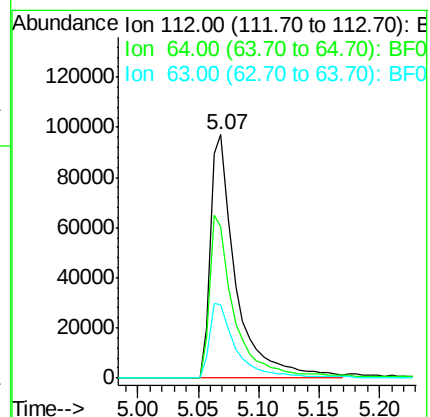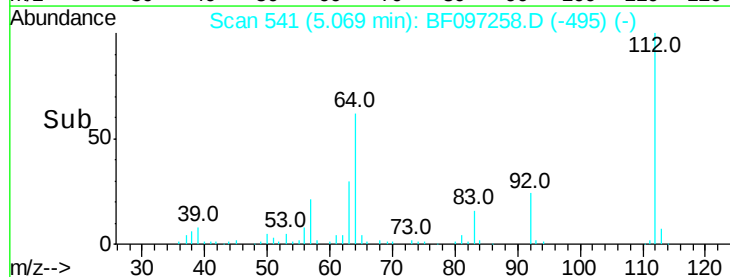

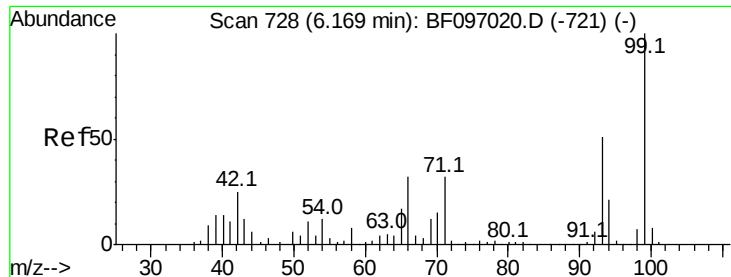

#7

Phenol-d6

Concen: 21.043 ng

RT: 6.13 min Scan# 722

Delta R.T. -0.04 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00

Instrument :


BNA_F

ClientSampleId :

E2-HS7-ESW

Tot Ion: 99 Resp: 165934




Ion	Ratio	Lower	Upper
99	100		
42	22.1	13.5	20.3#
71	30.5	24.5	36.7

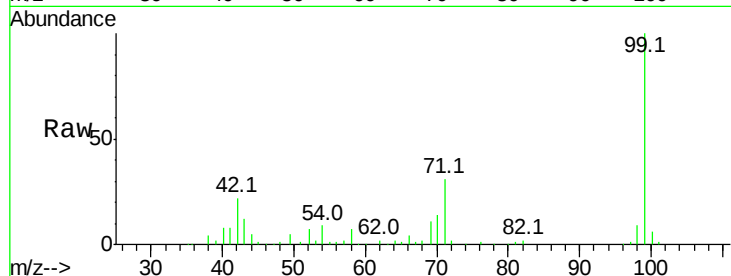

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

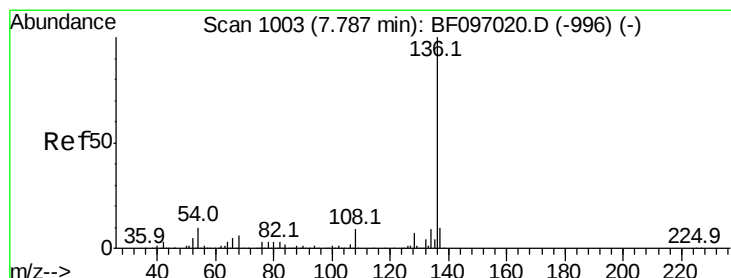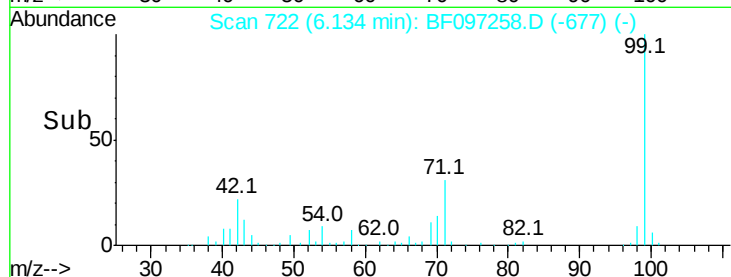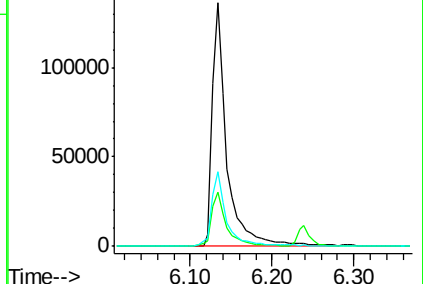

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.75 min Scan# 996

Delta R.T. -0.04 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00

Tgt Ion: 136 Resp: 391140




Ion	Ratio	Lower	Upper
136	100		
137	11.0	8.5	12.7
54	10.8	4.9	7.3#
68	5.4	4.1	6.1


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0


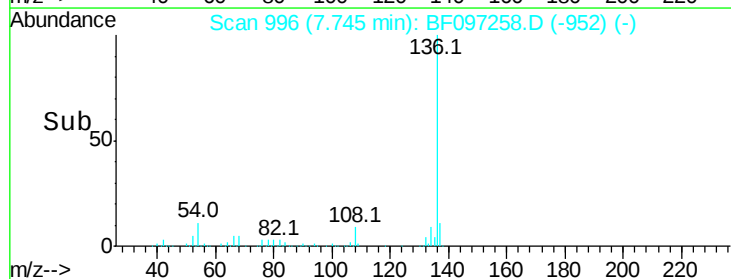
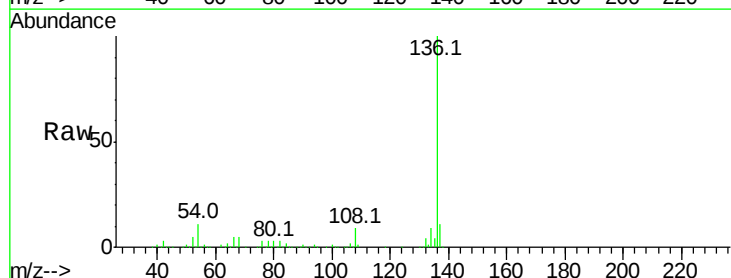
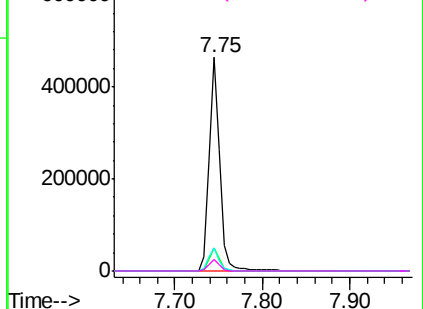


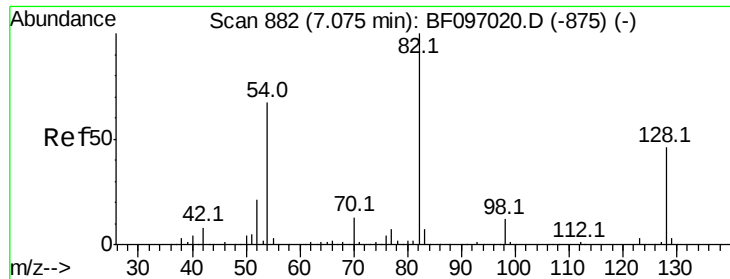

#23
 Nitrobenzene-d5
 Concen: 11.730 ng
 RT: 7.03 min Scan# 874
 Delta R.T. -0.05 min
 Lab File: BF097258.D
 Acq: 2 Aug 2017 7:00




Instrument :
 BNA_F
 ClientSampleId :
 E2-HS7-ESW


Tot Ion: 82 Resp: 78211
 Ion Ratio Lower Upper
 82 100
 128 41.7 34.0 51.0
 54 69.3 42.2 63.2#

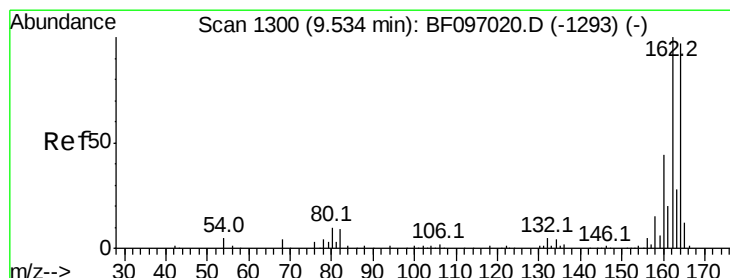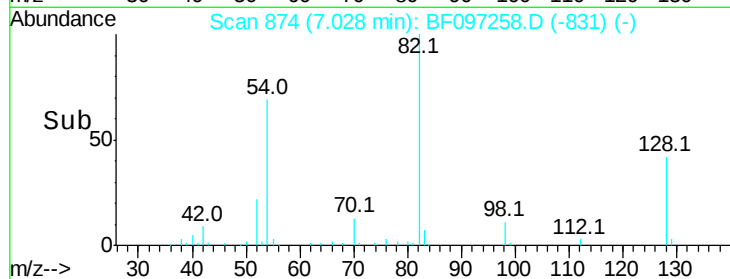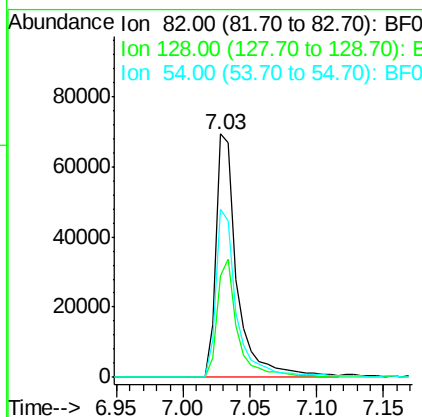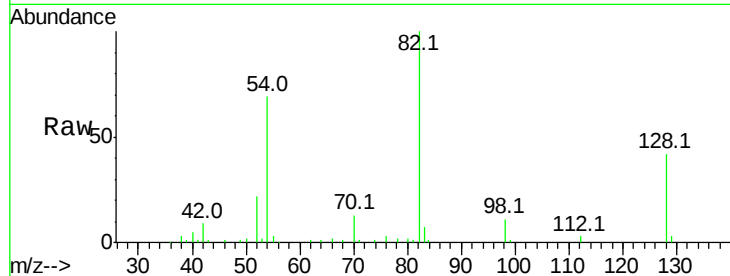

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.49 min Scan# 1293
 Delta R.T. -0.04 min
 Lab File: BF097258.D
 Acq: 2 Aug 2017 7:00

Tgt Ion:164 Resp: 159361
 Ion Ratio Lower Upper
 164 100
 162 104.5 82.6 123.8
 160 46.1 36.2 54.2

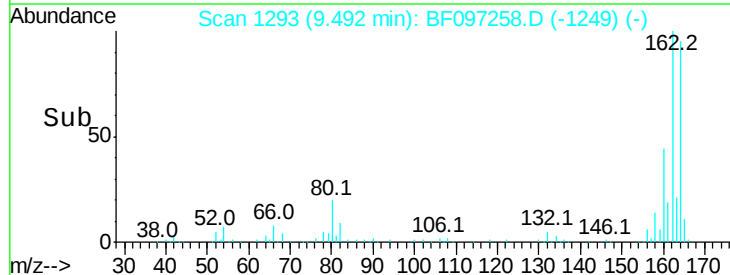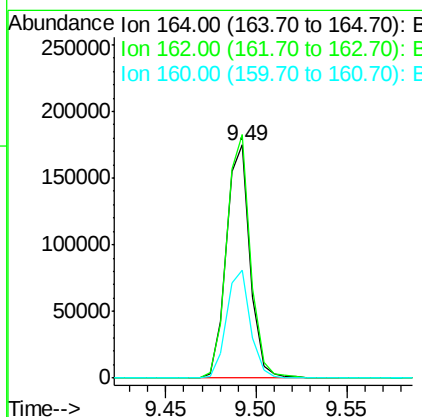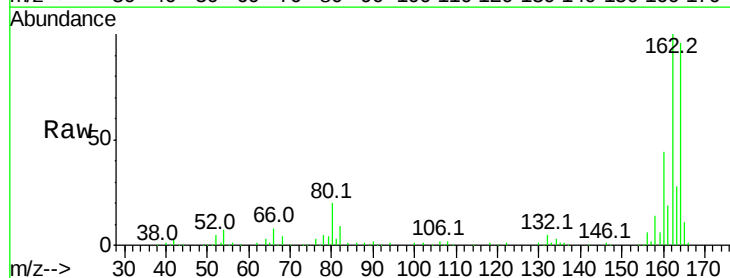


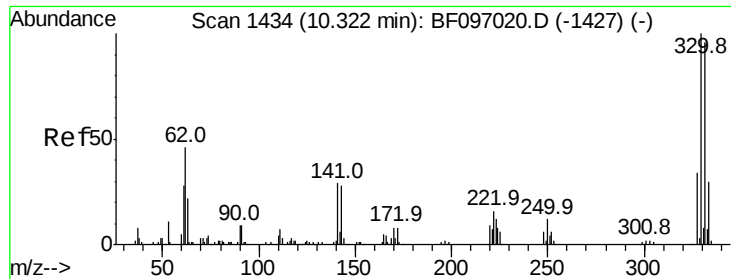




#41
 2,4,6-Tribromophenol
 Concen: 16.891 ng
 RT: 10.28 min Scan# 1427
 Delta R.T. -0.04 min
 Lab File: BF097258.D
 Acq: 2 Aug 2017 7:00

Instrument :
 BNA_F
 ClientSampleId :
 E2-HS7-ESW

Tot Ion:330 Resp: 21268
 Ion Ratio Lower Upper
 330 100
 332 91.6 76.6 115.0
 141 39.1 31.4 47.2

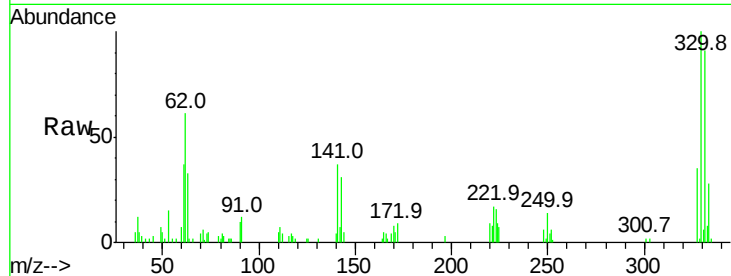


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

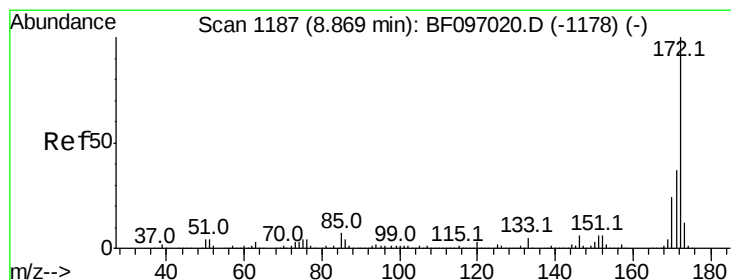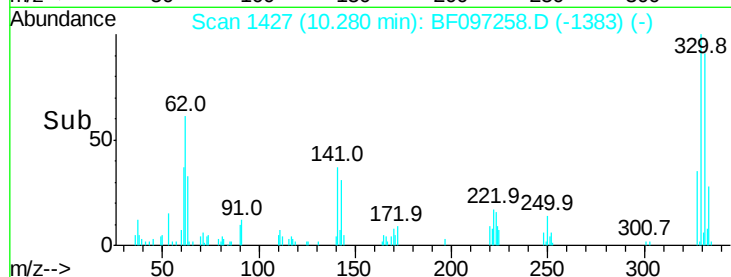
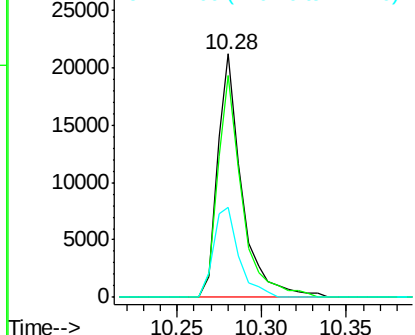



#44
 2-Fluorobiphenyl
 Concen: 16.654 ng
 RT: 8.82 min Scan# 1179
 Delta R.T. -0.05 min
 Lab File: BF097258.D
 Acq: 2 Aug 2017 7:00

Tgt Ion:172 Resp: 156384
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.6 44.4
 170 24.3 19.8 29.8

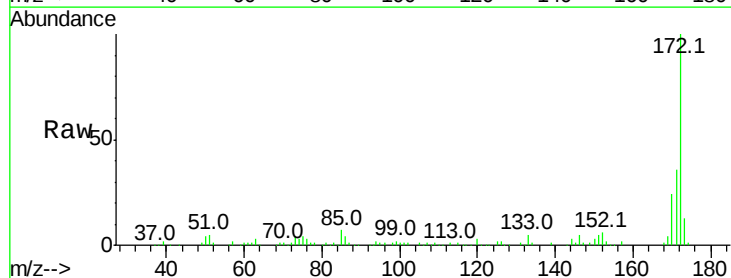

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

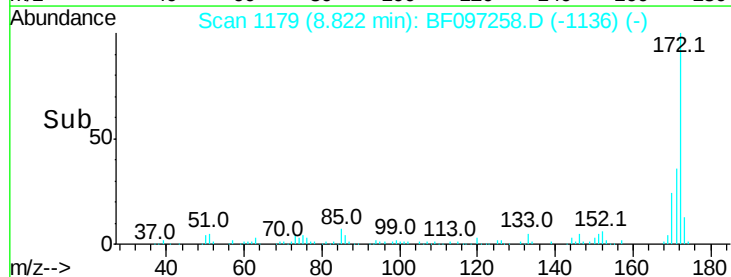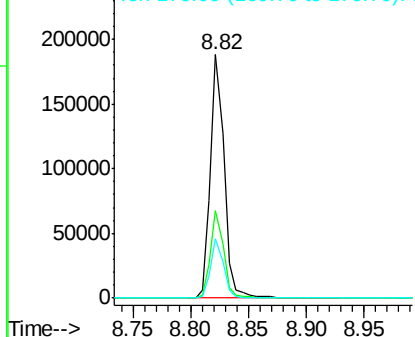

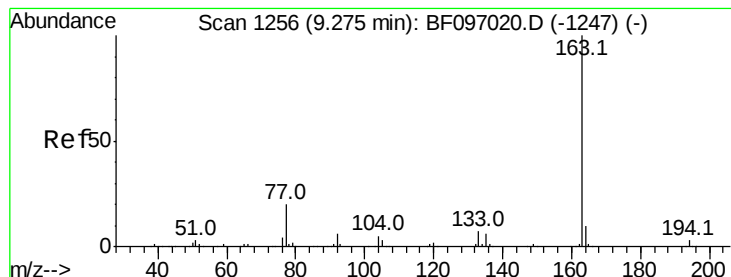

#49

Dimethylphthalate

Concen: 2.478 ng

RT: 9.23 min Scan# 1248

Delta R.T. -0.05 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00

Instrument :

BNA_F

ClientSampleId :

E2-HS7-ESW





Tot Ion:163 Resp: 29983

Ion Ratio Lower Upper

163 100

194 3.3 2.6 4.0

164 9.2 8.4 12.6

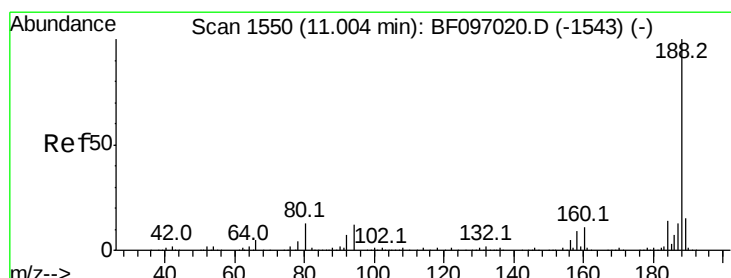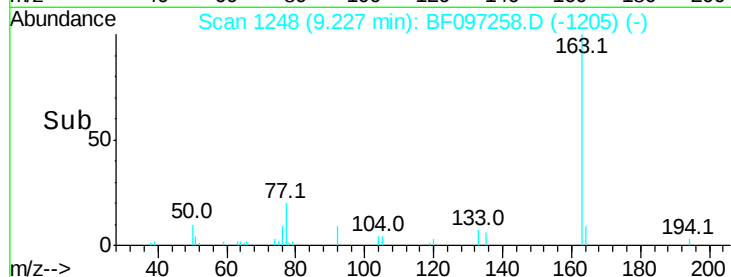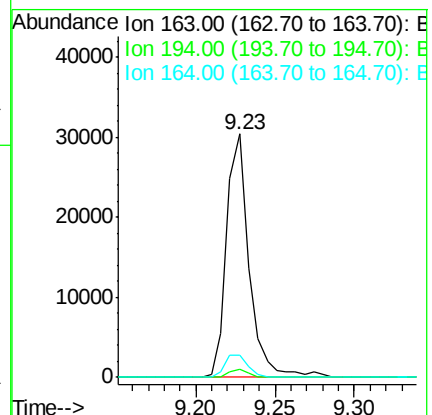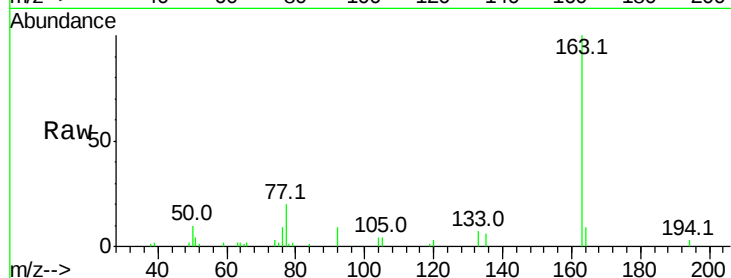

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 10.96 min Scan# 1543

Delta R.T. -0.04 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00




Tgt Ion:188 Resp: 209430


Ion Ratio Lower Upper

188 100

94 11.2 9.4 14.2

80 12.0 10.2 15.2

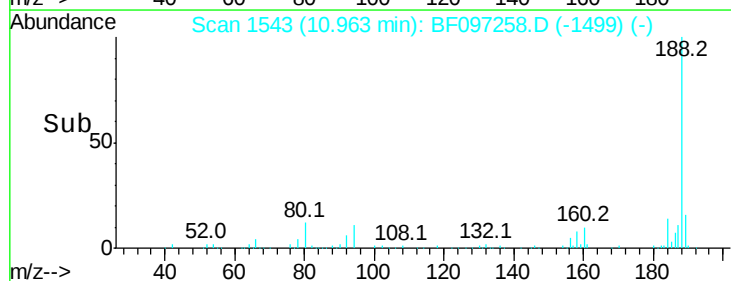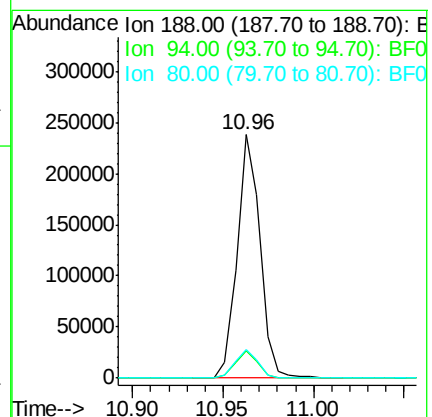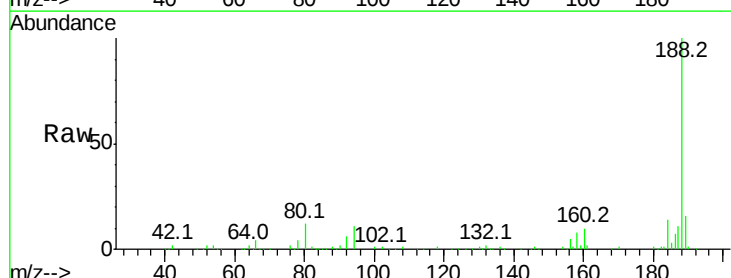

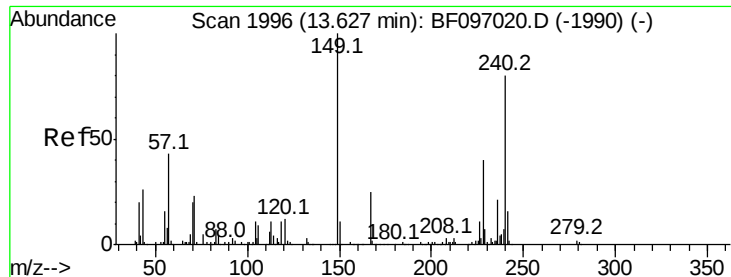

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.59 min Scan# 1989

Delta R.T. -0.04 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00

Instrument :

BNA_F

ClientSampleId :

E2-HS7-ESW


Tot Ion:240 Resp: 210198

Ion Ratio Lower Upper

240 100

120 15.0 5.8 8.8#




236 25.3 20.5 30.7

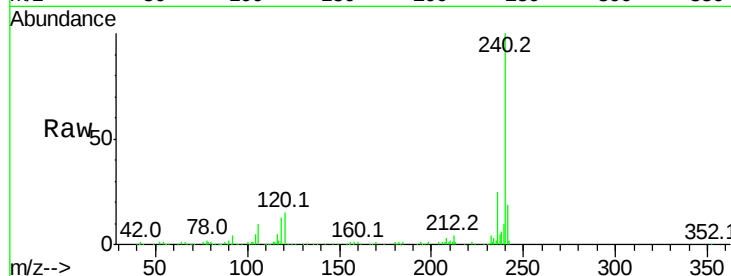

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

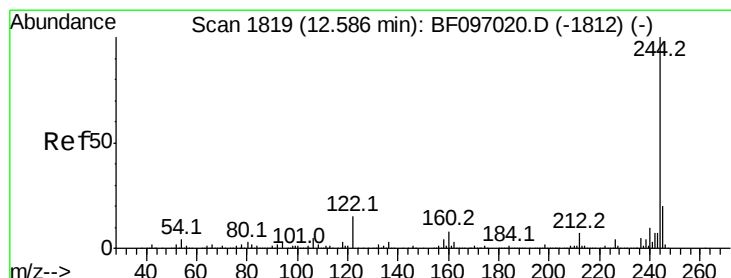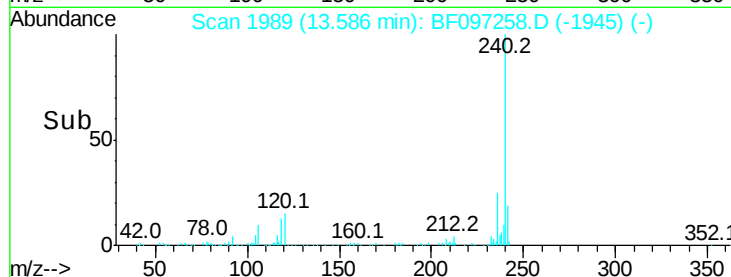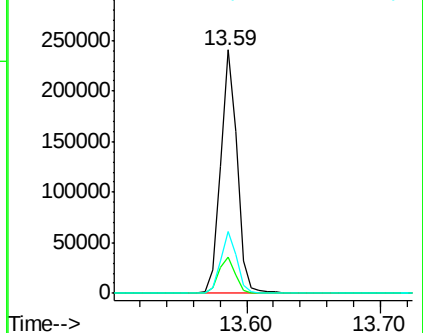

#78

Terphenyl-d14

Concen: 9.288 ng

RT: 12.54 min Scan# 1812

Delta R.T. -0.04 min

Lab File: BF097258.D

Acq: 2 Aug 2017 7:00


Tgt Ion:244 Resp: 95759

Ion Ratio Lower Upper

244 100

212 6.6 6.0 9.0



122 13.1 10.3 15.5

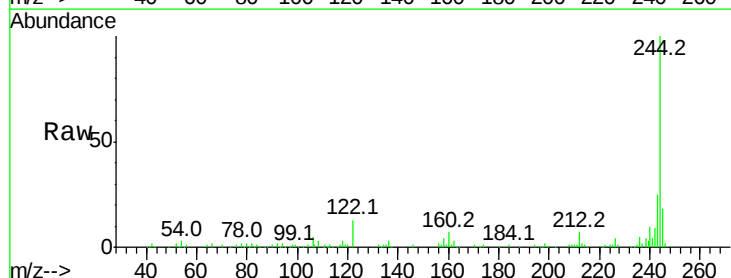


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

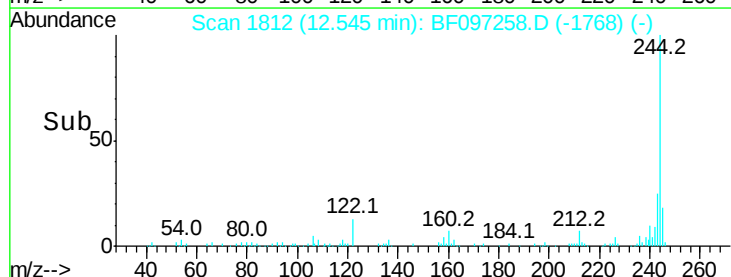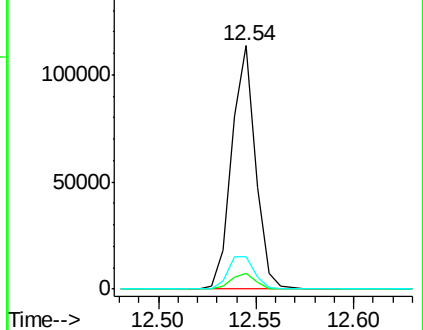


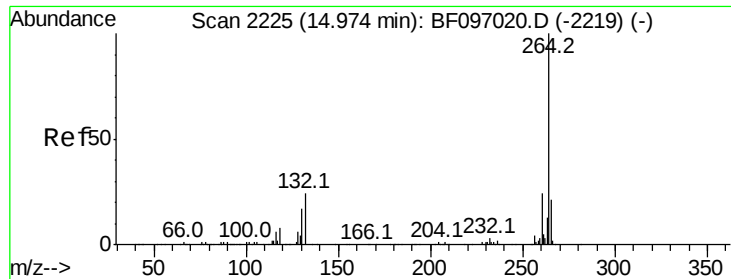

#86
Pervlene-d12
Concen: 20.000 ng
RT: 14.93 min Scan# 2218
Delta R.T. -0.04 min
Lab File: BF097258.D
Acq: 2 Aug 2017 7:00

Instrument :
BNA_F
ClientSampleId :
E2-HS7-ESW

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.5	29.3
265	22.0	17.2	25.8

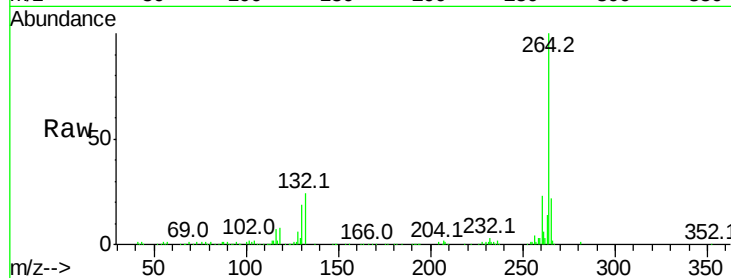

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

