

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
 Data File : BF097252.D
 Acq On : 2 Aug 2017 4:14
 Operator : SJ/JU
 Sample : I4471-16 2X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-BASE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.593	457	460	471	rBV	85269	126954	9.48%	0.721%
2	4.675	471	474	479	rVB	17437	19731	1.47%	0.112%
3	5.063	537	540	564	rBV	1120608	1327972	99.19%	7.547%
4	6.134	718	722	732	rBV	1227749	1338803	100.00%	7.608%
5	6.204	732	734	736	rVV	30906	31451	2.35%	0.179%
6	6.234	736	739	746	rVB	1302187	1282473	95.79%	7.288%
7	6.463	775	778	786	rBV	752434	673828	50.33%	3.829%
8	6.616	801	804	815	rBV	1011667	921682	68.84%	5.238%
9	7.028	871	874	889	rVB	801780	735891	54.97%	4.182%
10	7.745	992	996	999	rBV	977485	802060	59.91%	4.558%
11	8.463	1114	1118	1126	rVB	37040	36987	2.76%	0.210%
12	8.557	1130	1134	1139	rVB	25523	24588	1.84%	0.140%
13	8.822	1175	1179	1183	rBV	1206402	985655	73.62%	5.601%
14	9.086	1220	1224	1228	rBV3	13526	19485	1.46%	0.111%
15	9.157	1231	1236	1239	rBV2	20697	22959	1.71%	0.130%
16	9.222	1245	1247	1254	rVB	156972	137598	10.28%	0.782%
17	9.492	1289	1293	1296	rBV	717560	678653	50.69%	3.857%
18	9.522	1296	1298	1301	rVB	70283	53645	4.01%	0.305%
19	9.698	1324	1328	1332	rVB	34883	33340	2.49%	0.189%
20	9.922	1364	1366	1368	rVB	22029	15480	1.16%	0.088%
21	9.945	1368	1370	1374	rVB	22696	17995	1.34%	0.102%
22	10.033	1382	1385	1389	rBV	47220	44507	3.32%	0.253%
23	10.163	1403	1407	1410	rBV4	11990	18389	1.37%	0.105%
24	10.275	1423	1426	1437	rVB	462286	457585	34.18%	2.600%
25	10.416	1447	1450	1457	rVB	31787	37987	2.84%	0.216%
26	10.851	1521	1524	1528	rVB2	355657	314008	23.45%	1.784%
27	10.910	1528	1534	1538	rVB	137750	117231	8.76%	0.666%
28	10.963	1539	1543	1545	rBV	700977	584821	43.68%	3.324%
29	10.986	1545	1547	1551	rVV	423317	338891	25.31%	1.926%
30	11.039	1551	1556	1560	rVB	91377	85051	6.35%	0.483%
31	11.204	1579	1584	1592	rVB	40787	41360	3.09%	0.235%
32	11.369	1608	1612	1616	rVB2	31808	29341	2.19%	0.167%
33	11.463	1626	1628	1631	rBV	34533	29239	2.18%	0.166%
34	11.492	1631	1633	1636	rVV	47600	42963	3.21%	0.244%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
 Data File : BF097252.D
 Acq On : 2 Aug 2017 4:14
 Operator : SJ/JU
 Sample : I4471-16 2X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-BASE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	11.539	1639	1641	1644	rVV	21813	20455	1.53%	0.116%
36	11.574	1644	1647	1649	rVV	74094	67290	5.03%	0.382%
37	11.598	1649	1651	1657	rVB	24762	23801	1.78%	0.135%
38	11.757	1676	1678	1682	rVB	25666	23088	1.72%	0.131%
39	11.798	1682	1685	1689	rVB	17018	16673	1.25%	0.095%
40	12.010	1719	1721	1724	rBV	18990	19722	1.47%	0.112%
41	12.051	1724	1728	1730	rVV3	15177	22449	1.68%	0.128%
42	12.098	1734	1736	1744	rVB2	19982	24317	1.82%	0.138%
43	12.169	1744	1748	1752	rBV	551070	473243	35.35%	2.689%
44	12.316	1769	1773	1776	rBV	26153	24503	1.83%	0.139%
45	12.392	1781	1786	1790	rBV	533498	512114	38.25%	2.910%
46	12.445	1793	1795	1797	rVV2	19737	19259	1.44%	0.109%
47	12.468	1797	1799	1803	rVB	18027	16950	1.27%	0.096%
48	12.521	1803	1808	1809	rBV	29925	30125	2.25%	0.171%
49	12.545	1809	1812	1819	rVB	928799	828289	61.87%	4.707%
50	12.621	1819	1825	1828	rBV2	22513	34907	2.61%	0.198%
51	12.698	1835	1838	1839	rBV3	20509	16779	1.25%	0.095%
52	12.721	1839	1842	1847	rVB	55610	67977	5.08%	0.386%
53	12.792	1851	1854	1856	rVV	42099	38161	2.85%	0.217%
54	12.827	1856	1860	1867	rVB2	46069	54425	4.07%	0.309%
55	12.916	1873	1875	1878	rVB	21488	20689	1.55%	0.118%
56	12.951	1878	1881	1884	rBV	22065	23575	1.76%	0.134%
57	13.092	1903	1905	1908	rBV	29889	30588	2.28%	0.174%
58	13.239	1927	1930	1933	rVB	31825	29994	2.24%	0.170%
59	13.339	1943	1947	1949	rBV2	46253	48755	3.64%	0.277%
60	13.363	1949	1951	1953	rVV	40584	36065	2.69%	0.205%
61	13.392	1953	1956	1957	rVV	31025	32877	2.46%	0.187%
62	13.410	1957	1959	1962	rVB2	30577	29547	2.21%	0.168%
63	13.445	1962	1965	1967	rBV	34842	32739	2.45%	0.186%
64	13.492	1967	1973	1982	rVB7	33782	84724	6.33%	0.481%
65	13.586	1982	1989	1992	rBV2	785877	988442	73.83%	5.617%
66	13.610	1992	1993	1997	rVB	223144	159841	11.94%	0.908%
67	13.686	2002	2006	2009	rBV	45350	49457	3.69%	0.281%
68	13.786	2020	2023	2024	rBV3	17888	16647	1.24%	0.095%
69	13.821	2027	2029	2031	rVB	24822	20120	1.50%	0.114%
70	13.939	2046	2049	2051	rBV2	26636	28094	2.10%	0.160%
71	13.974	2053	2055	2059	rVV2	48578	49013	3.66%	0.279%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
 Data File : BF097252.D
 Acq On : 2 Aug 2017 4:14
 Operator : SJ/JU
 Sample : I4471-16 2X
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-BASE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	14.010	2059	2061	2065	rVB	24833	20195	1.51%	0.115%
73	14.068	2065	2071	2074	rBV6	22617	41991	3.14%	0.239%
74	14.121	2077	2080	2083	rVB3	27800	29564	2.21%	0.168%
75	14.198	2091	2093	2096	rBV4	9158	14167	1.06%	0.081%
76	14.292	2105	2109	2110	rBV3	15481	22106	1.65%	0.126%
77	14.380	2121	2124	2127	rVB	25500	26474	1.98%	0.150%
78	14.445	2132	2135	2138	rBV3	18197	20303	1.52%	0.115%
79	14.580	2154	2158	2169	rBV	233338	381958	28.53%	2.171%
80	14.668	2170	2173	2177	rVB2	56192	49603	3.71%	0.282%
81	14.715	2177	2181	2186	rBV5	40701	70274	5.25%	0.399%
82	14.827	2197	2200	2206	rVB	102103	117041	8.74%	0.665%
83	14.880	2206	2209	2212	rBV	153704	158862	11.87%	0.903%
84	14.933	2213	2218	2222	rBV	477685	550369	41.11%	3.128%
85	15.333	2283	2286	2289	rVB2	35524	42630	3.18%	0.242%
86	15.404	2294	2298	2309	rBV4	55130	142109	10.61%	0.808%
87	15.739	2350	2355	2358	rBV	29983	45378	3.39%	0.258%
88	15.839	2370	2372	2376	rVB5	14445	14910	1.11%	0.085%
89	16.145	2419	2424	2429	rVB2	54527	90932	6.79%	0.517%
90	16.209	2431	2435	2441	rVB3	32595	57587	4.30%	0.327%
91	16.298	2444	2450	2455	rBV10	14178	34537	2.58%	0.196%
92	16.409	2467	2469	2476	rVB8	12067	22054	1.65%	0.125%
93	16.504	2480	2485	2495	rVB	35714	85029	6.35%	0.483%
94	16.715	2517	2521	2524	rBV4	16865	21115	1.58%	0.120%
95	16.751	2525	2527	2534	rVB8	20050	34176	2.55%	0.194%
96	18.156	2762	2766	2769	rBV5	10516	19001	1.42%	0.108%
97	18.421	2809	2811	2814	rBV4	16945	21866	1.63%	0.124%
98	18.845	2879	2883	2884	rBV4	13500	17919	1.34%	0.102%


Sum of corrected areas: 17596447

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data File : BF097252.D
Acq On : 2 Aug 2017 4:14
Operator : SJ/JU
Sample : I4471-16 2X
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampled :
E2-L6-BASE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

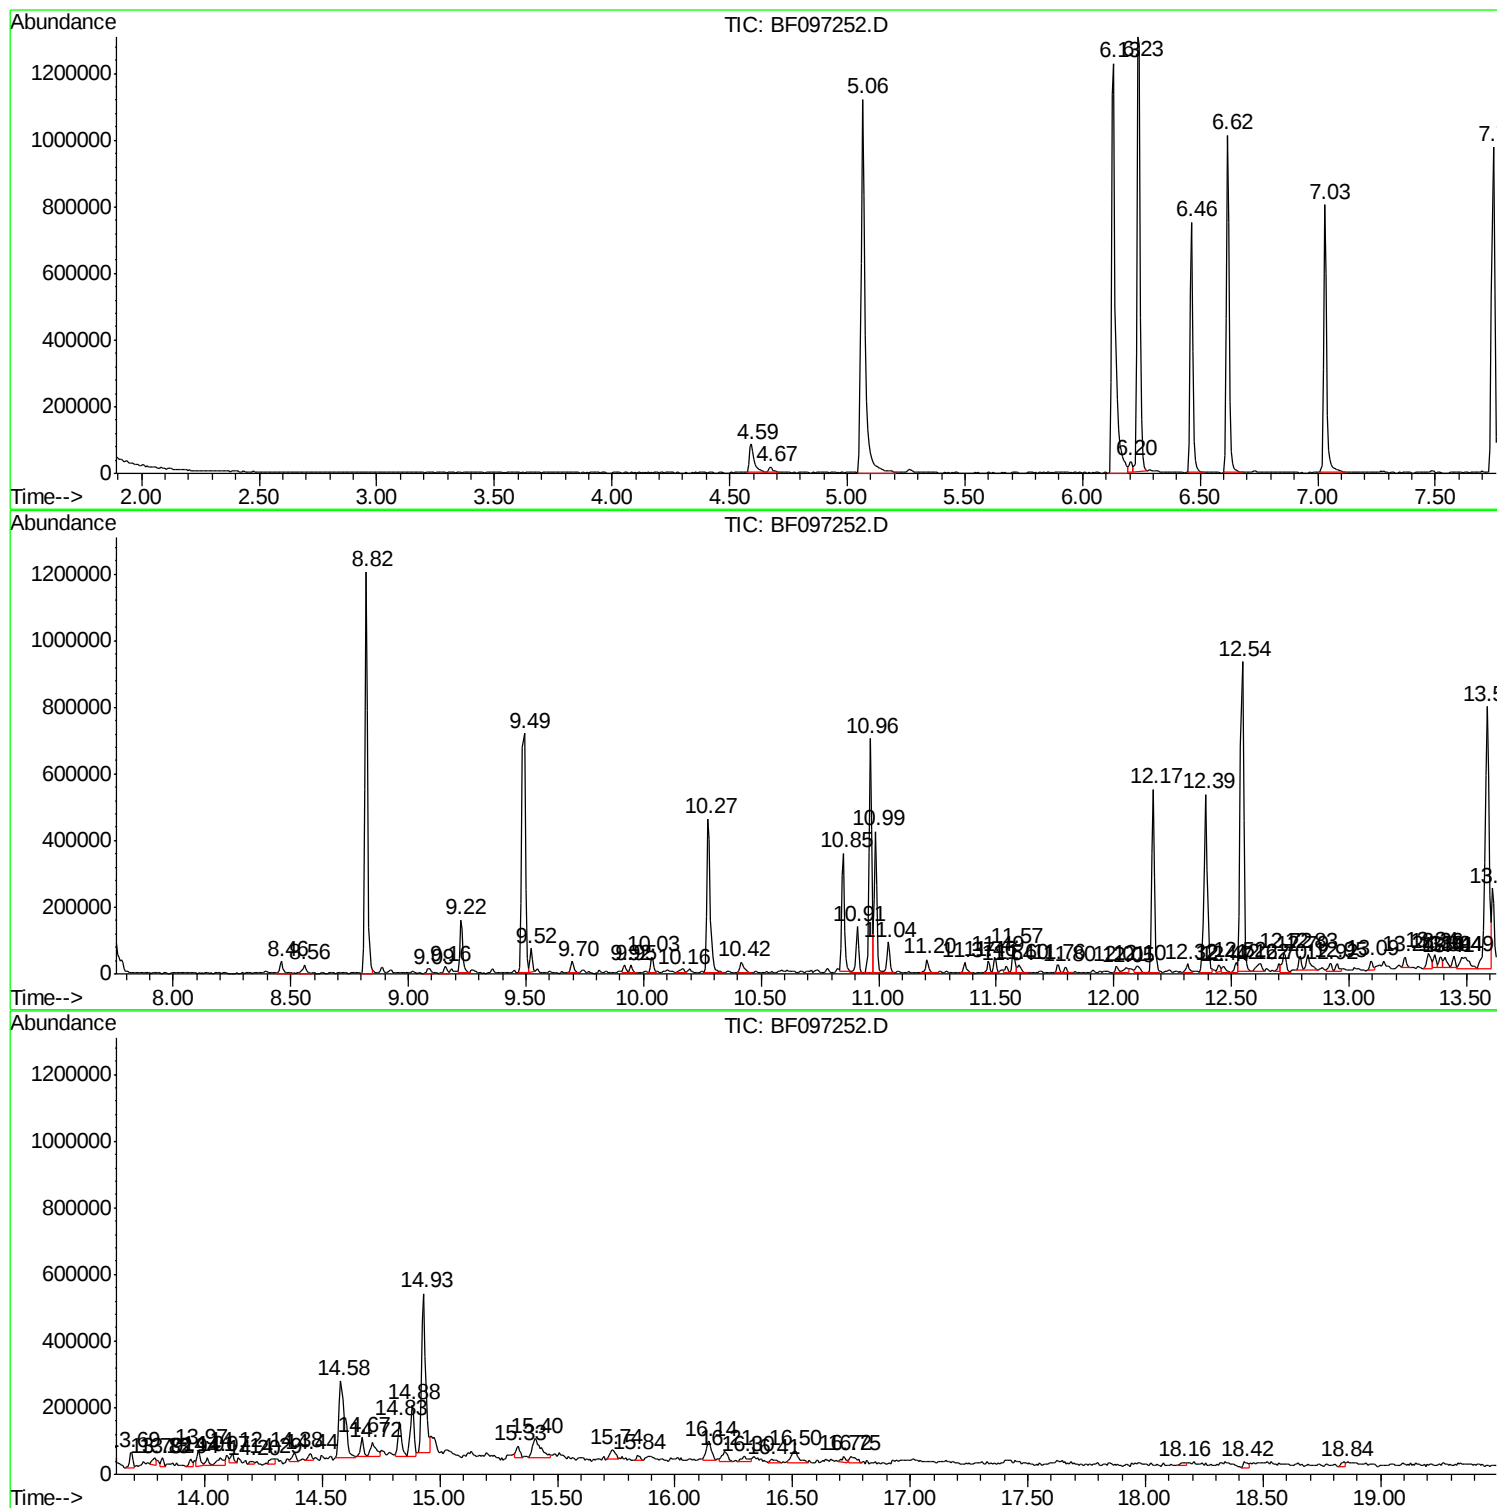

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data_File : BF097252.D
Acq_On : 2_Aug_2017. 4:144
Operator : SJ/JUU
Sample : I4471-16_2XX
Misc :
ALS_Vial : 28 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-L6-BASE

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
