

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
 Data File : BF097253.D
 Acq On : 2 Aug 2017 4:42
 Operator : SJ/JU
 Sample : I4471-17
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-WSW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.610	121	123	139	rBV2	86049	212409	7.23%	0.834%
2	4.604	458	462	471	rBV	177050	290699	9.89%	1.142%
3	4.675	471	474	479	rVV	45200	49163	1.67%	0.193%
4	5.069	537	541	559	rBV	2600277	2939305	100.00%	11.545%
5	6.140	718	723	732	rBV	2538991	2801413	95.31%	11.003%
6	6.204	732	734	737	rVV	385526	346997	11.81%	1.363%
7	6.240	737	740	747	rVB	2670664	2563264	87.21%	10.068%
8	6.463	775	778	782	rBV	827987	730771	24.86%	2.870%
9	6.622	800	805	812	rBV	1828602	1884624	64.12%	7.402%
10	6.675	812	814	821	rVB2	24771	39092	1.33%	0.154%
11	6.793	831	834	838	rBV2	32453	32250	1.10%	0.127%
12	7.034	871	875	878	rBV	1810943	1573125	53.52%	6.179%
13	7.087	881	884	888	rVB	39217	37252	1.27%	0.146%
14	7.181	898	900	906	rVB2	44279	58400	1.99%	0.229%
15	7.245	906	911	913	rVV4	39465	38289	1.30%	0.150%
16	7.269	913	915	920	rVB	68506	62437	2.12%	0.245%
17	7.387	928	935	938	rBV6	37522	52579	1.79%	0.207%
18	7.457	943	947	949	rVV3	20530	30276	1.03%	0.119%
19	7.492	949	953	955	rVV3	36955	40608	1.38%	0.159%
20	7.575	962	967	972	rVB2	64626	112466	3.83%	0.442%
21	7.657	978	981	983	rBV	217558	187325	6.37%	0.736%
22	7.675	983	984	987	rVB	40640	33002	1.12%	0.130%
23	7.745	992	996	999	rBV	1110496	1026343	34.92%	4.031%
24	7.834	1008	1011	1016	rVB2	66718	74354	2.53%	0.292%
25	7.939	1021	1029	1032	rBV5	53790	94236	3.21%	0.370%
26	8.010	1037	1041	1044	rBV3	42065	61853	2.10%	0.243%
27	8.039	1044	1046	1052	rVB5	40981	49272	1.68%	0.194%
28	8.134	1060	1062	1068	rVB3	153796	168897	5.75%	0.663%
29	8.192	1068	1072	1074	rBV	118943	141016	4.80%	0.554%
30	8.257	1081	1083	1086	rVB3	31622	30997	1.05%	0.122%
31	8.363	1096	1101	1104	rBV2	127017	173553	5.90%	0.682%
32	8.457	1114	1117	1120	rVB	194087	176759	6.01%	0.694%
33	8.498	1120	1124	1127	rBV	226307	233215	7.93%	0.916%
34	8.557	1131	1134	1136	rBV	139314	130538	4.44%	0.513%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data File : BF097253.D
Acq On : 2 Aug 2017 4:42
Operator : SJ/JU
Sample : I4471-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-L6-WSW

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.610	1141	1143	1146	rBV3	50752	58878	2.00%	0.231%
36	8.681	1151	1155	1159	rBV3	46413	76408	2.60%	0.300%
37	8.722	1159	1162	1166	rBV4	91037	171918	5.85%	0.675%
38	8.787	1171	1173	1176	rVB	129158	119401	4.06%	0.469%
39	8.822	1176	1179	1183	rBV	1826855	1776831	60.45%	6.979%
40	9.163	1233	1237	1240	rBV2	216909	288152	9.80%	1.132%
41	9.228	1245	1248	1253	rVB	598156	598955	20.38%	2.353%
42	9.316	1261	1263	1266	rVB3	105144	87536	2.98%	0.344%
43	9.492	1290	1293	1297	rVB2	710509	686844	23.37%	2.698%
44	9.945	1368	1370	1373	rVB2	205858	185757	6.32%	0.730%
45	10.281	1424	1427	1431	rBV	825757	783550	26.66%	3.078%
46	10.969	1541	1544	1547	rBV	576385	527777	17.96%	2.073%
47	12.045	1725	1727	1731	rVB	380050	389261	13.24%	1.529%
48	12.551	1810	1813	1816	rVB	1033201	983280	33.45%	3.862%
49	13.098	1904	1906	1908	rBV2	183559	171127	5.82%	0.672%
50	13.598	1988	1991	1994	rVB	534941	491502	16.72%	1.931%
51	14.480	2138	2141	2148	rVB4	551808	824757	28.06%	3.239%
52	14.557	2151	2154	2159	rVB3	349924	448778	15.27%	1.763%
53	14.792	2192	2194	2197	rVB2	419084	312121	10.62%	1.226%


Sum of corrected areas: 25459612

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
Data File : BF097253.D
Acq On : 2 Aug 2017 4:42
Operator : SJ/JU
Sample : I4471-17
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-L6-WSW

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

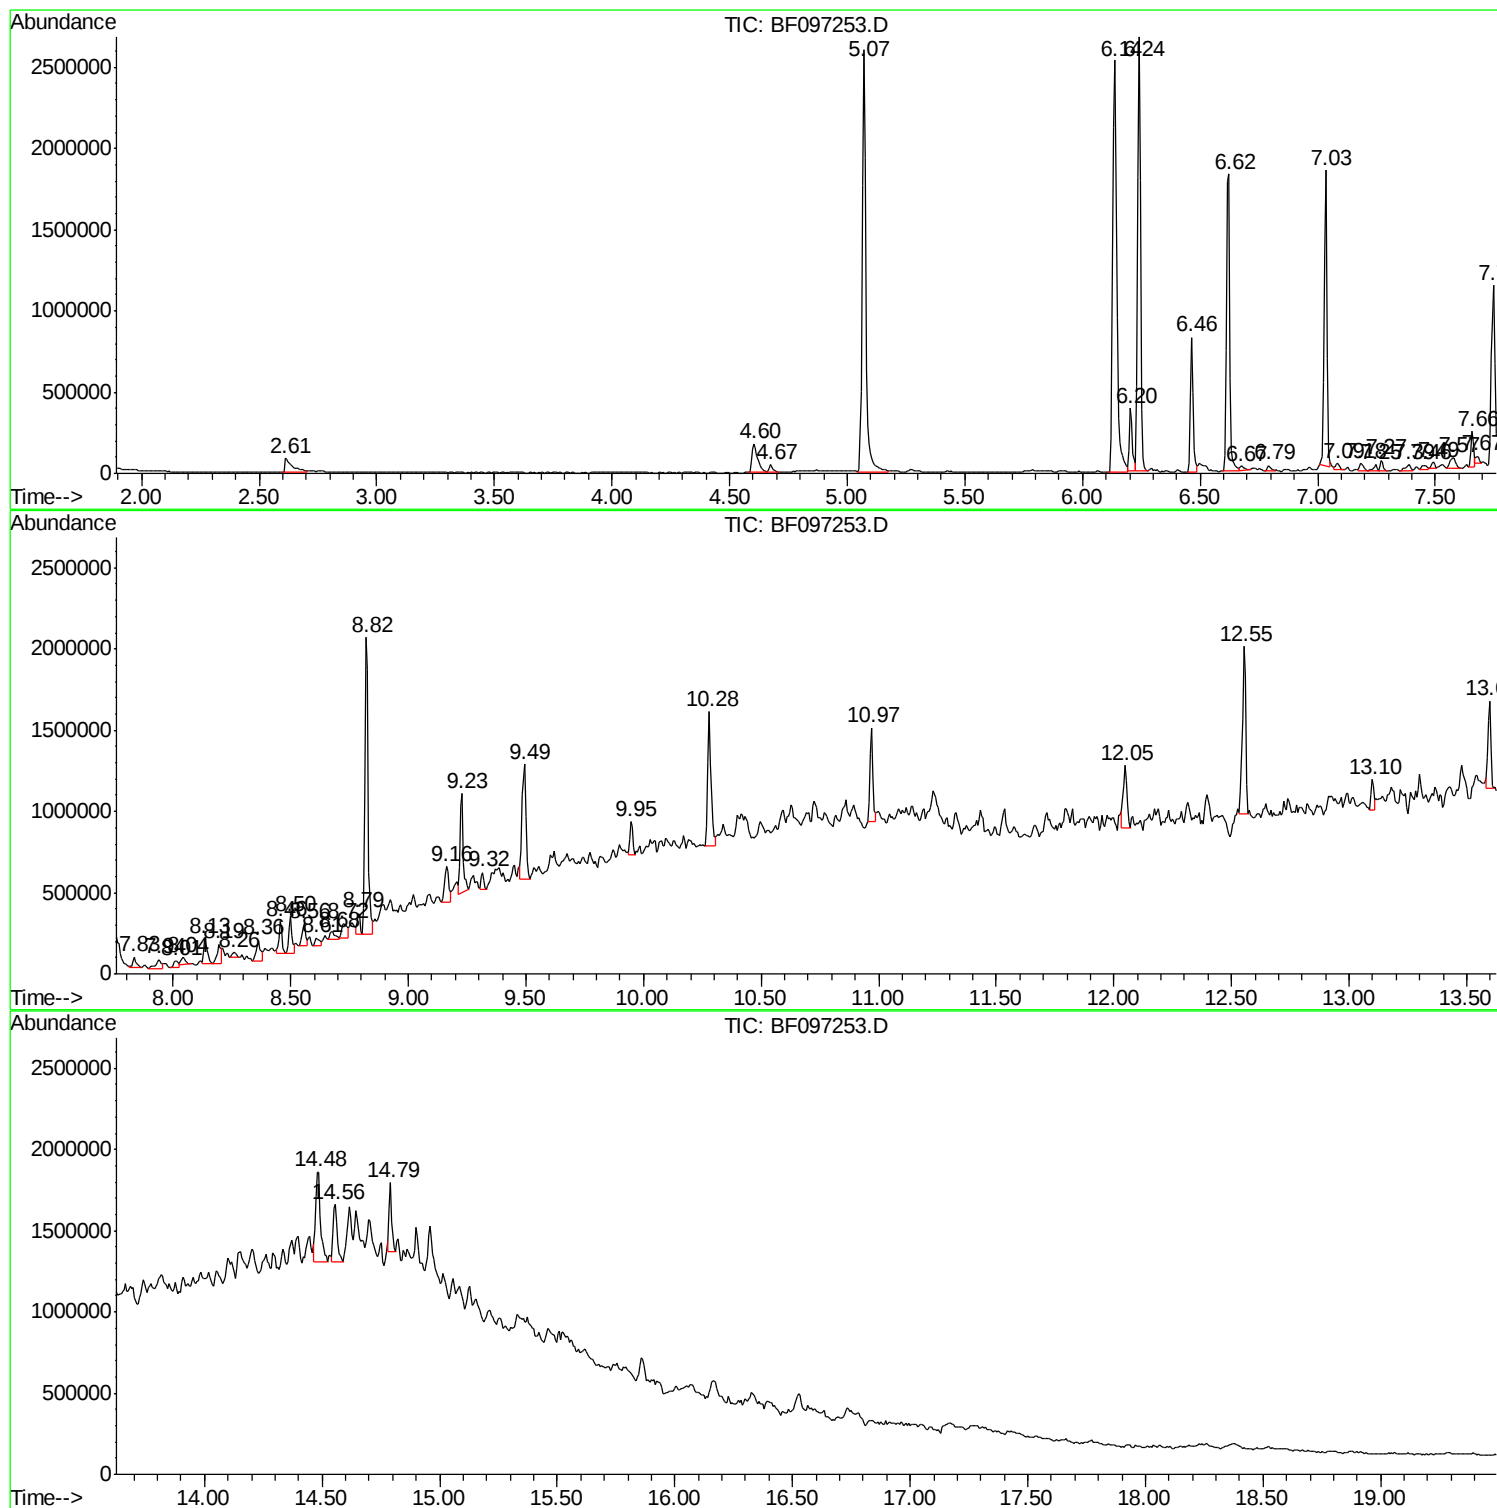

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data_File : BF097253.D
Acq_On : 2_Aug_2017. 4:422
Operator : SJ/JUU
Sample : I4471-177
Misc :
ALS_Vial : 29 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-L6-WSW

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
