

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
 Data File : BF097254.D
 Acq On : 2 Aug 2017 5:09
 Operator : SJ/JU
 Sample : I4471-18 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-NSW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.881	164	169	175	rBV5	4408	9152	1.35%	0.126%
2	4.593	456	460	468	rBV	26374	41491	6.13%	0.573%
3	4.675	471	474	483	rVB4	5926	10587	1.56%	0.146%
4	5.069	538	541	556	rBV	358308	470585	69.53%	6.495%
5	6.134	719	722	737	rVB	382507	447204	66.07%	6.172%
6	6.240	737	740	747	rBV	495456	476569	70.41%	6.578%
7	6.463	775	778	789	rVB	619256	527066	77.87%	7.275%
8	6.616	801	804	815	rBV	343085	323126	47.74%	4.460%
9	7.028	872	874	886	rBV	236493	266455	39.37%	3.678%
10	7.745	993	996	1006	rBV	830235	676849	100.00%	9.342%
11	8.822	1176	1179	1186	rBV	356176	286323	42.30%	3.952%
12	9.222	1245	1247	1252	rVB	42578	42478	6.28%	0.586%
13	9.492	1289	1293	1297	rBV	635412	557522	82.37%	7.695%
14	9.522	1297	1298	1302	rVB2	14862	9807	1.45%	0.135%
15	9.922	1360	1366	1368	rBV	24176	23018	3.40%	0.318%
16	10.039	1383	1386	1391	rVB	12587	12753	1.88%	0.176%
17	10.280	1424	1427	1433	rBV	180322	173972	25.70%	2.401%
18	10.416	1447	1450	1455	rBV2	8134	9562	1.41%	0.132%
19	10.963	1539	1543	1546	rBV	528049	472855	69.86%	6.526%
20	10.986	1546	1547	1551	rVV	123442	85917	12.69%	1.186%
21	11.039	1553	1556	1560	rVB	25815	23134	3.42%	0.319%
22	11.469	1626	1629	1631	rBV	27763	22988	3.40%	0.317%
23	11.492	1631	1633	1637	rVB	30970	27641	4.08%	0.382%
24	11.545	1637	1642	1644	rBV2	10617	12011	1.77%	0.166%
25	11.574	1644	1647	1649	rVV	37593	37185	5.49%	0.513%
26	11.598	1649	1651	1658	rVB	23459	20867	3.08%	0.288%
27	11.763	1674	1679	1683	rBV	11271	11735	1.73%	0.162%
28	11.910	1699	1704	1707	rBV3	9968	9299	1.37%	0.128%
29	12.016	1716	1722	1724	rBV	18851	19833	2.93%	0.274%
30	12.051	1724	1728	1730	rVB4	9680	10432	1.54%	0.144%
31	12.110	1735	1738	1741	rVV3	8125	9832	1.45%	0.136%
32	12.169	1745	1748	1753	rVB	140706	113562	16.78%	1.567%
33	12.392	1782	1786	1790	rBV	144639	140857	20.81%	1.944%
34	12.545	1809	1812	1815	rBV	244804	201330	29.75%	2.779%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
 Data File : BF097254.D
 Acq On : 2 Aug 2017 5:09
 Operator : SJ/JU
 Sample : I4471-18 5X
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-NSW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.616	1820	1824	1828	rBV2	12213	15379	2.27%	0.212%
36	12.704	1836	1839	1840	rBV	10230	9498	1.40%	0.131%
37	12.727	1840	1843	1847	rVB	19829	21281	3.14%	0.294%
38	12.792	1850	1854	1858	rBV3	28787	33137	4.90%	0.457%
39	12.827	1858	1860	1863	rBV	18108	15448	2.28%	0.213%
40	12.921	1873	1876	1878	rBV	13352	11730	1.73%	0.162%
41	12.951	1878	1881	1884	rVB	12018	10711	1.58%	0.148%
42	13.092	1902	1905	1909	rBV4	7516	9067	1.34%	0.125%
43	13.139	1909	1913	1918	rBV6	7940	15183	2.24%	0.210%
44	13.345	1943	1948	1949	rBV4	12568	14111	2.08%	0.195%
45	13.363	1949	1951	1954	rVB4	11882	12445	1.84%	0.172%
46	13.392	1954	1956	1957	rBV2	12535	9035	1.33%	0.125%
47	13.410	1957	1959	1963	rVB5	9339	9023	1.33%	0.125%
48	13.468	1966	1969	1977	rVV5	25732	35963	5.31%	0.496%
49	13.586	1984	1989	1992	rBV	624347	629219	92.96%	8.685%
50	13.610	1992	1993	1998	rVB	55826	51779	7.65%	0.715%
51	13.698	2004	2008	2009	rBV3	13537	15696	2.32%	0.217%
52	13.974	2052	2055	2056	rBV3	9922	11213	1.66%	0.155%
53	14.010	2058	2061	2065	rVB4	16523	18036	2.66%	0.249%
54	14.068	2065	2071	2072	rBV6	15384	26867	3.97%	0.371%
55	14.086	2072	2074	2075	rBV	22700	13906	2.05%	0.192%
56	14.457	2135	2137	2139	rBV3	15494	15706	2.32%	0.217%
57	14.580	2155	2158	2162	rBV	40744	50382	7.44%	0.695%
58	14.668	2170	2173	2177	rBV2	23749	26776	3.96%	0.370%
59	14.833	2198	2201	2206	rBV	24391	28225	4.17%	0.390%
60	14.880	2206	2209	2213	rBV	34706	46098	6.81%	0.636%
61	14.933	2214	2218	2224	rBV	393720	440358	65.06%	6.078%
62	15.327	2282	2285	2290	rBV4	21480	32899	4.86%	0.454%
63	15.733	2351	2354	2360	rVB2	18864	32073	4.74%	0.443%


Sum of corrected areas: 7245241

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data File : BF097254.D
Acq On : 2 Aug 2017 5:09
Operator : SJ/JU
Sample : I4471-18 5X
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-L6-NSW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

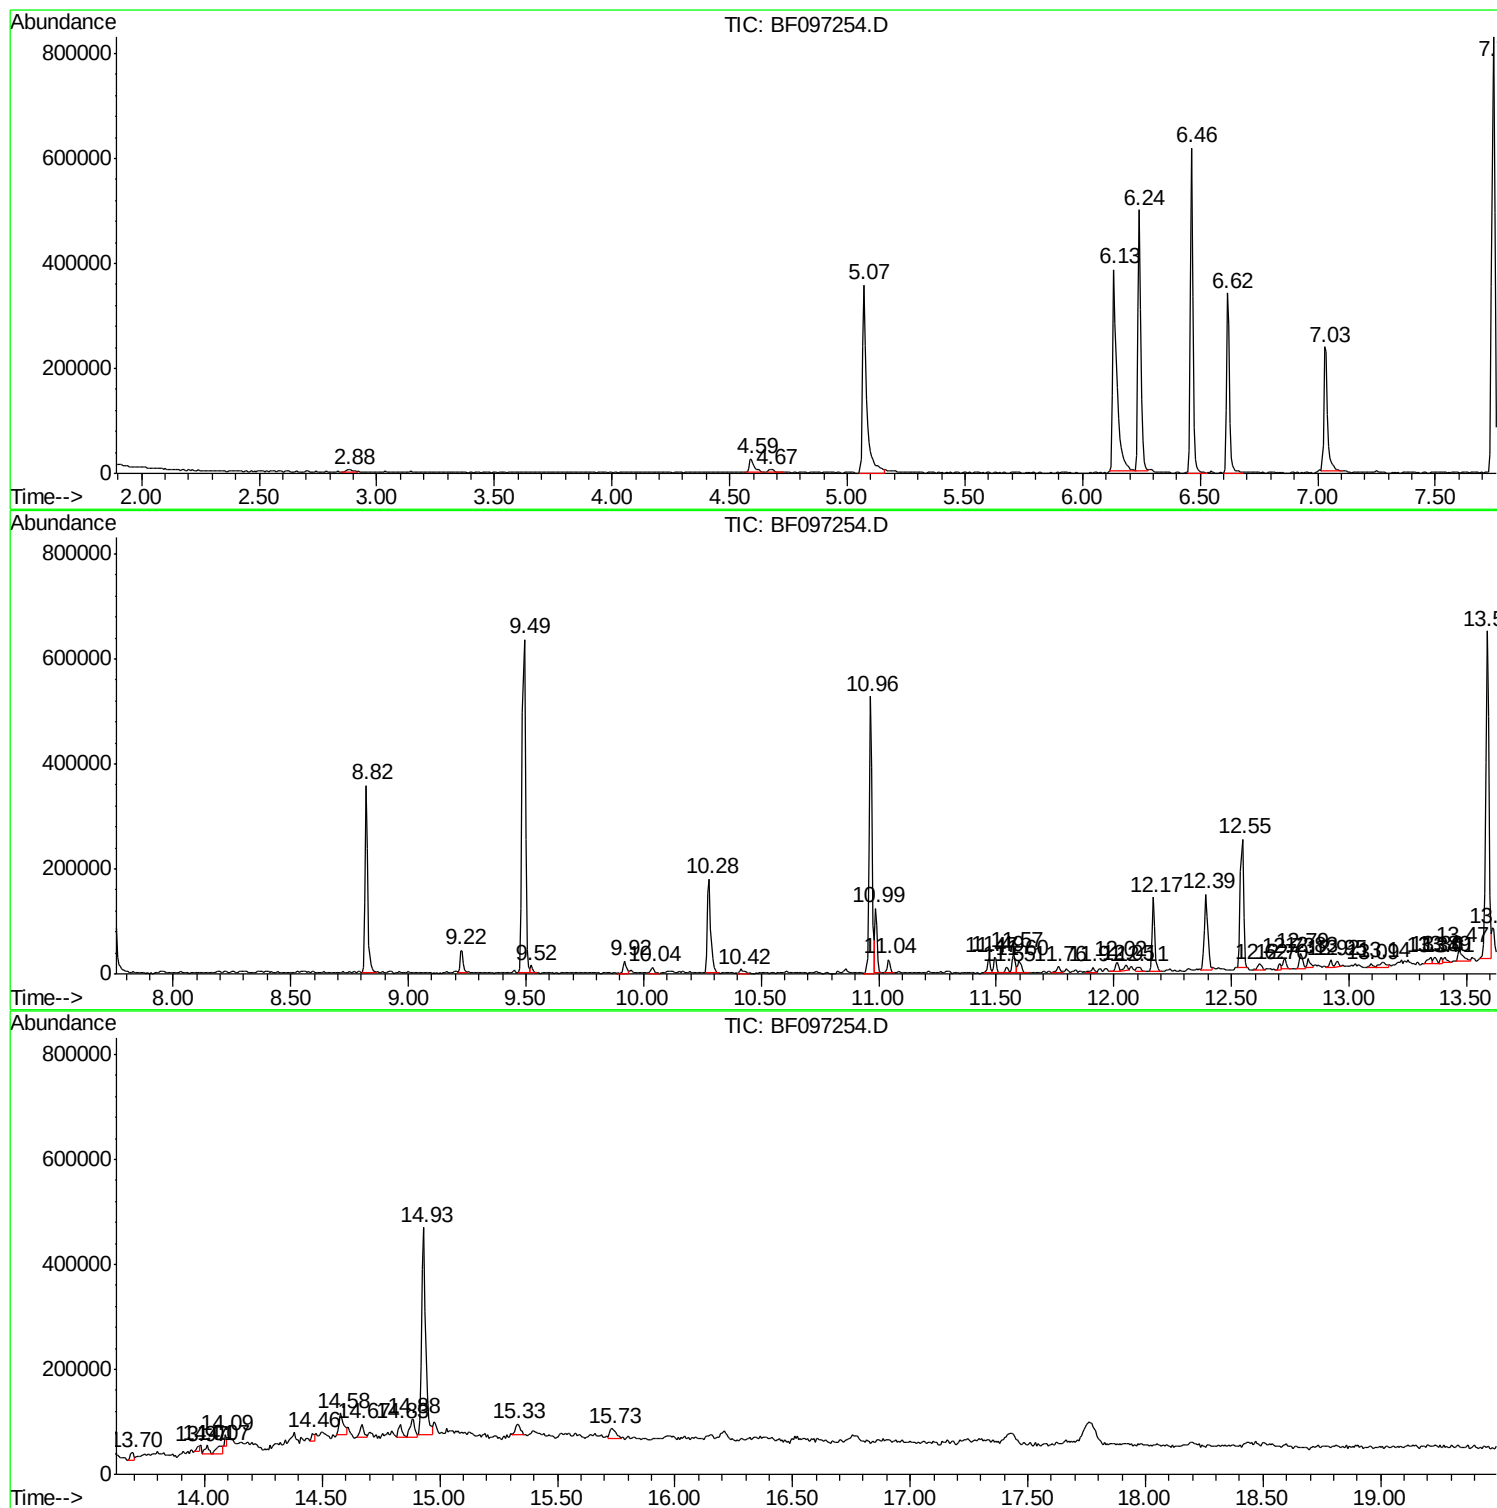

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data_File : BF097254.D
Acq_On : 2_Aug_2017. 5:099
Operator : SJ/JUU
Sample : I4471-18_5XX
Misc :
ALS_Vial : 30 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-L6-NSW

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	Internal Standard
				#	RT Resp Conc

No Library Search Compounds Detected
