

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
 Data File : BF097255.D
 Acq On : 2 Aug 2017 5:37
 Operator : SJ/JU
 Sample : I4471-22 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-ESW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.063	537	540	558	rBV	1181613	1502015	15.32%	1.140%
2	6.134	718	722	733	rBV	1289818	1342538	13.69%	1.019%
3	6.240	736	740	746	rVB	1336437	1280590	13.06%	0.972%
4	6.463	775	778	783	rBV	753199	640700	6.53%	0.486%
5	6.616	801	804	814	rVB	998305	970322	9.89%	0.736%
6	7.028	872	874	886	rVB	745363	735471	7.50%	0.558%
7	7.745	993	996	998	rBV	1010832	859830	8.77%	0.653%
8	7.769	998	1000	1004	rVV	701094	595409	6.07%	0.452%
9	8.457	1112	1117	1121	rVB	525449	453285	4.62%	0.344%
10	8.557	1129	1134	1138	rBV	580453	506891	5.17%	0.385%
11	8.822	1176	1179	1185	rVB	1114049	967478	9.87%	0.734%
12	9.016	1206	1212	1219	rVB	267439	355179	3.62%	0.270%
13	9.081	1219	1223	1228	rBV	371617	516831	5.27%	0.392%
14	9.157	1233	1236	1238	rVV	699971	661415	6.74%	0.502%
15	9.181	1238	1240	1245	rVV	413778	391152	3.99%	0.297%
16	9.228	1245	1248	1250	rVV	298133	306217	3.12%	0.232%
17	9.275	1253	1256	1261	rVB	338557	396646	4.04%	0.301%
18	9.351	1264	1269	1272	rBV2	357048	330253	3.37%	0.251%
19	9.492	1288	1293	1295	rVV2	755926	841163	8.58%	0.638%
20	9.528	1295	1299	1303	rVV	1887186	1873634	19.11%	1.422%
21	9.598	1308	1311	1316	rVV	210961	309478	3.16%	0.235%
22	9.645	1316	1319	1322	rVV2	345215	365811	3.73%	0.278%
23	9.698	1322	1328	1332	rVV	1097490	1095139	11.17%	0.831%
24	9.739	1332	1335	1338	rVV	335302	298061	3.04%	0.226%
25	10.039	1382	1386	1388	rBV	1857509	1596085	16.28%	1.211%
26	10.104	1392	1397	1398	rBV2	406483	497889	5.08%	0.378%
27	10.192	1410	1412	1418	rVB2	469175	527482	5.38%	0.400%
28	10.281	1418	1427	1430	rBV2	900993	1111230	11.33%	0.843%
29	10.410	1445	1449	1452	rBV4	221582	340288	3.47%	0.258%
30	10.580	1471	1478	1481	rVV3	504749	828484	8.45%	0.629%
31	10.610	1481	1483	1486	rVV	418276	409417	4.17%	0.311%
32	10.733	1502	1504	1506	rVV2	313761	326372	3.33%	0.248%
33	10.786	1510	1513	1517	rVV	526188	564888	5.76%	0.429%
34	10.828	1517	1520	1523	rVV	463948	507318	5.17%	0.385%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
 Data File : BF097255.D
 Acq On : 2 Aug 2017 5:37
 Operator : SJ/JU
 Sample : I4471-22 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-ESW

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.863	1523	1526	1529	rVV	1047891	998212	10.18%	0.758%
36	11.022	1541	1553	1555	rBV	4476331	9566843	97.56%	7.261%
37	11.063	1555	1560	1562	rVV	2940234	3318540	33.84%	2.519%
38	11.086	1562	1564	1567	rVV2	342556	357612	3.65%	0.271%
39	11.210	1578	1585	1587	rVV2	892187	1024828	10.45%	0.778%
40	11.263	1592	1594	1597	rVV	501641	473562	4.83%	0.359%
41	11.292	1597	1599	1606	rVB3	339488	533770	5.44%	0.405%
42	11.475	1625	1630	1632	rVV	1802799	1967600	20.06%	1.493%
43	11.504	1632	1635	1638	rVV	2183337	2092143	21.33%	1.588%
44	11.551	1638	1643	1646	rVV	1024623	1064524	10.86%	0.808%
45	11.586	1646	1649	1651	rVV	2605895	2918102	29.76%	2.215%
46	11.610	1651	1653	1656	rVV	1552472	1174269	11.97%	0.891%
47	11.692	1663	1667	1672	rVV3	194212	354481	3.61%	0.269%
48	11.769	1677	1680	1683	rVV	1501563	1383142	14.10%	1.050%
49	11.810	1683	1687	1690	rVV	722376	820662	8.37%	0.623%
50	11.916	1699	1705	1707	rBV	562653	638442	6.51%	0.485%
51	11.945	1707	1710	1712	rVV	426717	386603	3.94%	0.293%
52	12.022	1719	1723	1726	rBV	916954	1164091	11.87%	0.883%
53	12.057	1726	1729	1732	rVV2	588716	850585	8.67%	0.646%
54	12.127	1736	1741	1745	rVB3	641445	1061097	10.82%	0.805%
55	12.210	1745	1755	1757	rBV	4000490	9214635	93.96%	6.993%
56	12.251	1760	1762	1768	rVB4	393961	516903	5.27%	0.392%
57	12.327	1772	1775	1781	rBV3	590557	738159	7.53%	0.560%
58	12.439	1783	1794	1796	rVV3	3895274	9806502	100.00%	7.443%
59	12.463	1796	1798	1803	rVB2	593496	723245	7.38%	0.549%
60	12.527	1806	1809	1811	rBV	632615	628162	6.41%	0.477%
61	12.557	1811	1814	1820	rVB2	864777	1481002	15.10%	1.124%
62	12.633	1820	1827	1830	rBV2	936881	1590080	16.21%	1.207%
63	12.739	1838	1845	1848	rVB	1530587	2630178	26.82%	1.996%
64	12.804	1853	1856	1859	rBV	1139631	1116500	11.39%	0.847%
65	12.845	1859	1863	1869	rVV2	1264908	1674187	17.07%	1.271%
66	12.933	1875	1878	1880	rVB	834151	721399	7.36%	0.547%
67	12.963	1880	1883	1886	rBV	962310	861543	8.79%	0.654%
68	13.051	1895	1898	1902	rVB	302118	319453	3.26%	0.242%
69	13.157	1910	1916	1918	rBV2	319170	479890	4.89%	0.364%
70	13.251	1929	1932	1935	rVV	707954	790720	8.06%	0.600%
71	13.351	1944	1949	1951	rBV2	838778	1146326	11.69%	0.870%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080117\
 Data File : BF097255.D
 Acq On : 2 Aug 2017 5:37
 Operator : SJ/JU
 Sample : I4471-22 2X
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 E2-L6-ESW

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.374	1951	1953	1956	rVV	1150895	1274635	13.00%	0.967%
73	13.404	1956	1958	1964	rVV3	1077520	1377126	14.04%	1.045%
74	13.469	1964	1969	1973	rVV	662272	820663	8.37%	0.623%
75	13.610	1985	1993	1995	rBV2	2774318	5718703	58.32%	4.340%
76	13.651	1996	2000	2005	rVB	2906620	4270036	43.54%	3.241%
77	13.716	2005	2011	2016	rBV	1149704	1249089	12.74%	0.948%
78	13.951	2048	2051	2053	rVV2	444375	439375	4.48%	0.333%
79	13.992	2053	2058	2061	rVV	1179175	1459708	14.89%	1.108%
80	14.021	2061	2063	2066	rVV	685059	623763	6.36%	0.473%
81	14.086	2067	2074	2076	rVV3	504068	1102089	11.24%	0.836%
82	14.110	2076	2078	2080	rVV	582771	640949	6.54%	0.486%
83	14.133	2080	2082	2085	rVV	676775	612311	6.24%	0.465%
84	14.180	2088	2090	2096	rVB2	452733	446180	4.55%	0.339%
85	14.310	2107	2112	2119	rVV5	339342	620397	6.33%	0.471%
86	14.463	2135	2138	2142	rBV	411448	413346	4.22%	0.314%
87	14.616	2156	2164	2166	rBV	2202021	4739734	48.33%	3.597%
88	14.692	2174	2177	2180	rVB	774853	712505	7.27%	0.541%
89	14.863	2200	2206	2210	rBV	1536963	2404543	24.52%	1.825%
90	14.921	2210	2216	2219	rVV	2082171	3194042	32.57%	2.424%
91	14.957	2219	2222	2224	rVV	336341	341296	3.48%	0.259%
92	14.986	2224	2227	2232	rVB2	998111	1130970	11.53%	0.858%
93	16.186	2422	2431	2434	rBV	959300	1934793	19.73%	1.468%
94	16.304	2446	2451	2455	rBV	262223	449409	4.58%	0.341%
95	16.357	2455	2460	2465	rVB2	195928	324277	3.31%	0.246%
96	16.551	2484	2493	2500	rVB	935747	2092187	21.33%	1.588%
97	16.733	2517	2524	2535	rVB	343241	777672	7.93%	0.590%
98	18.368	2792	2802	2813	rBV3	235926	761901	7.77%	0.578%
99	18.527	2822	2829	2835	rBV	124485	385175	3.93%	0.292%
100	19.386	2971	2975	2989	rVB5	169288	552878	5.64%	0.420%


Sum of corrected areas: 131762705

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data File : BF097255.D
Acq On : 2 Aug 2017 5:37
Operator : SJ/JU
Sample : I4471-22 2X
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
E2-L6-ESW

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

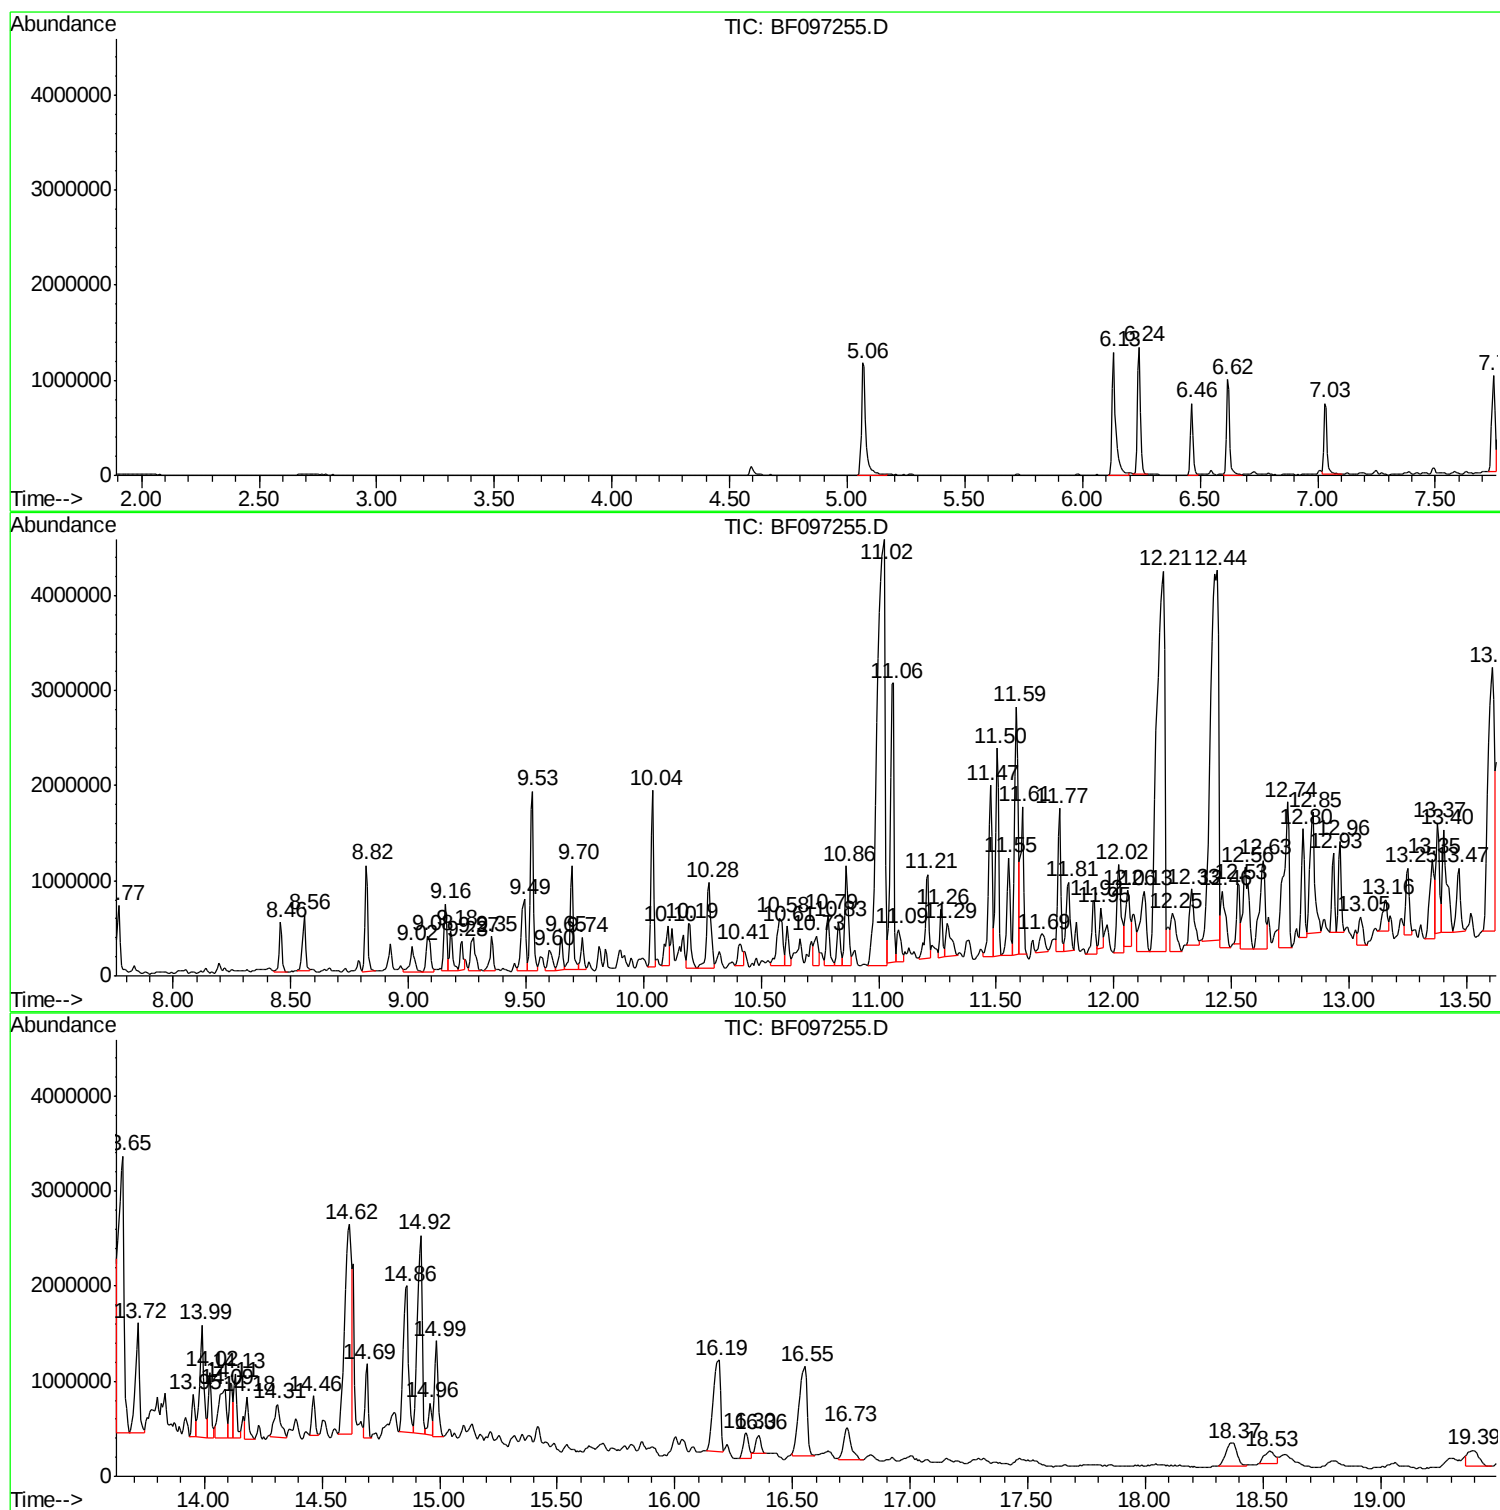

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF080117\
Data_File : BF097255.D
Acq_On : 2_Aug_2017. 5:377
Operator : SJ/JUU
Sample : I4471-22_2XX
Misc :
ALS_Vial : 31 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
E2-L6-ESW

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.MM
Quant_Title : ASP. BNA. STANDARDS. FOR. 5. POINT. CALIBRATION

TIC_Library : C:\DATABASE\NIST11.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
