


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080117\
 Data File : BF097248.D
 Acq On : 2 Aug 2017 00:18
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072517.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Aug 02 11:39:11 2017

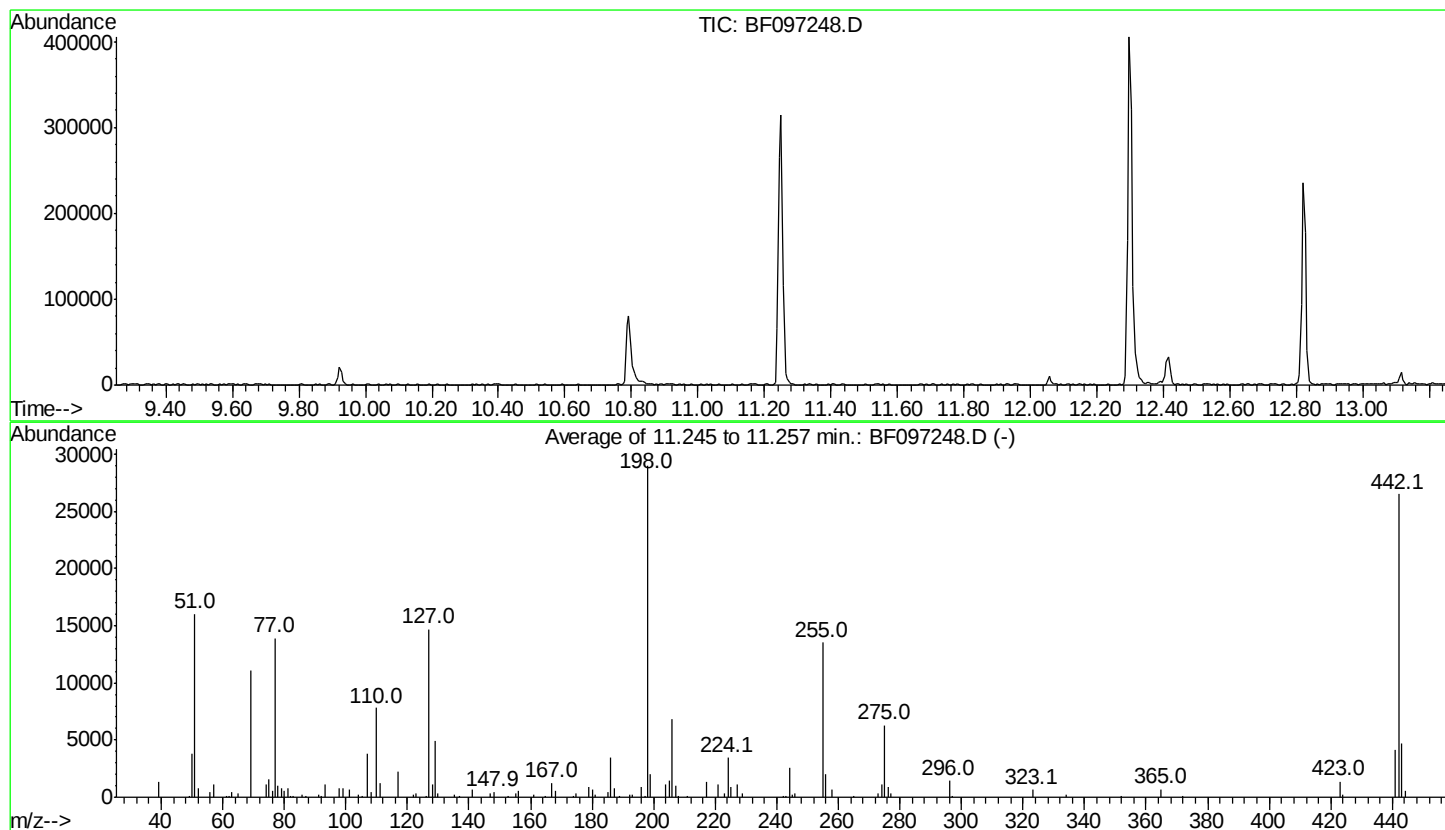

AutoFind: Scans 1591, 1592, 1593; Background Corrected with Scan 1586

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	55.3	16027	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.2	11062	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	14716	PASS
197	198	0.00	2	0.4	115	PASS
198	198	100	100	100.0	28991	PASS
199	198	5	9	6.8	1975	PASS
275	198	10	60	21.7	6291	PASS
365	198	1	100	2.4	695	PASS
441	442	0.01	24	15.8	4189	PASS
442	198	50	100	91.3	26482	PASS
443	442	15	24	17.8	4717	PASS