

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080119\
 Data File : BF115910.D
 Acq On : 1 Aug 2019 17:02
 Operator : HP/JU
 Sample : K4079-01
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TANK-4

Quant Time: Aug 02 04:59:51 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jul 31 15:31:51 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.85	152	132830	20.00	ng	0.00
21) Naphthalene-d8	8.13	136	489961	20.00	ng	0.00
39) Acenaphthene-d10	9.89	164	249578	20.00	ng	0.00
64) Phenanthrene-d10	11.38	188	379260	20.00	ng	0.00
76) Chrysene-d12	14.02	240	273455	20.00	ng	0.00
87) Perylene-d12	15.49	264	331860	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.47	112	343834	43.33	ng	0.00
7) Phenol-d6	6.48	99	261313	26.10	ng	0.00
23) Nitrobenzene-d5	7.42	82	838646	98.80	ng	0.00
42) 2,4,6-Tribromophenol	10.69	330	223240	92.26	ng	0.00
45) 2-Fluorobiphenyl	9.22	172	1386006	104.02	ng	0.00
79) Terphenyl-d14	12.96	244	1095073	84.38	ng	0.00
Target Compounds						
4) n-Nitrosodimethylamine	3.40	42	18026	4.079	ng	Qvalue
10) Phenol	6.49	94	42779	3.629	ng	# 1
19) n-Nitroso-di-n-propylamine	7.42	70	113987	18.375	ng	# 93
25) Isophorone	7.42	82	838634	51.670	ng	# 79
50) Dimethylphthalate	9.60	163	110129	6.481	ng	# 66
57) 2,4-Dinitrotoluene	9.89	165	32887	6.689	ng	# 100
67) 4-Bromophenyl-phenylether	10.69	248	13429	3.308	ng	# 26
						# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080119\
Data File : BF115910.D
Acq On : 1 Aug 2019 17:02
Operator : HP/JU
Sample : K4079-01
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TANK-4

Quant Time: Aug 02 04:59:51 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

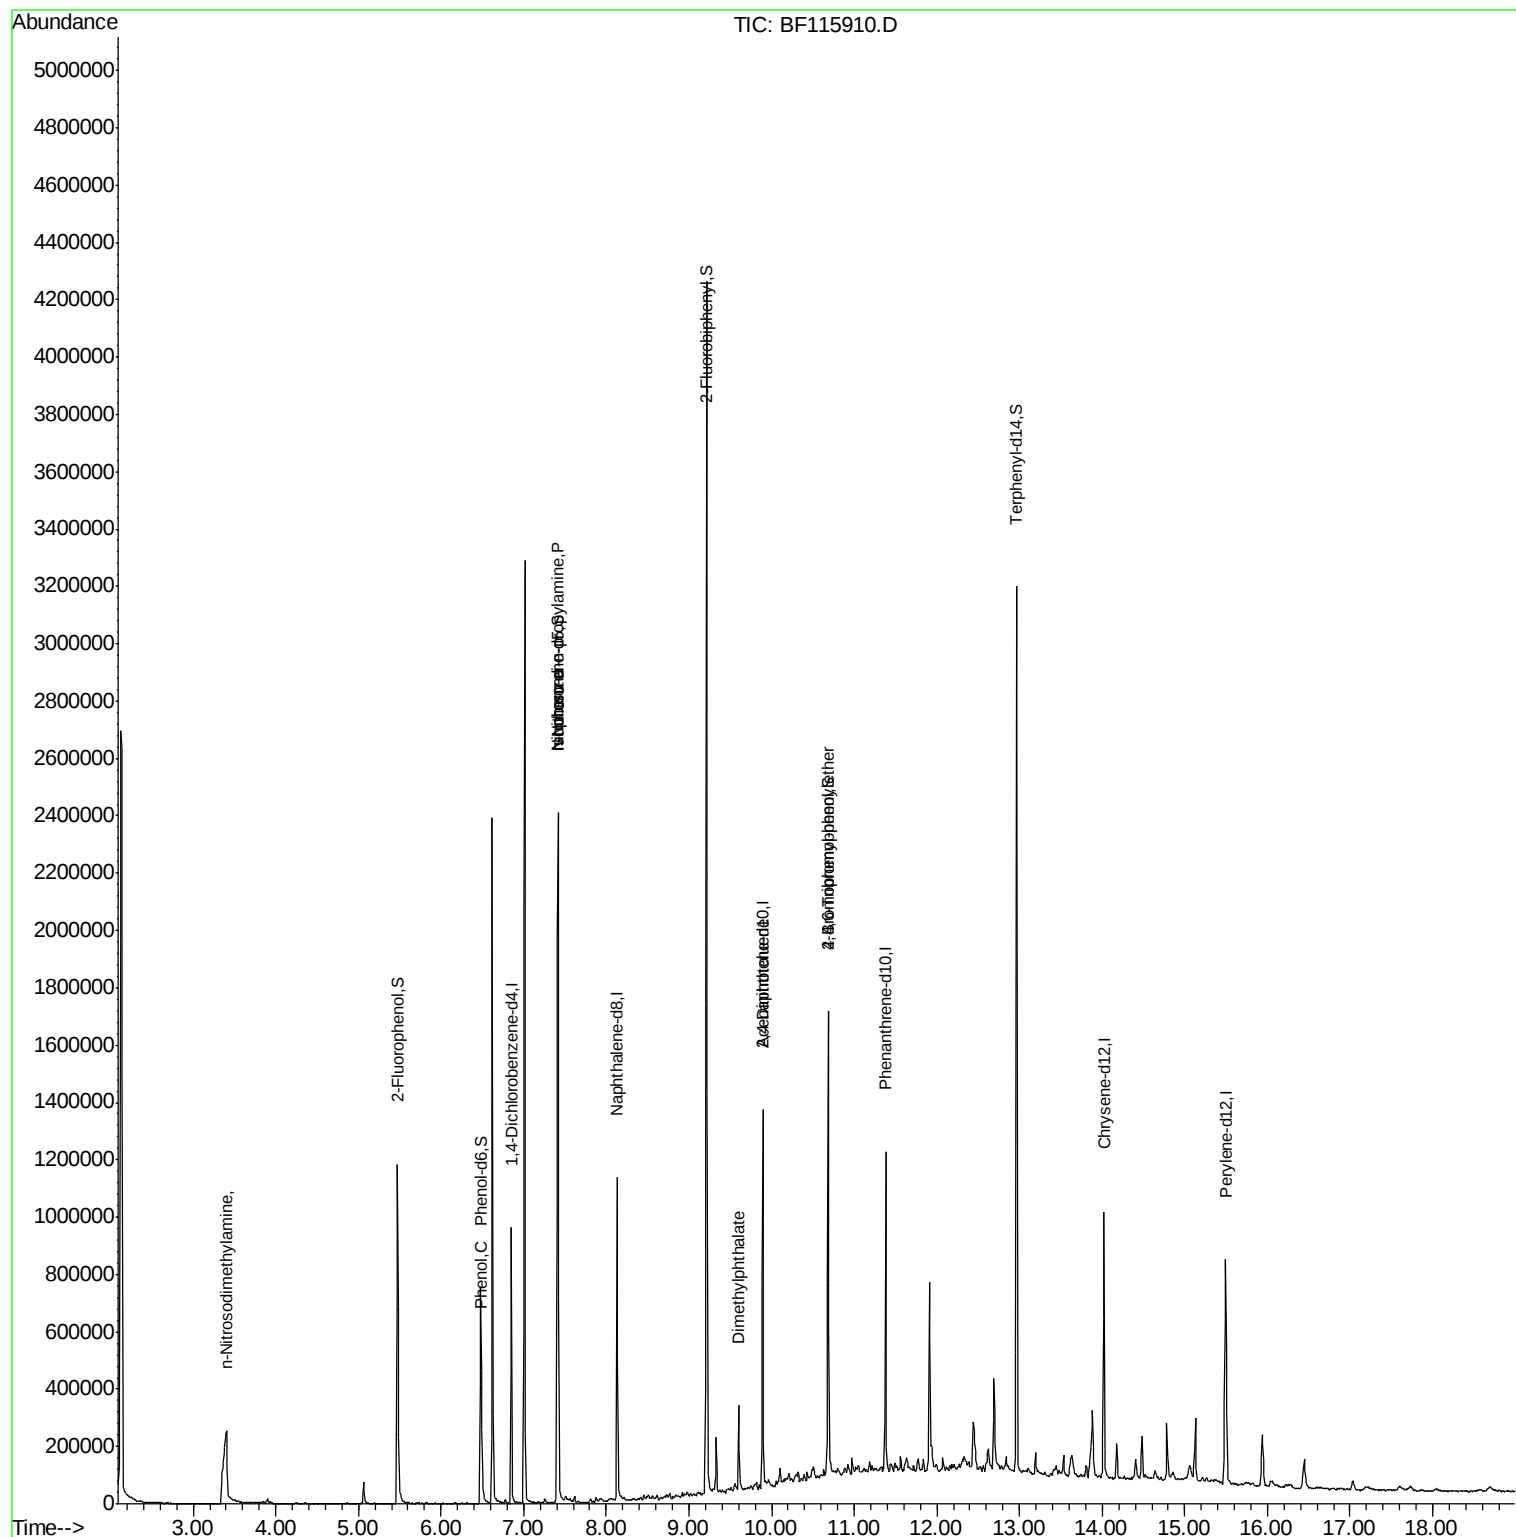



#1

1,4-Dichlorobenzene-d4

Concen: 20.000 ng

RT: 6.85 min Scan# 810

Delta R.T. 0.00 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02

Instrument :

BNA_F

ClientSampleId :

TANK-4





Tgt Ion: 152 Resp: 132830

Ion Ratio Lower Upper

152 100

150 155.2 127.4 191.0

115 60.5 51.8 77.8

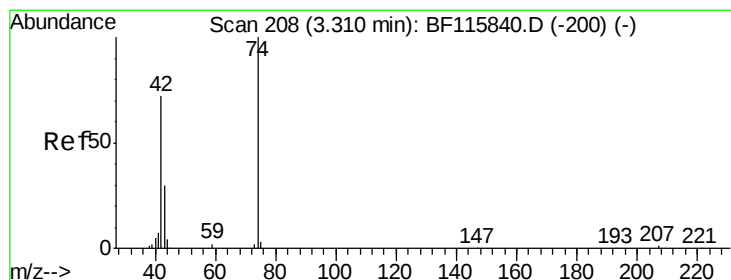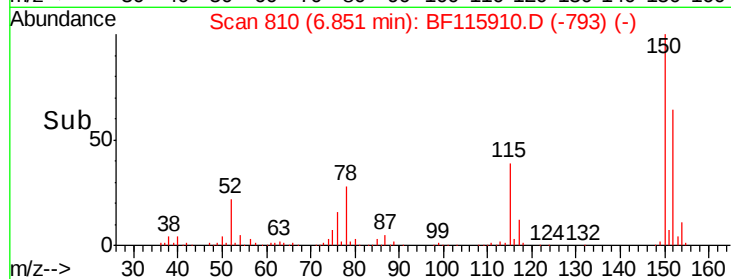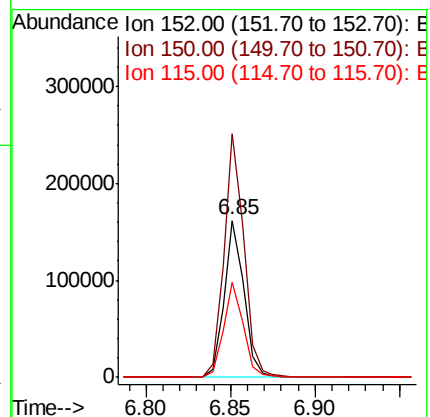

#4

n-Nitrosodimethylamine

Concen: 4.079 ng

RT: 3.40 min Scan# 224

Delta R.T. 0.09 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02




Tgt Ion: 42 Resp: 18026


Ion Ratio Lower Upper

42 100

74 0.0 111.0 166.4#

44 163.4 4.7 7.1#

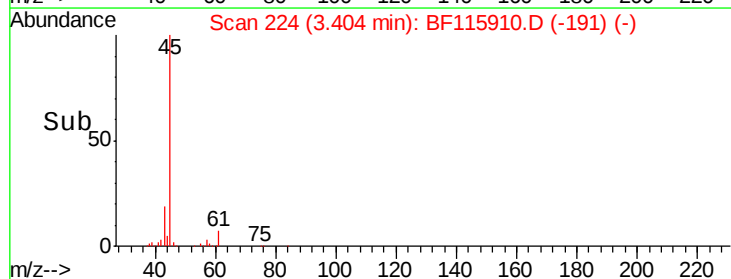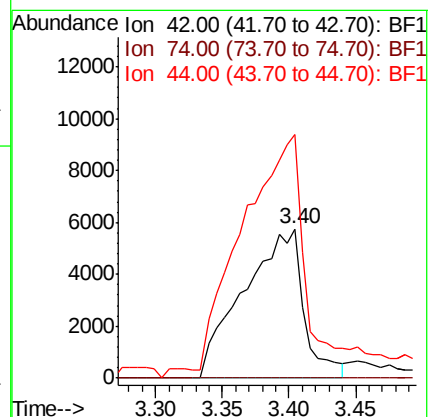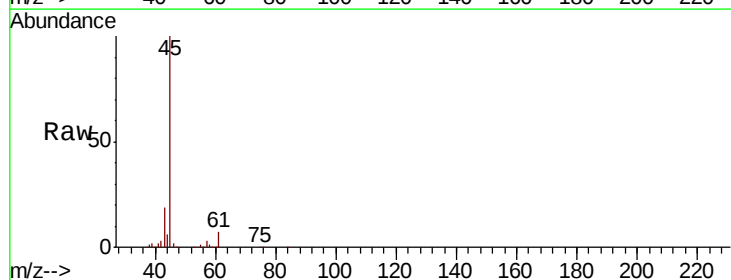

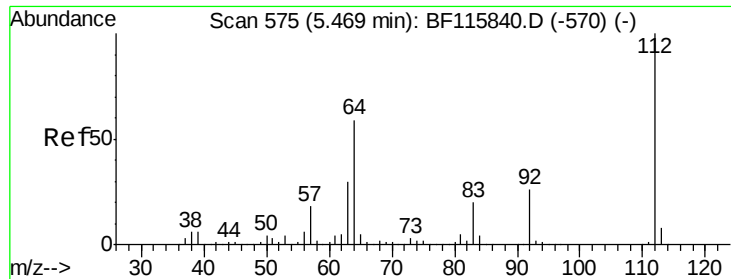

#5

2-Fluorophenol

Concen: 43.334 ng

RT: 5.47 min Scan# 576

Delta R.T. 0.01 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02

Instrument :

BNA_F

ClientSampleId :

TANK-4


Tgt Ion: 112 Resp: 343834

Ion Ratio Lower Upper

112 100

64 56.4 46.8 70.2




63 30.0 24.2 36.2

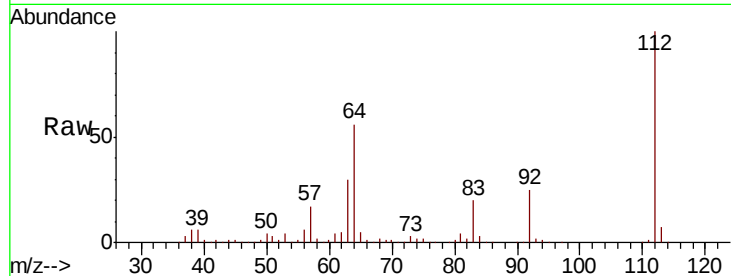

Abundance Ion 112.00 (111.70 to 112.70): BF1

Ion 64.00 (63.70 to 64.70): BF1

Ion 63.00 (62.70 to 63.70): BF1

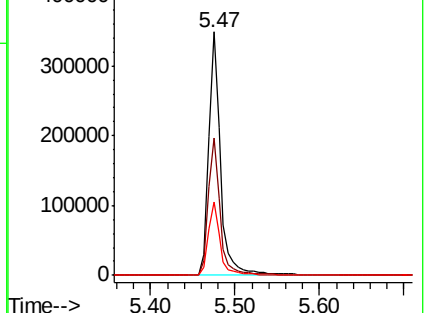

#7

Phenol-d6

Concen: 26.103 ng

RT: 6.48 min Scan# 747

Delta R.T. -0.01 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02


Tgt Ion: 99 Resp: 261313

Ion Ratio Lower Upper

99 100

42 16.9 13.8 20.6



71 32.4 27.1 40.7




Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

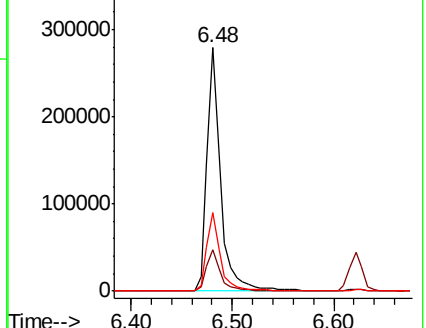



#10

Phenol

Concen: 3.629 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.01 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02

Instrument :

BNA_F

ClientSampled :

TANK-4





Tgt Ion: 94 Resp: 42779

Ion Ratio Lower Upper

94 100

65 29.9 8.9 48.9

66 44.3 18.0 58.0

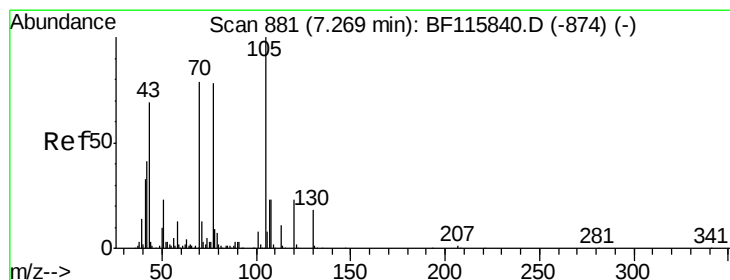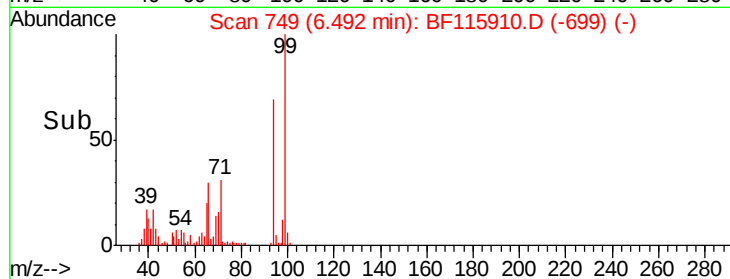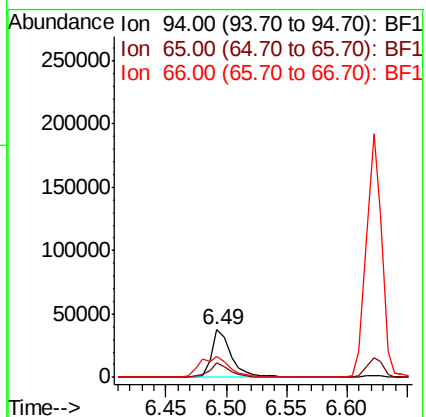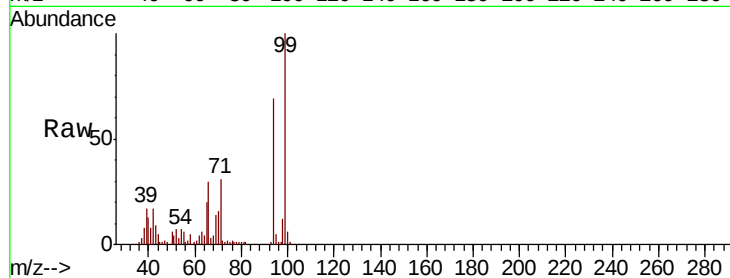

#19

n-Nitroso-di-n-propylamine

Concen: 18.375 ng

RT: 7.42 min Scan# 906

Delta R.T. 0.15 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02

Tgt Ion: 70 Resp: 113987




Ion Ratio Lower Upper


70 100

42 43.9 41.8 62.8

101 0.0 7.7 11.5#

130 2.1 17.8 26.6#

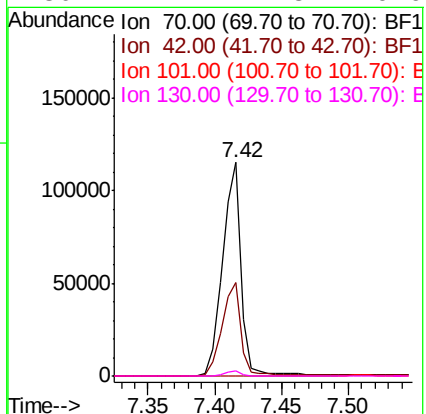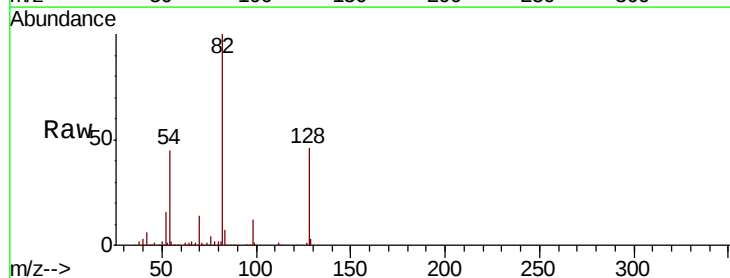







#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.13 min Scan# 1028
Delta R.T. 0.00 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Instrument :
BNA_F
ClientSampleId :
TANK-4

Tgt Ion:	136	Resp:	489961
Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.1	13.7
54	6.8	6.1	9.1
68	6.0	5.4	8.2

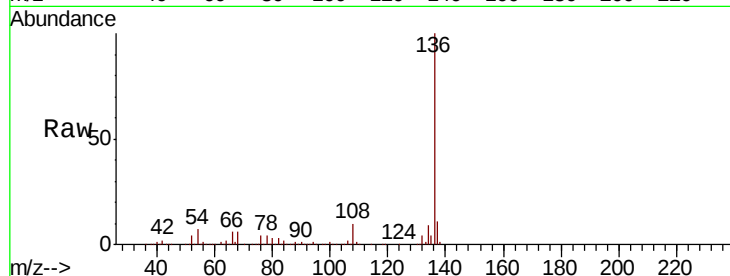


Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

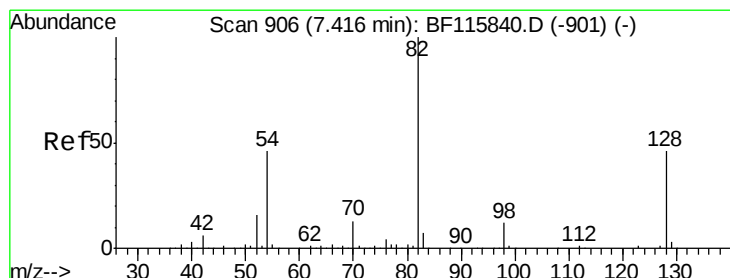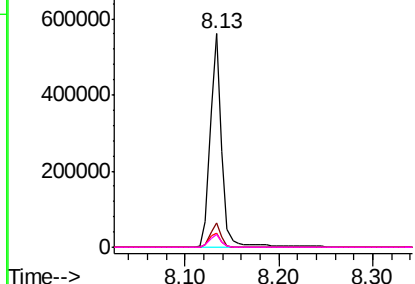




#23
Nitrobenzene-d5
Concen: 98.802 ng
RT: 7.42 min Scan# 906
Delta R.T. 0.00 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Tgt Ion:	82	Resp:	838646
Ion	Ratio	Lower	Upper
82	100		
128	46.5	36.6	55.0
54	45.2	36.6	55.0

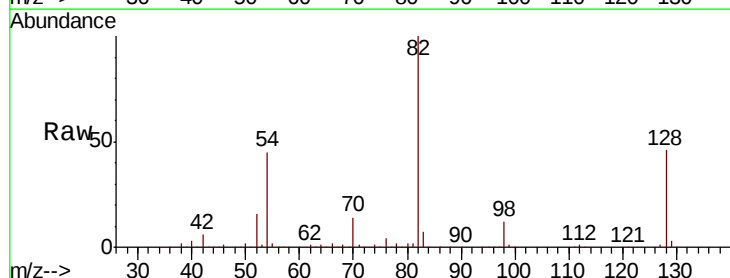

Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): E
Ion 54.00 (53.70 to 54.70): BF1

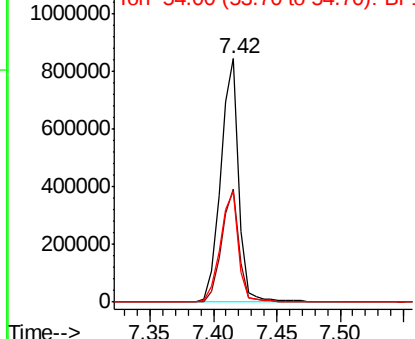

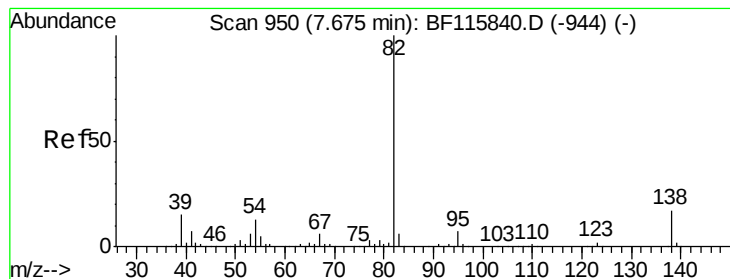

#25

Isophorone

Concen: 51.670 ng

RT: 7.42 min Scan# 906

Delta R.T. -0.26 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02

Instrument :

BNA_F

ClientSampled :

TANK-4


Tgt Ion: 82 Resp: 838634

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#




138 0.0 13.9 20.9#

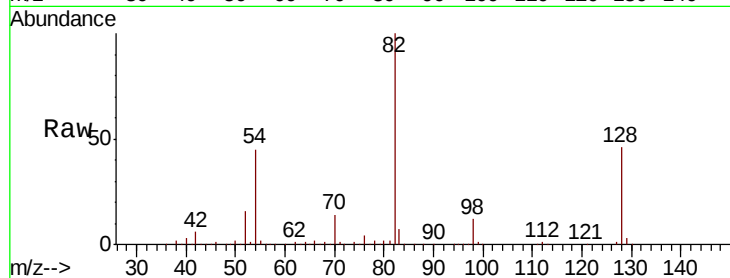

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): E

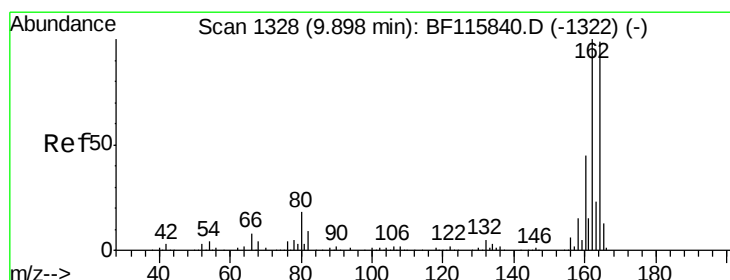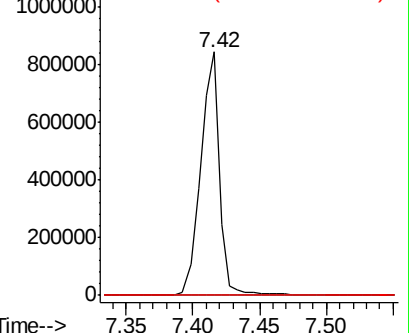

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.89 min Scan# 1327

Delta R.T. -0.01 min

Lab File: BF115910.D

Acq: 1 Aug 2019 17:02


Tgt Ion: 164 Resp: 249578

Ion Ratio Lower Upper

164 100

162 102.8 80.8 121.2



160 46.2 36.2 54.4

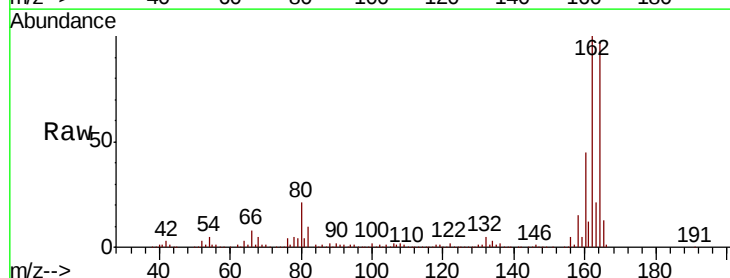


Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

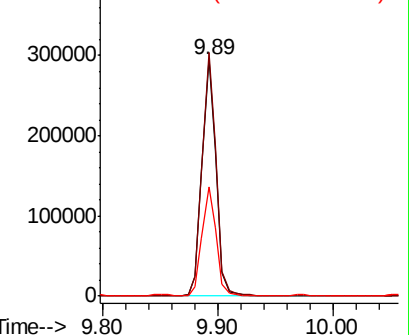







#42
 2,4,6-Tribromophenol
 Concen: 92.258 ng
 RT: 10.69 min Scan# 1462
 Delta R.T. 0.00 min
 Lab File: BF115910.D
 Acq: 1 Aug 2019 17:02

Instrument :
 BNA_F
 ClientSampleId :
 TANK-4

Tgt Ion:330 Resp: 223240
 Ion Ratio Lower Upper
 330 100
 332 97.1 77.7 116.5
 141 34.6 28.1 42.1

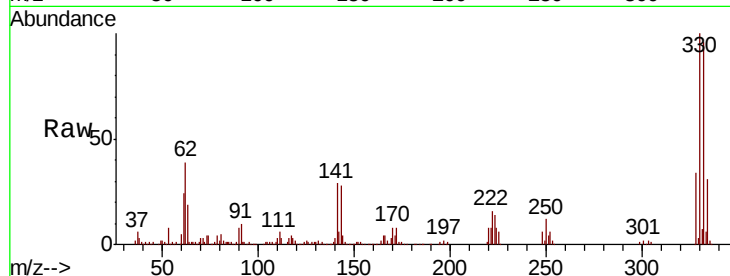


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

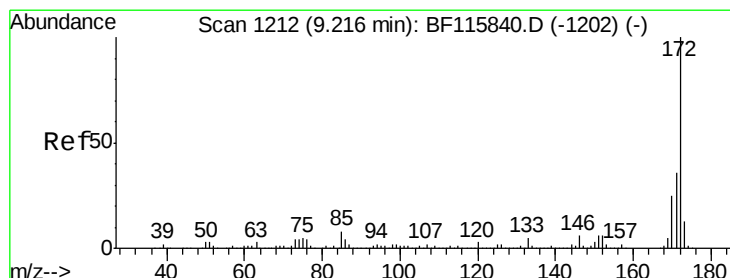
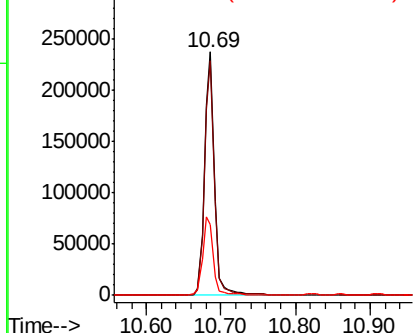



#45
 2-Fluorobiphenyl
 Concen: 104.019 ng
 RT: 9.22 min Scan# 1212
 Delta R.T. 0.00 min
 Lab File: BF115910.D
 Acq: 1 Aug 2019 17:02

Tgt Ion:172 Resp: 1386006
 Ion Ratio Lower Upper
 172 100
 171 36.6 29.1 43.7
 170 25.2 20.1 30.1

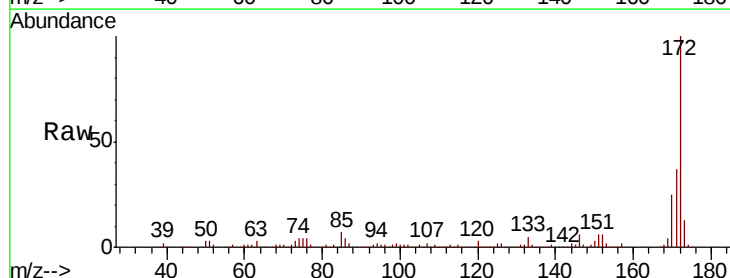

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

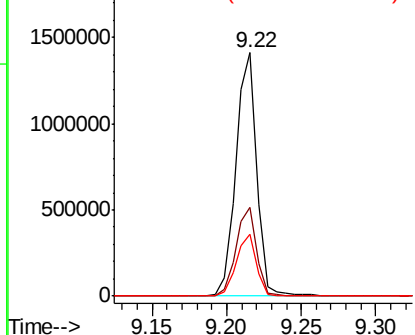







#50
Dimethylphthalate
Concen: 6.481 ng
RT: 9.60 min Scan# 1278
Delta R.T. -0.01 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Instrument :
BNA_F
ClientSampleId :
TANK-4

Tgt Ion	Ratio	Lower	Upper
163	100		
194	3.8	3.0	4.6
164	10.3	8.4	12.6




Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E


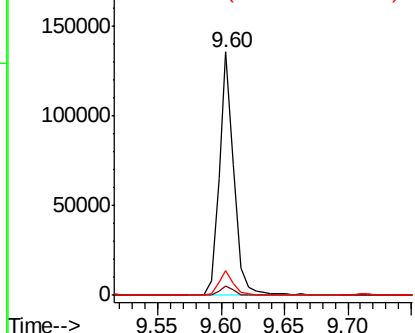



#57
2,4-Dinitrotoluene
Concen: 6.689 ng
RT: 9.89 min Scan# 1327
Delta R.T. -0.19 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Tgt Ion	Ratio	Lower	Upper
165	100		
63	2.1	33.2	49.8#
89	2.1	57.3	85.9#
182	0.0	2.1	3.1#



Abundance Ion 165.00 (164.70 to 165.70): E
Ion 63.00 (62.70 to 63.70): BF1
Ion 89.00 (88.70 to 89.70): BF1
Ion 182.00 (181.70 to 182.70): E

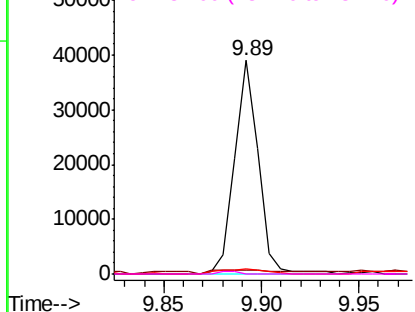


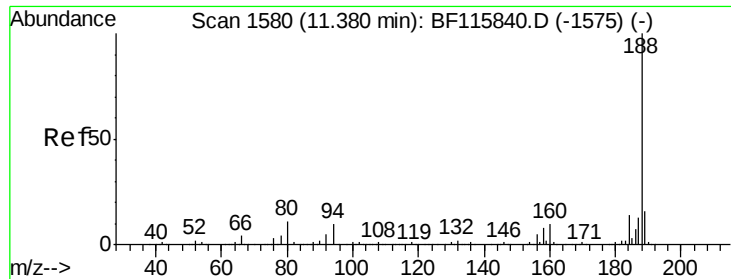




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.38 min Scan# 1580
Delta R.T. 0.00 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Instrument :
BNA_F
ClientSampleId :
TANK-4

Tgt Ion:188 Resp: 379260
Ion Ratio Lower Upper
188 100
94 8.8 8.0 12.0
80 10.0 8.6 12.8




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

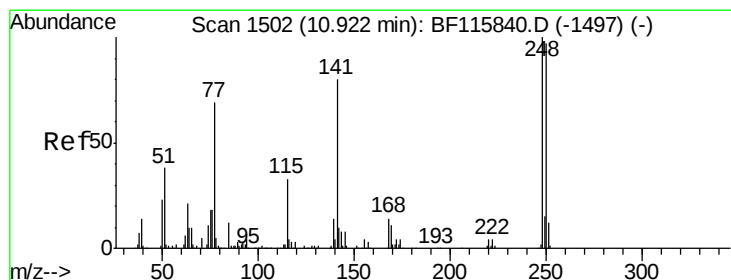
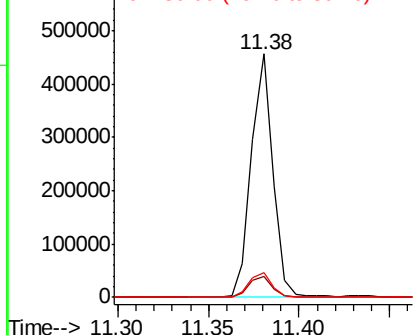



#67
4-Bromophenyl-phenylether
Concen: 3.308 ng
RT: 10.69 min Scan# 1462
Delta R.T. -0.24 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Tgt Ion:248 Resp: 13429
Ion Ratio Lower Upper
248 100
250 208.6 77.8 116.6#
141 498.9 64.3 96.5#



Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E




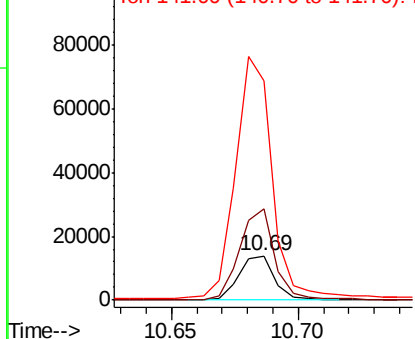




#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.02 min Scan# 2029
Delta R.T. -0.01 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02




Instrument :
BNA_F
ClientSampleId :
TANK-4


Tgt Ion:240 Resp: 273455
Ion Ratio Lower Upper
240 100
120 10.9 8.5 12.7
236 26.4 22.2 33.2

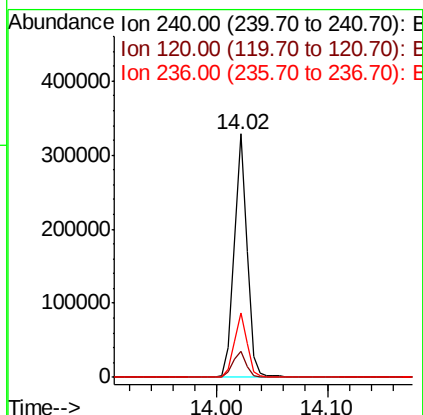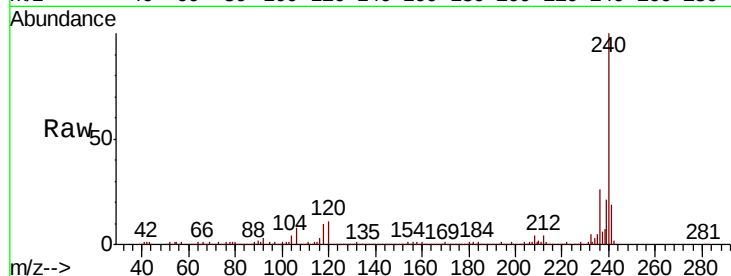

#79
Terphenyl-d14
Concen: 84.383 ng
RT: 12.96 min Scan# 1849
Delta R.T. -0.01 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Tgt Ion:244 Resp: 1095073
Ion Ratio Lower Upper
244 100
212 7.3 5.6 8.4
122 12.9 8.6 13.0

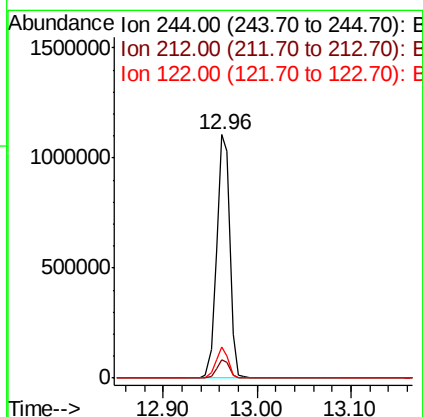

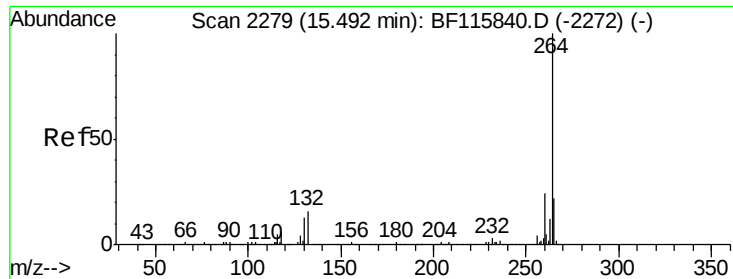

#87
Perylene-d12
Concen: 20.000 ng
RT: 15.49 min Scan# 2279
Delta R.T. 0.00 min
Lab File: BF115910.D
Acq: 1 Aug 2019 17:02

Instrument :
BNA_F
ClientSampleId :
TANK-4

Tgt Ion	Ratio	Lower	Upper
264	100		
260	24.6	19.4	29.2
265	21.4	17.5	26.3

