
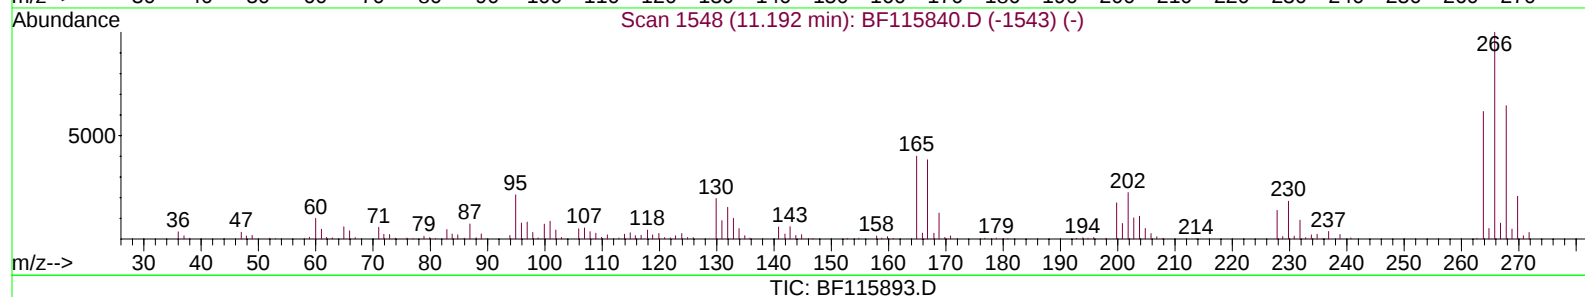
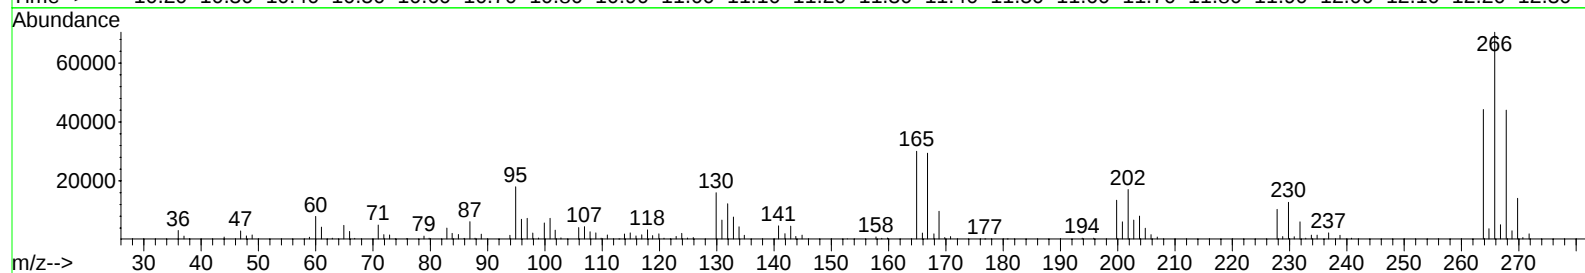


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080119\
Data File : BF115893.D
Acq On : 1 Aug 2019 8:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 18:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

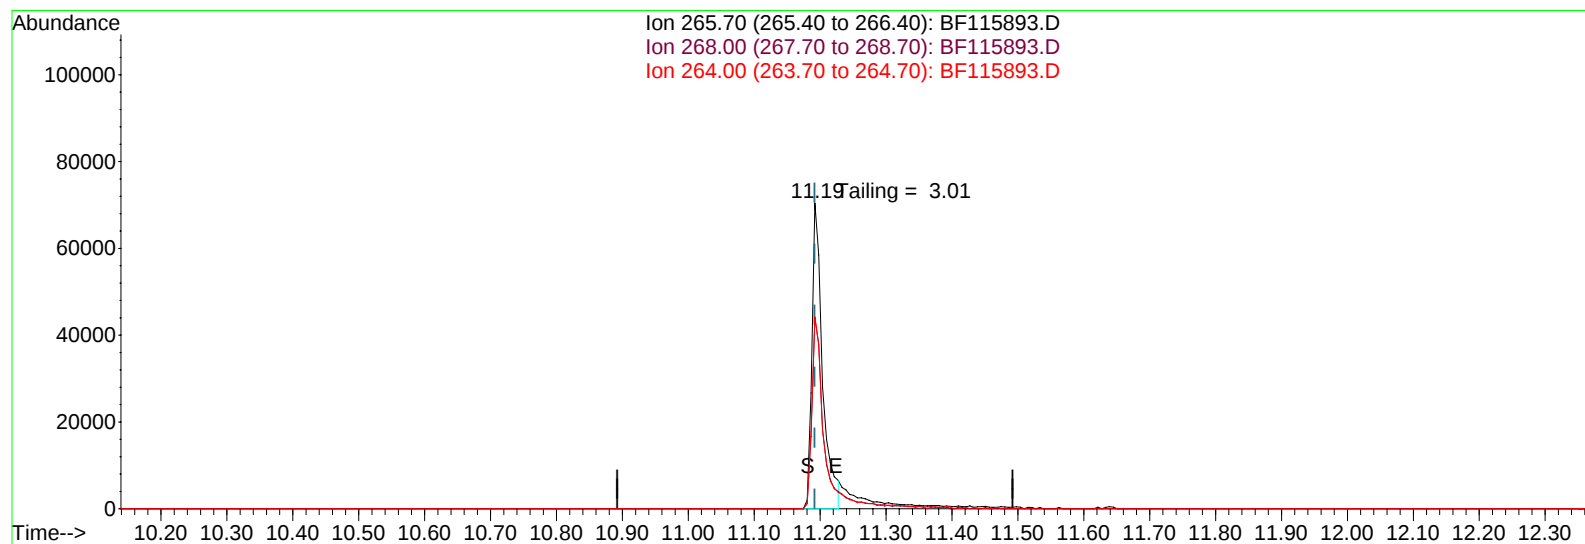

(70) Pentachlorophenol (C)




11.192min (-0.000) 53705.82ng

response 94246

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	62.49
264.00	61.70	62.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF080119\
Data File : BF115893.D
Acq On : 1 Aug 2019 8:23
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 18:42:56 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jul 31 15:31:51 2019
Response via : Initial Calibration

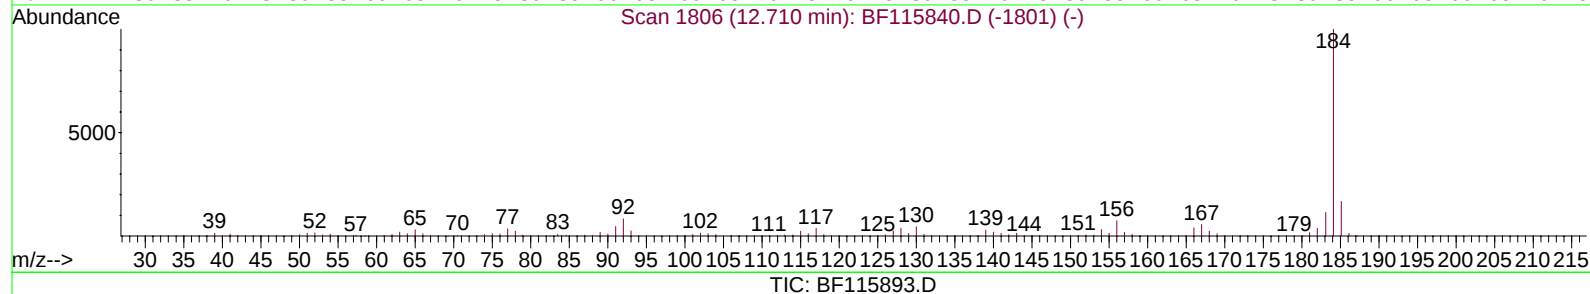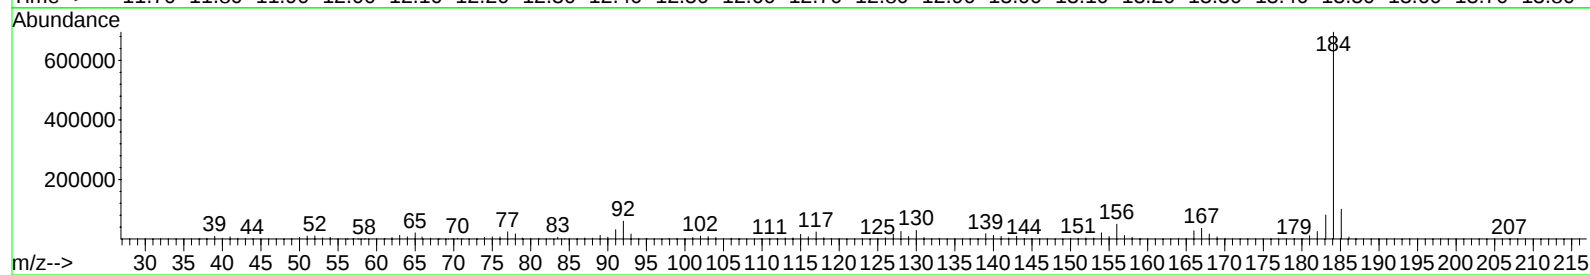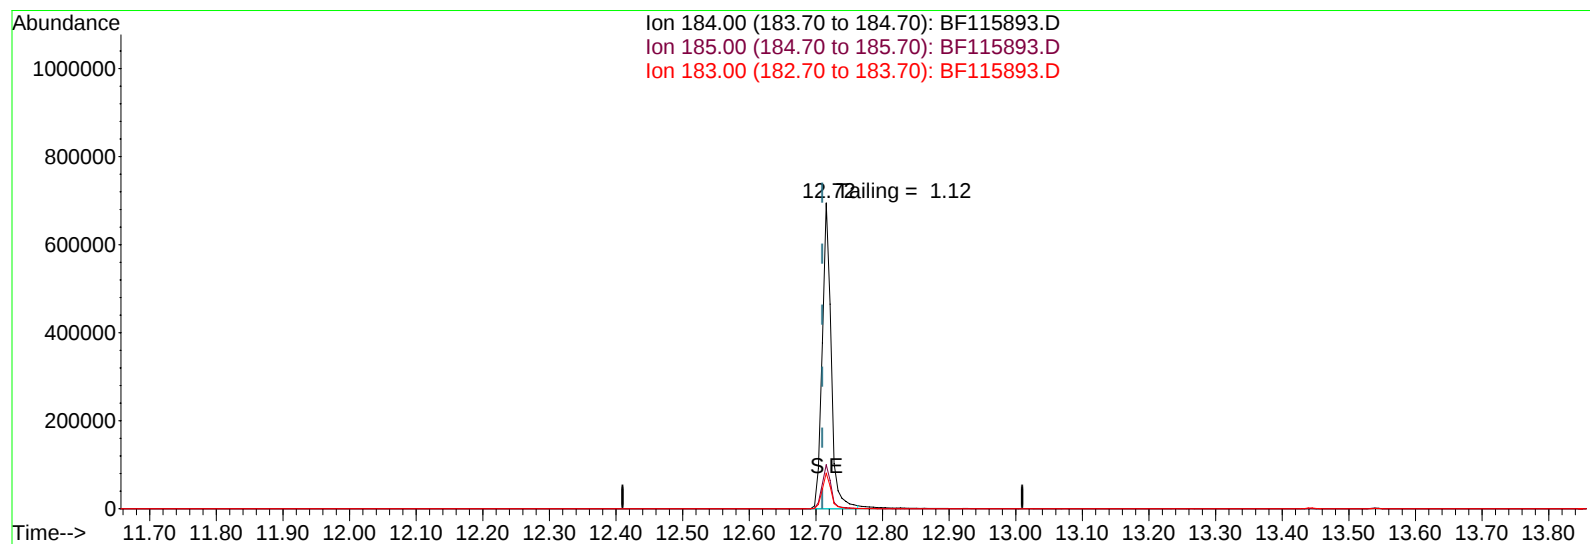

(77) Benzidine

12.715min (+0.006) 0.00ng

response 665071

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	14.42
183.00	11.40	11.68
0.00	0.00	0.00