

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080119\
 Data File : BF115897.D
 Acq On : 1 Aug 2019 10:29
 Operator : HP/JU
 Sample : PB121854BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB121854BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.228	17	24	30	rVB	89892	125753	2.68%	0.340%
2	5.492	574	579	582	rBV	3402472	3674579	78.37%	9.948%
3	6.492	743	749	752	rBV	3541163	3824599	81.57%	10.355%
4	6.628	767	772	775	rBV	3913677	3931575	83.86%	10.644%
5	6.851	807	810	822	rVB	1176369	1009890	21.54%	2.734%
6	7.010	833	837	841	rBV	3361452	3220228	68.68%	8.718%
7	7.416	900	906	909	rBV	2454230	2578338	54.99%	6.980%
8	8.133	1023	1028	1053	rBV	1374472	1284981	27.41%	3.479%
9	9.216	1205	1212	1215	rBV	4622663	4688518	100.00%	12.693%
10	9.892	1322	1327	1350	rVB	1569773	1513792	32.29%	4.098%
11	10.686	1457	1462	1487	rBV	2765793	2831956	60.40%	7.667%
12	11.380	1576	1580	1588	rBV	1608142	1481711	31.60%	4.012%
13	12.968	1845	1850	1853	rBV	4497521	4601117	98.14%	12.457%
14	14.021	2025	2029	2039	rBV	1136025	1093624	23.33%	2.961%
15	15.498	2275	2280	2293	rBV	677712	1015695	21.66%	2.750%
16	15.951	2353	2357	2363	rVB2	39605	60055	1.28%	0.163%


Sum of corrected areas: 36936411

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080119\
Data File : BF115897.D
Acq On : 1 Aug 2019 10:29
Operator : HP/JU
Sample : PB121854BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121854BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

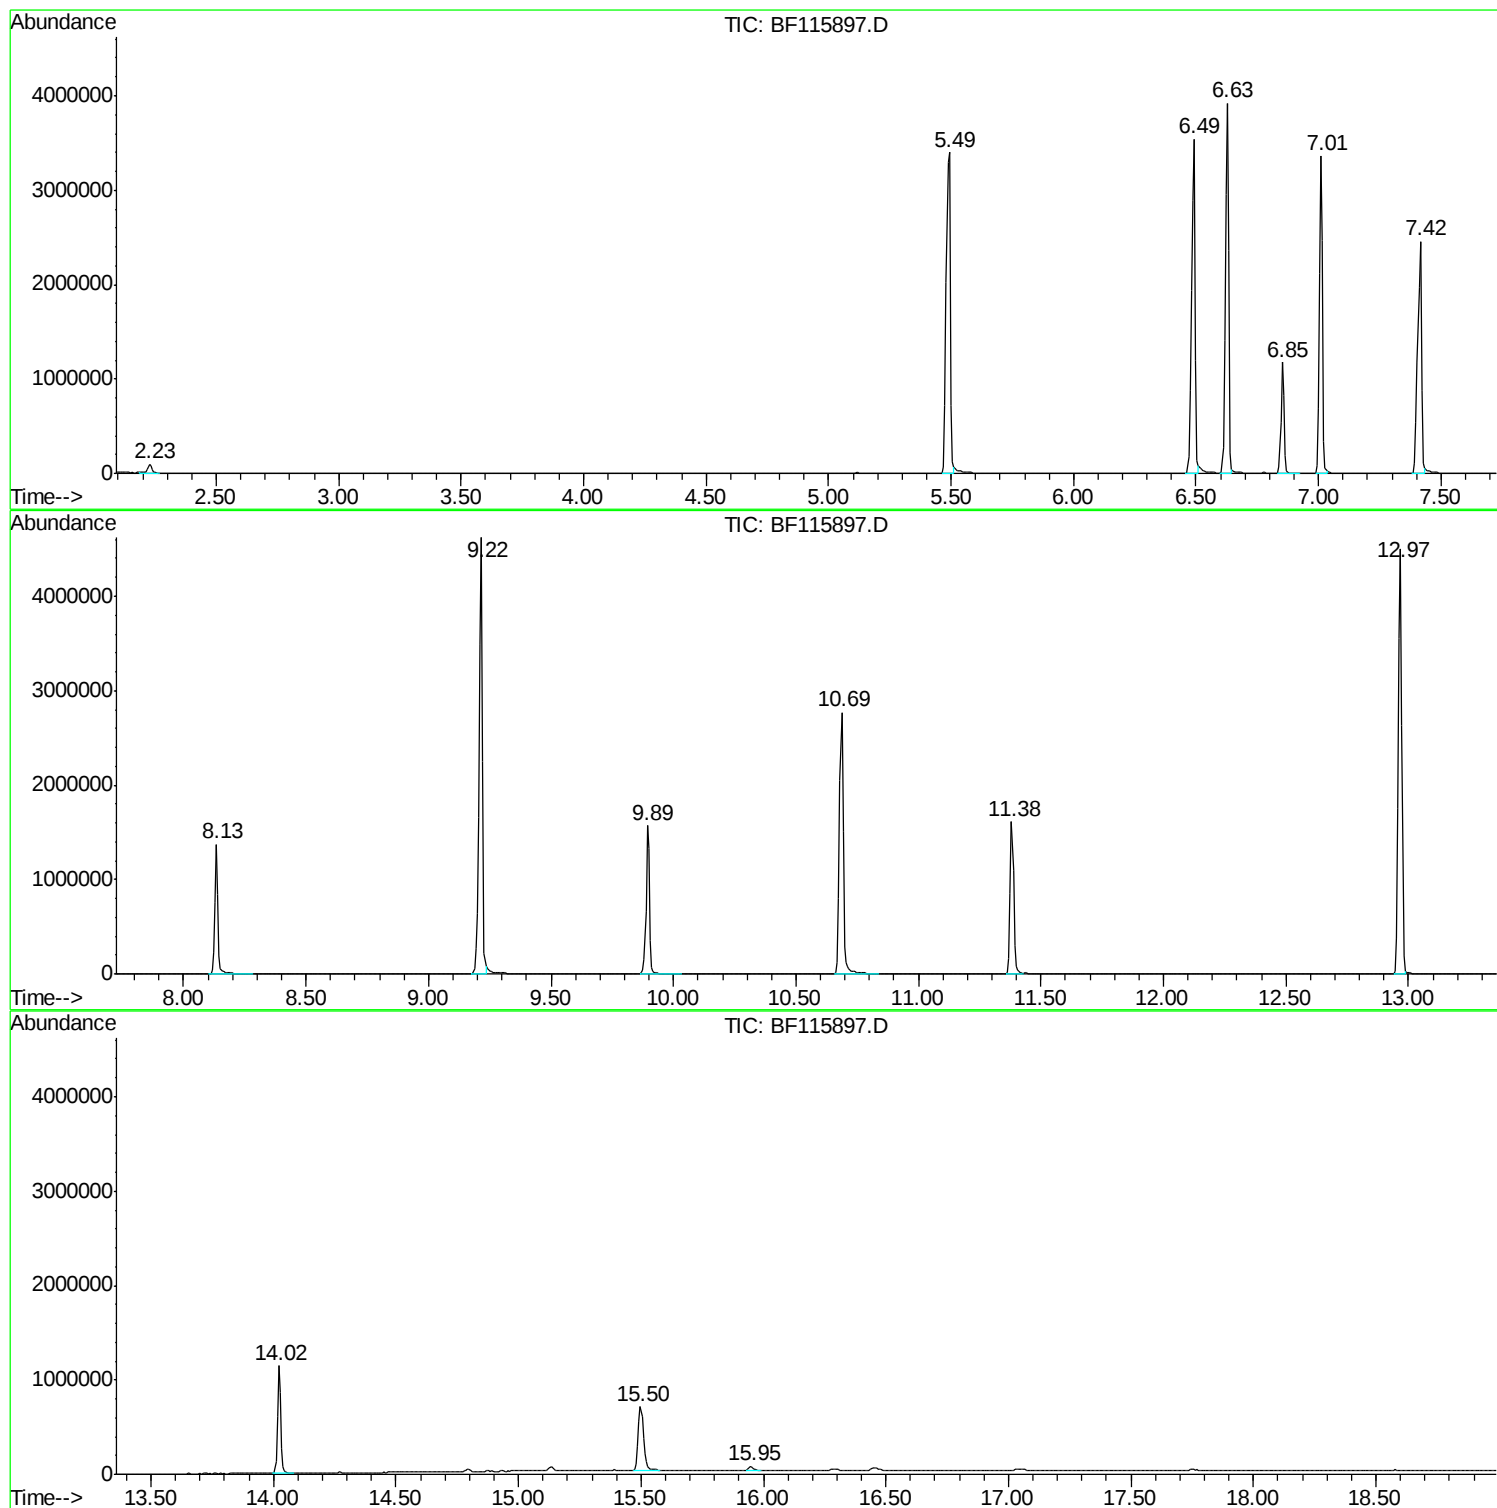

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080119\
Data File : BF115897.D
Acq On : 1 Aug 2019 10:29
Operator : HP/JU
Sample : PB121854BL
Misc :
ALS Vial : 5 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB121854BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.		
2.23	2.49 ng	125753	1,4-Dichlorobenzene-d4	6.85		
Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1		Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2		2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
3		Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	33
4		2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25
5		3-Hexanol, 2-methyl-	116	C7H16O	000617-29-8	25

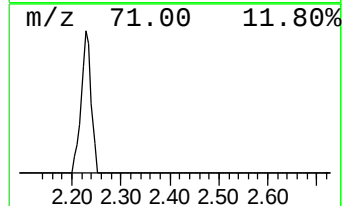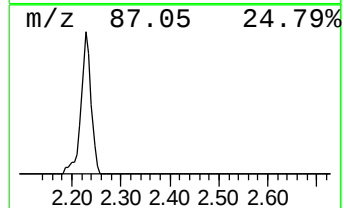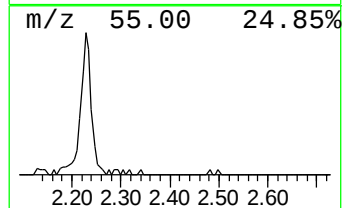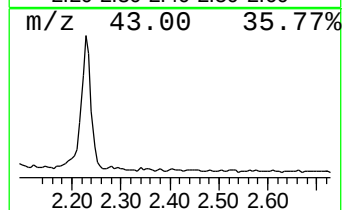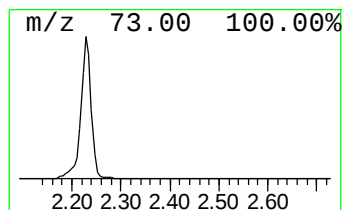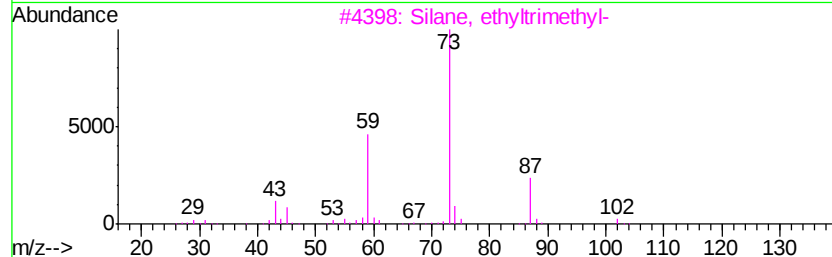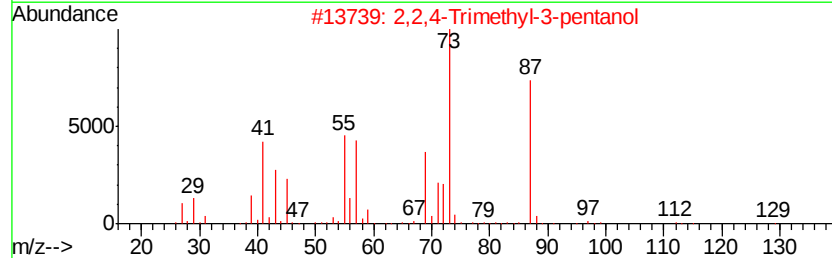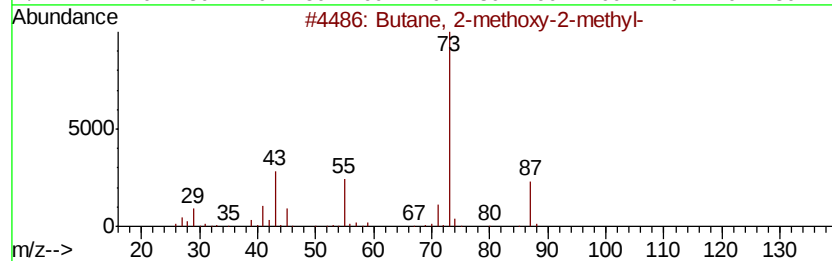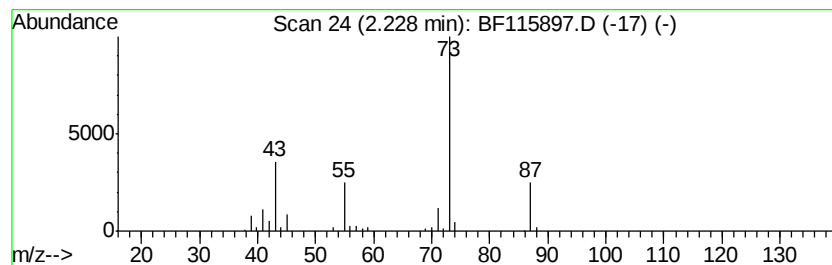

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF080119\
Data File : BF115897.D
Acq On : 1 Aug 2019 10:29
Operator : HP/JU
Sample : PB121854BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121854BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.63 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.63	77.86 ng	3931580	1,4-Dichlorobenzene-d4	6.85

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	12
3		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12
4		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
5		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

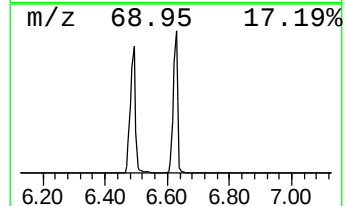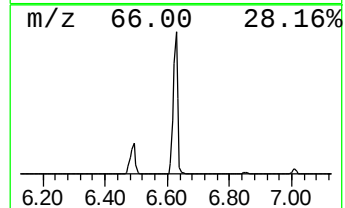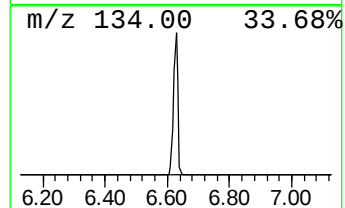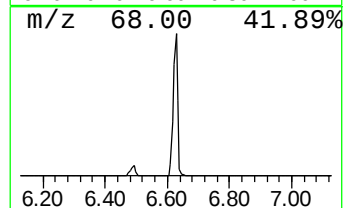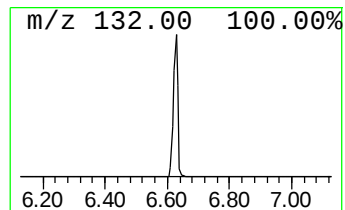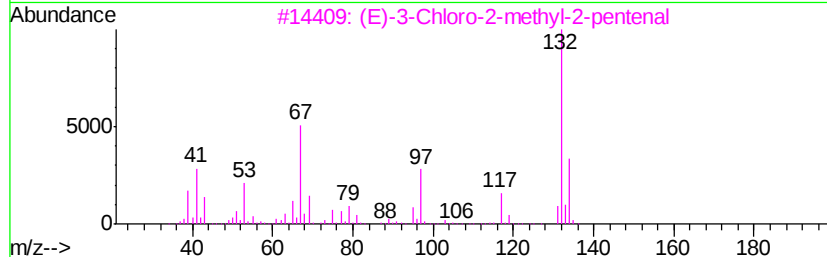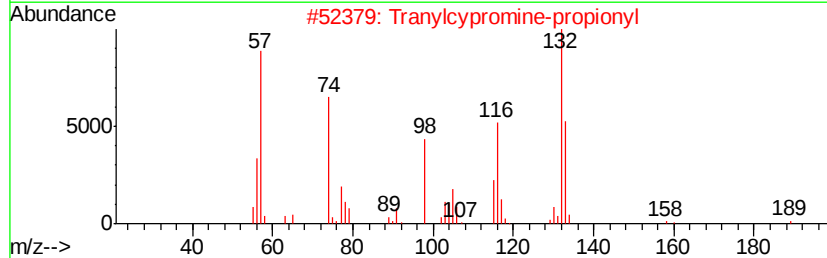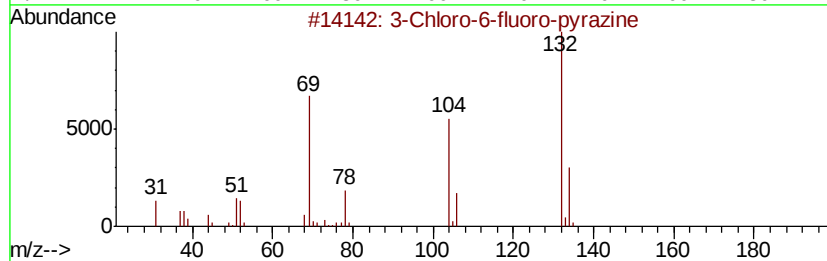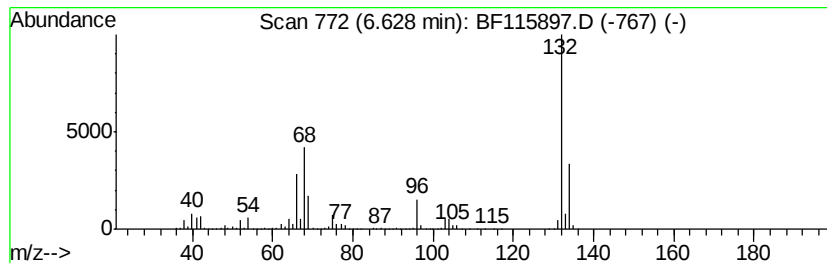

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080119\
Data File : BF115897.D
Acq On : 1 Aug 2019 10:29
Operator : HP/JU
Sample : PB121854BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB121854BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
Butane, 2-methoxy...	2.23	2.5	ng	125753	1	6.85	1009890	20.0
unknown6.63	6.63	77.9	ng	3931580	1	6.85	1009890	20.0