


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF080119\
 Data File : BF115908.D
 Acq On : 1 Aug 2019 16:02
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073019.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jul 31 15:31:51 2019

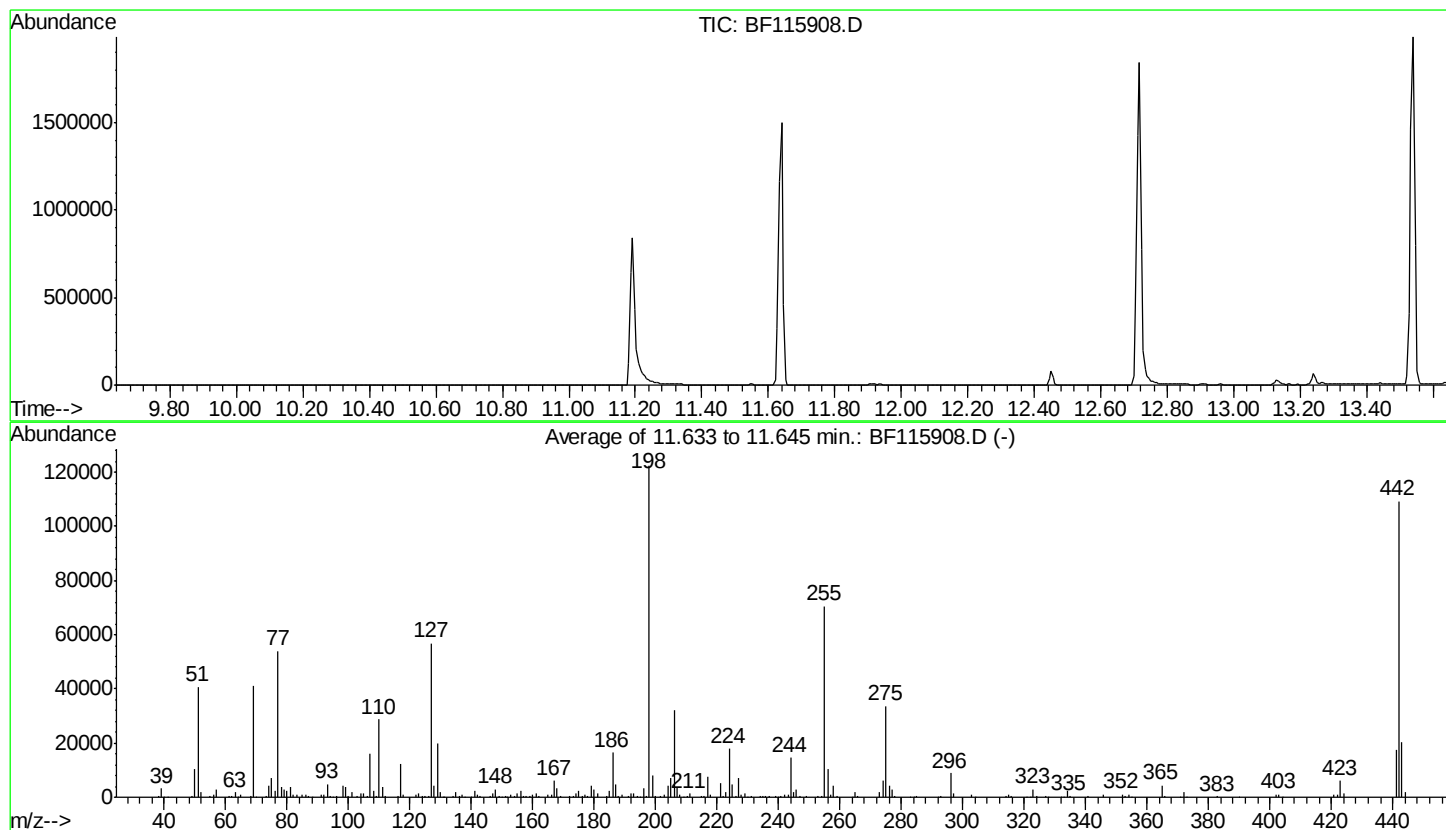

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.3	40800	PASS
68	69	0.00	2	1.5	614	PASS
69	198	0.00	100	33.6	41099	PASS
70	69	0.00	2	0.5	223	PASS
127	198	10	80	46.5	56890	PASS
197	198	0.00	2	0.6	723	PASS
198	198	100	100	100.0	122392	PASS
199	198	5	9	6.7	8235	PASS
275	198	10	60	27.5	33629	PASS
365	198	1	100	3.5	4323	PASS
441	198	0.01	100	14.3	17551	PASS
442	198	50	100	89.3	109269	PASS
443	442	15	24	18.6	20376	PASS