
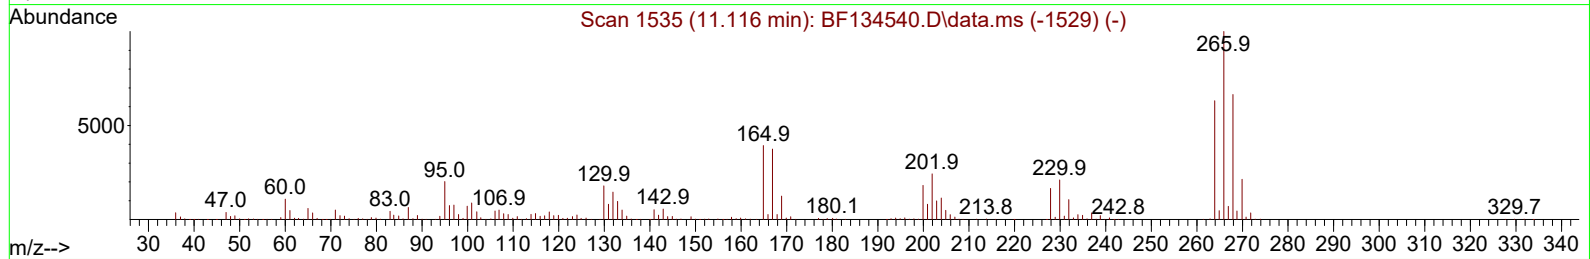
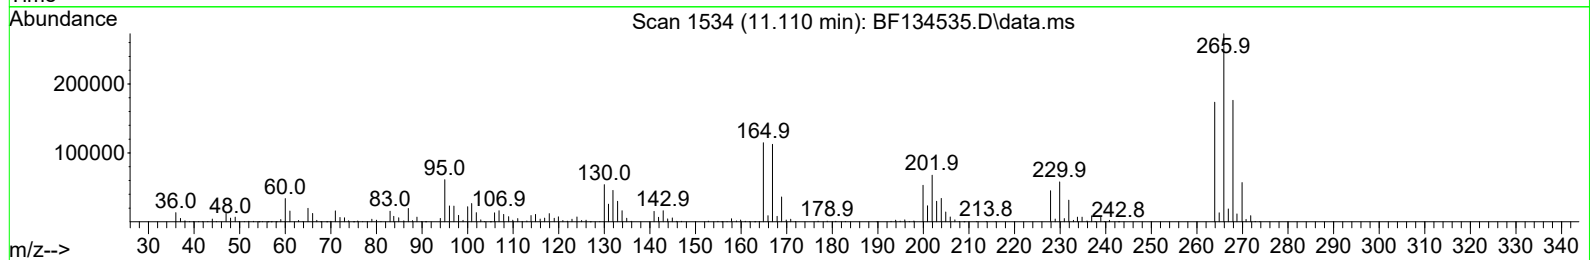


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080123\
Data File : BF134535.D
Acq On : 01 Aug 2023 07:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 02:26:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

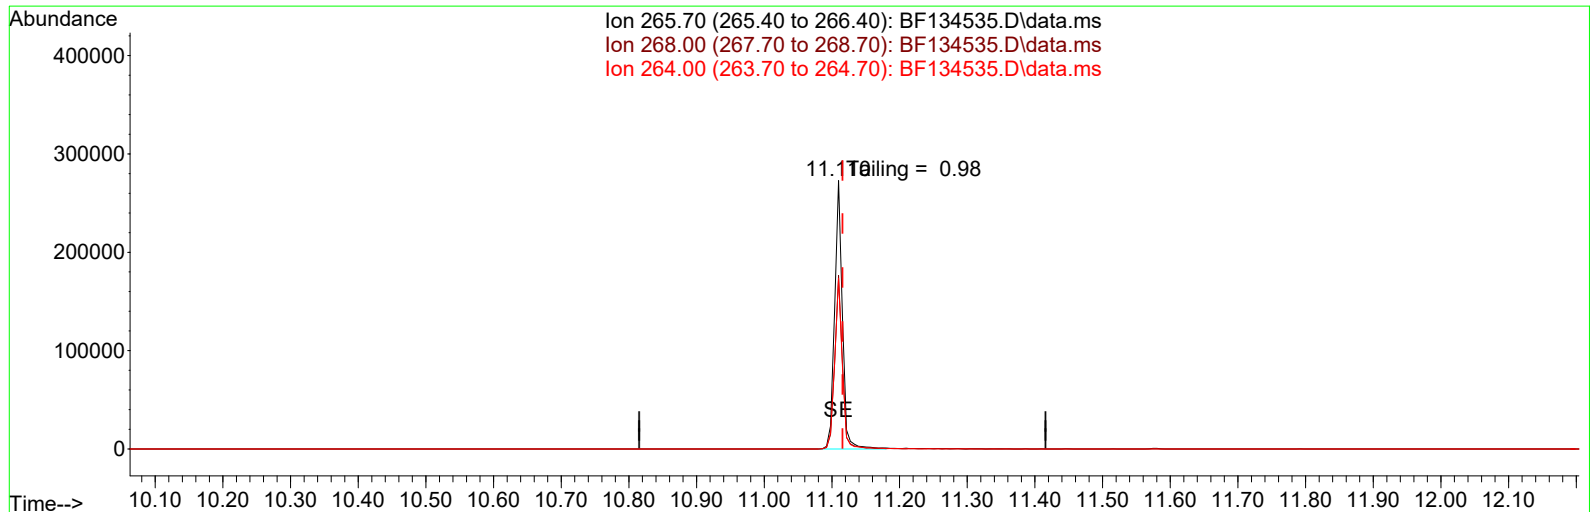

TIC: BF134535.D\data.ms

(70) Pentachlorophenol (C)




11.110min (-0.006) 31442.83 ng

response 218296

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	64.63
264.00	59.70	63.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080123\
Data File : BF134535.D
Acq On : 01 Aug 2023 07:20
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 02:26:34 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF080123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 02:20:34 2023
Response via : Initial Calibration

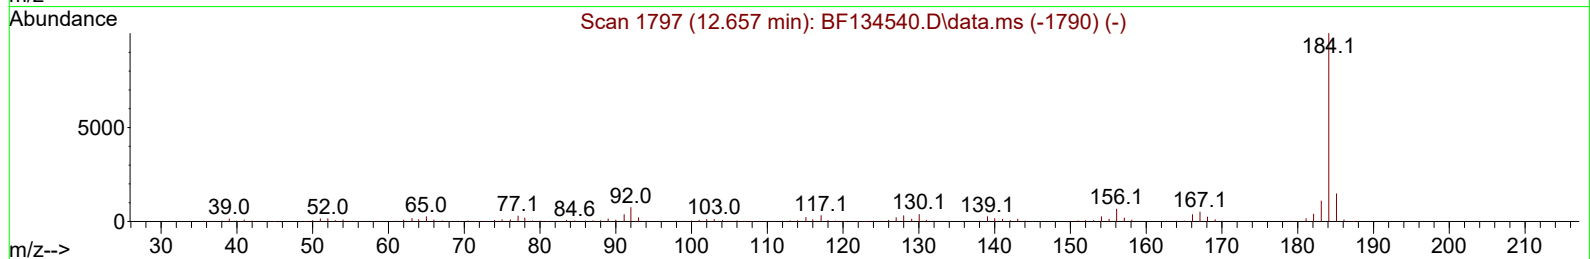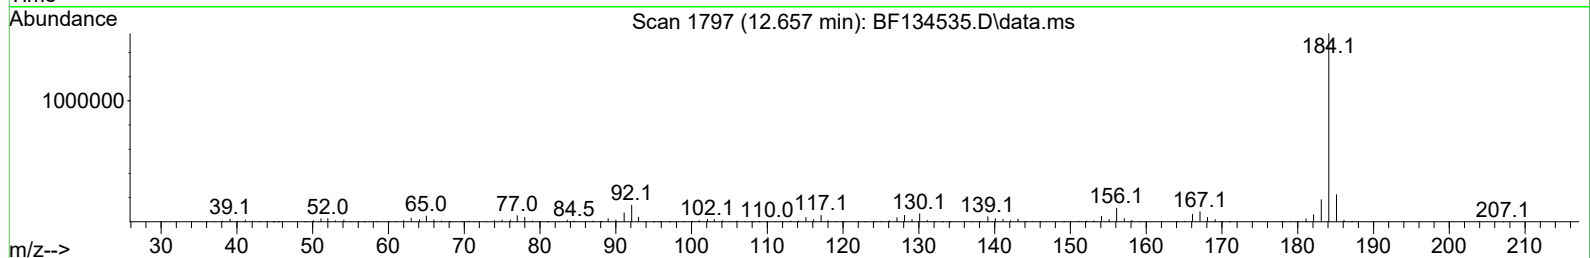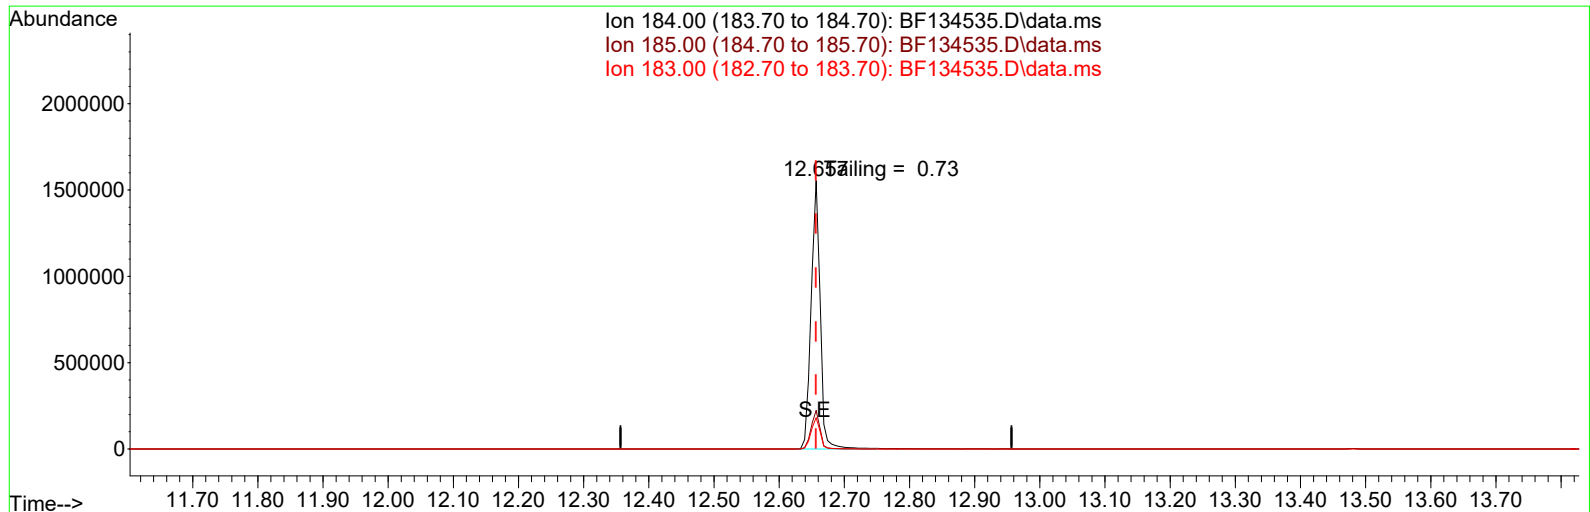

TIC: BF134535.D\data.ms

(77) Benzidine

12.657min (+ 0.000) 0.00 ng

response 1518267

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.40
183.00	10.80	11.72
0.00	0.00	0.00