
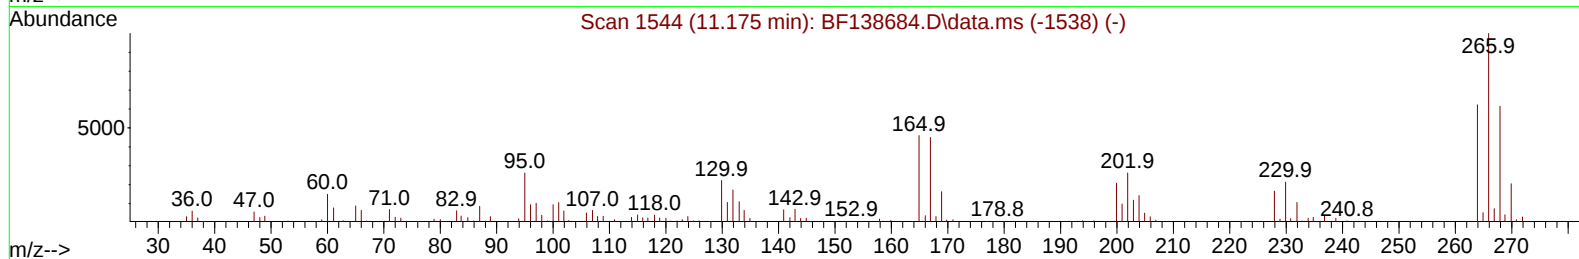
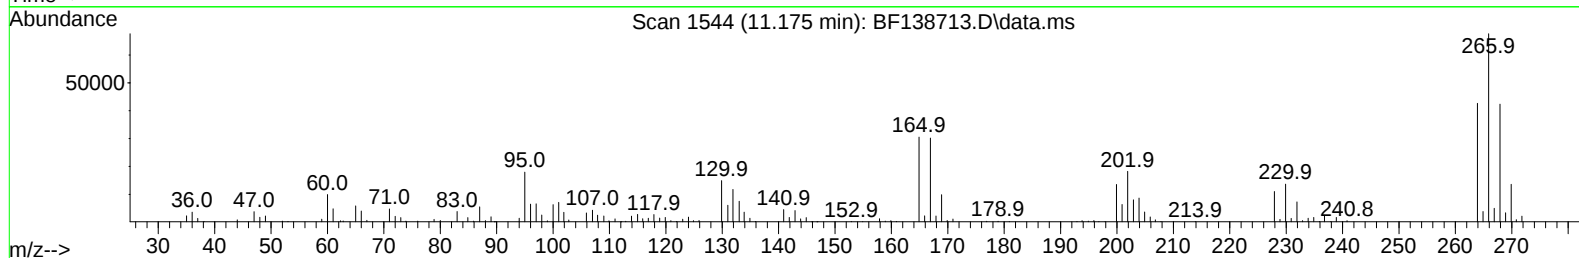


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138713.D
Acq On : 01 Aug 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 11:04:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

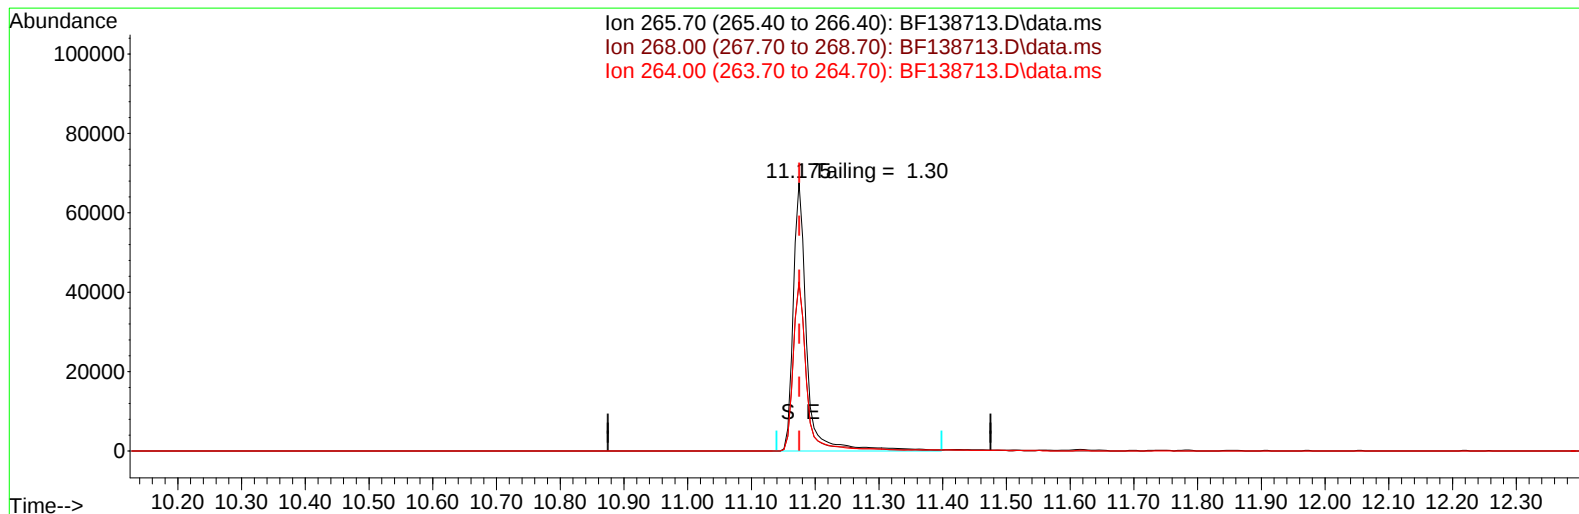

TIC: BF138713.D\data.ms

(70) Pentachlorophenol (C)




11.175min (-0.000) 35881.22 ng

response 99981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.64
264.00	62.20	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138713.D
Acq On : 01 Aug 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 11:04:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

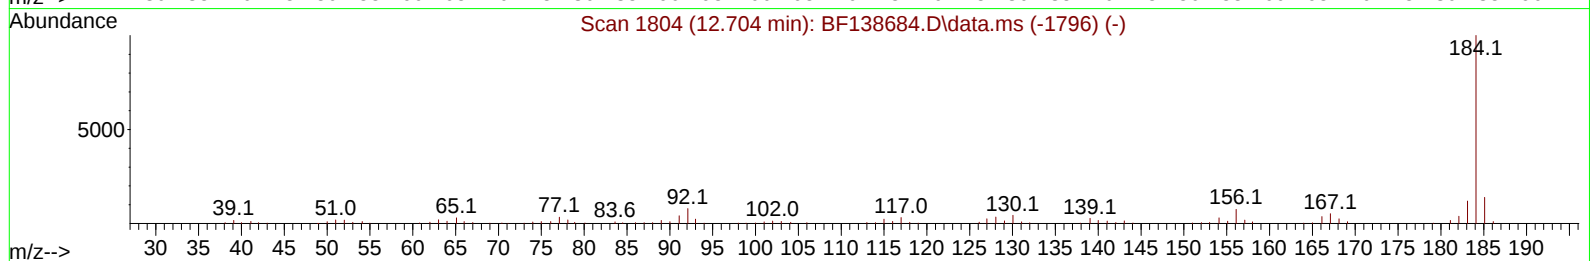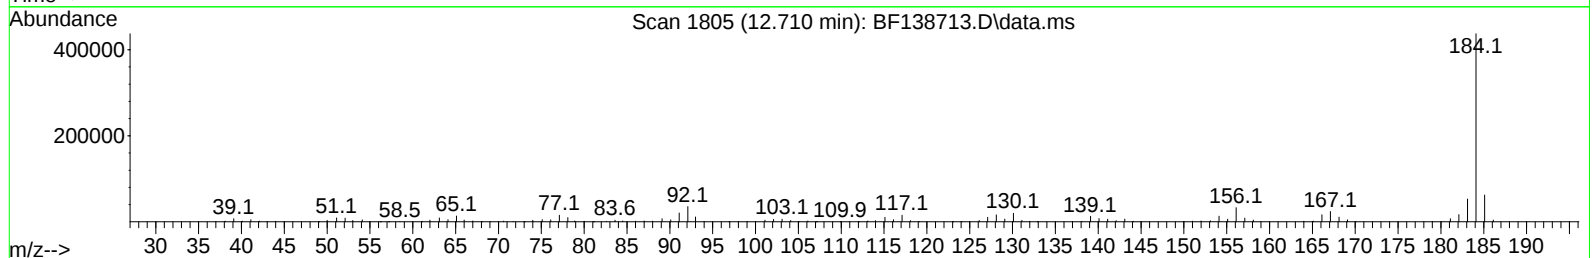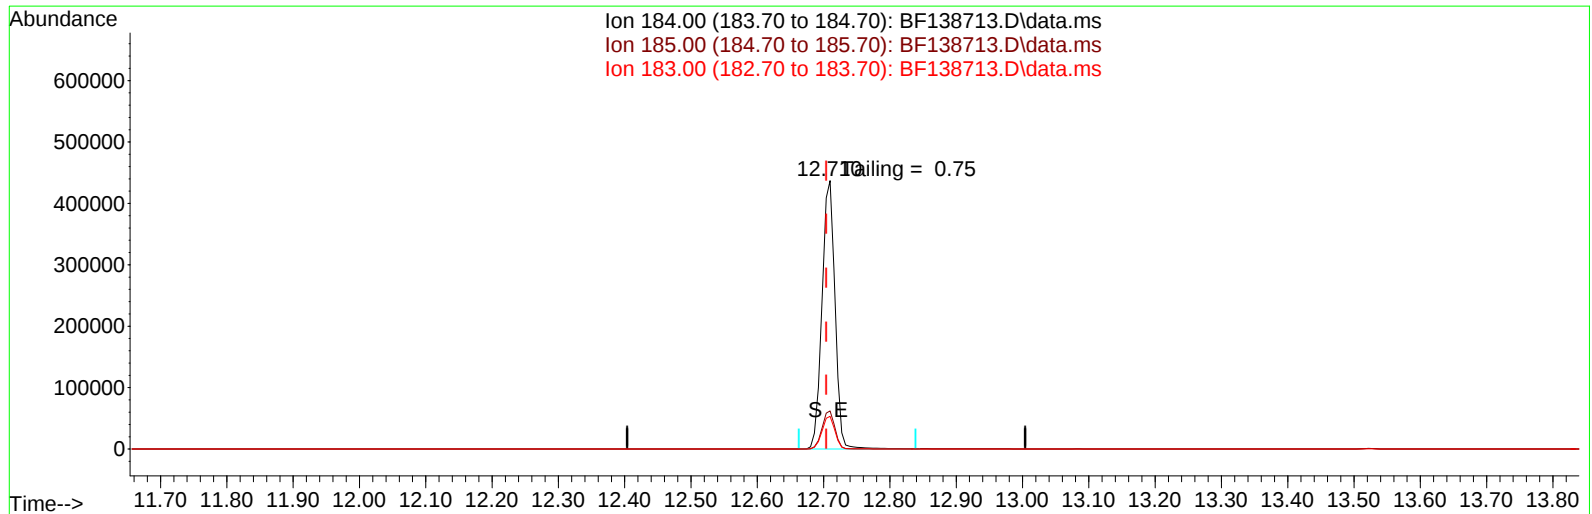

TIC: BF138713.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 598499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.21
183.00	12.00	12.16
0.00	0.00	0.00