

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138717.D
 Acq On : 01 Aug 2024 11:19
 Operator : RC/JU
 Sample : P3379-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-01-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138717.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.352	209	214	228	rBV	35633	90843	4.81%	0.627%
2	5.063	500	505	516	rVB	80448	117235	6.21%	0.809%
3	5.469	569	574	593	rBV	1148392	1509220	79.92%	10.413%
4	6.481	740	746	766	rBV	1199704	1617324	85.64%	11.159%
5	6.675	774	779	792	rBV	30996	52517	2.78%	0.362%
6	6.846	803	808	813	rBV	340649	413735	21.91%	2.855%
7	7.404	897	903	909	rBV	774553	1050515	55.63%	7.248%
8	7.657	942	946	952	rBV	36448	46518	2.46%	0.321%
9	8.128	1020	1026	1031	rBV	435810	560601	29.69%	3.868%
10	8.340	1058	1062	1067	rBV	17397	21283	1.13%	0.147%
11	8.440	1074	1079	1092	rBV	89233	146862	7.78%	1.013%
12	9.198	1202	1208	1213	rBV	1507784	1886282	99.89%	13.015%
13	9.881	1319	1324	1329	rBV	534761	660796	34.99%	4.559%
14	9.975	1334	1340	1355	rBV	735345	1173952	62.17%	8.100%
15	10.669	1453	1458	1474	rBV	929927	1221711	64.69%	8.429%
16	11.369	1571	1577	1584	rBV	529896	689042	36.49%	4.754%
17	11.892	1659	1666	1680	rBV2	115734	203822	10.79%	1.406%
18	12.457	1749	1762	1770	rBV4	28191	62093	3.29%	0.428%
19	12.675	1795	1799	1809	rBV2	21921	42955	2.27%	0.296%
20	12.951	1840	1846	1851	rBV	1497026	1888426	100.00%	13.029%
21	13.186	1880	1886	1896	rVB6	8081	21771	1.15%	0.150%
22	13.869	1994	2002	2015	rBV	63678	177069	9.38%	1.222%
23	14.004	2020	2025	2035	rVB	330460	428927	22.71%	2.959%
24	14.845	2164	2168	2176	rVB	19690	26512	1.40%	0.183%
25	15.474	2269	2275	2284	rBV	225853	351364	18.61%	2.424%
26	16.033	2364	2370	2375	rBV6	12661	32216	1.71%	0.222%




Sum of corrected areas: 14493591

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138717.D
Acq On : 01 Aug 2024 11:19
Operator : RC/JU
Sample : P3379-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-01-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

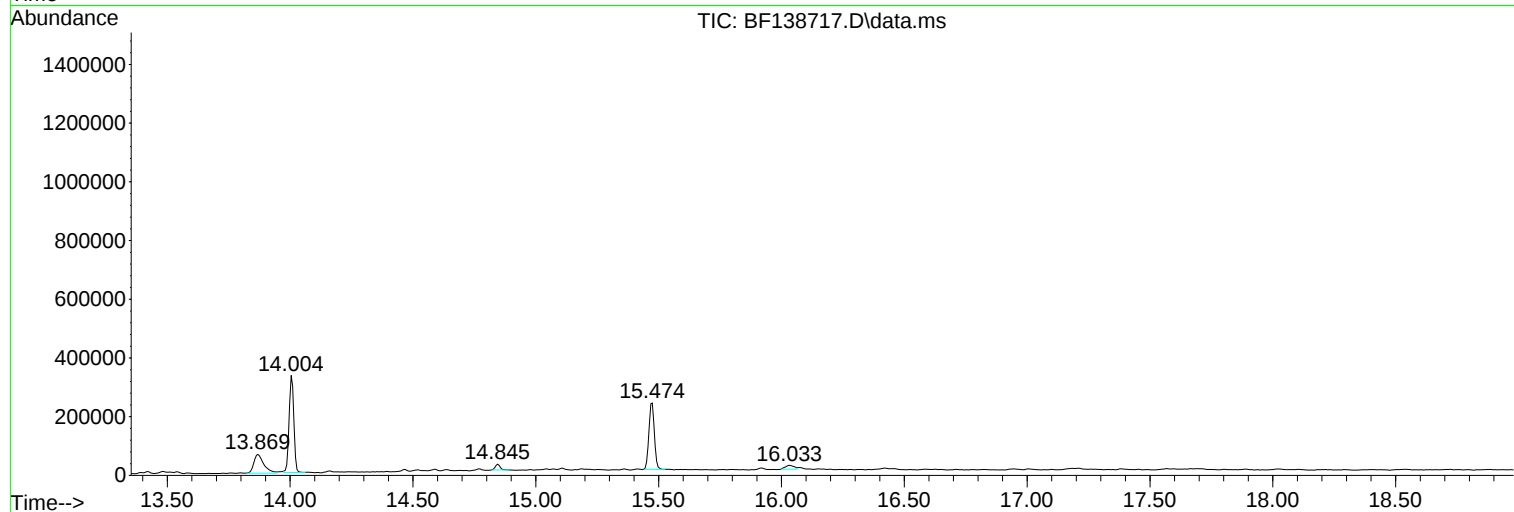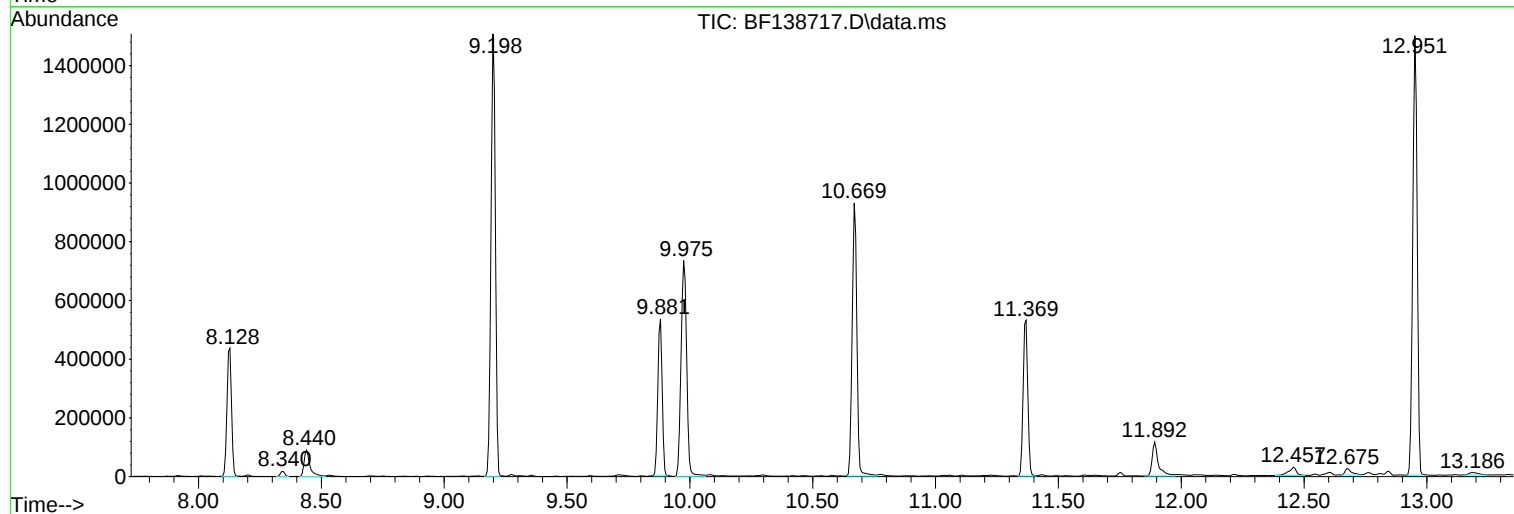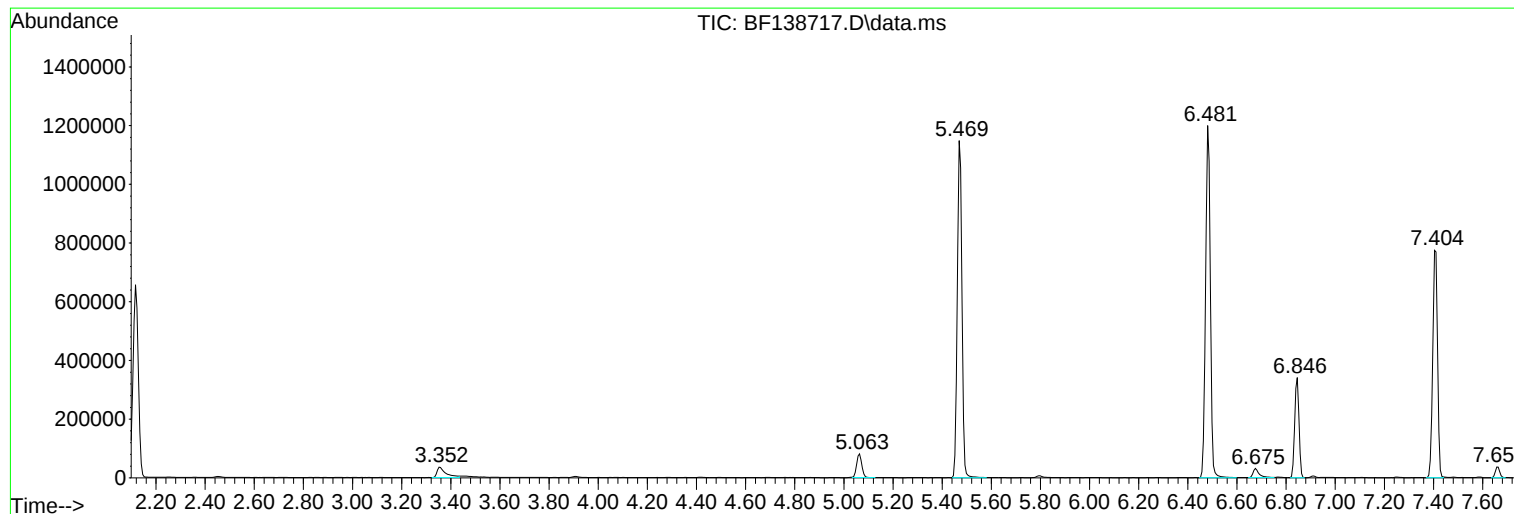

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138717.D
Acq On : 01 Aug 2024 11:19
Operator : RC/JU
Sample : P3379-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-01-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138717.D
Acq On : 01 Aug 2024 11:19
Operator : RC/JU
Sample : P3379-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-01-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------