

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138720.D
 Acq On : 01 Aug 2024 12:51
 Operator : RC/JU
 Sample : P3379-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-02-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138720.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.051	498	503	517	rVB	32462	47429	2.81%	0.493%
2	5.469	569	574	592	rBV	530352	714135	42.32%	7.424%
3	6.481	740	746	763	rBV	641608	851519	50.46%	8.852%
4	6.845	802	808	813	rBV	333568	421355	24.97%	4.380%
5	7.404	897	903	914	rBV	429426	540647	32.04%	5.620%
6	8.122	1020	1025	1031	rBV	453516	574134	34.02%	5.968%
7	8.439	1074	1079	1091	rBV	26589	45511	2.70%	0.473%
8	9.198	1202	1208	1213	rBV	999387	1223204	72.49%	12.715%
9	9.875	1318	1323	1329	rBV	536461	676416	40.08%	7.031%
10	9.969	1334	1339	1345	rBV	37920	56315	3.34%	0.585%
11	10.669	1452	1458	1473	rBV	918234	1187823	70.39%	12.348%
12	11.363	1571	1576	1582	rBV	535066	662095	39.24%	6.883%
13	11.892	1660	1666	1680	rBV2	29657	60297	3.57%	0.627%
14	12.951	1840	1846	1851	rBV	1277066	1687492	100.00%	17.542%
15	13.863	1993	2001	2014	rBV	41822	119320	7.07%	1.240%
16	14.004	2019	2025	2034	rVB	282126	368372	21.83%	3.829%
17	14.845	2163	2168	2173	rBV	16513	23842	1.41%	0.248%
18	15.468	2268	2274	2283	rBV	229354	359914	21.33%	3.741%




Sum of corrected areas: 9619820

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138720.D
Acq On : 01 Aug 2024 12:51
Operator : RC/JU
Sample : P3379-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

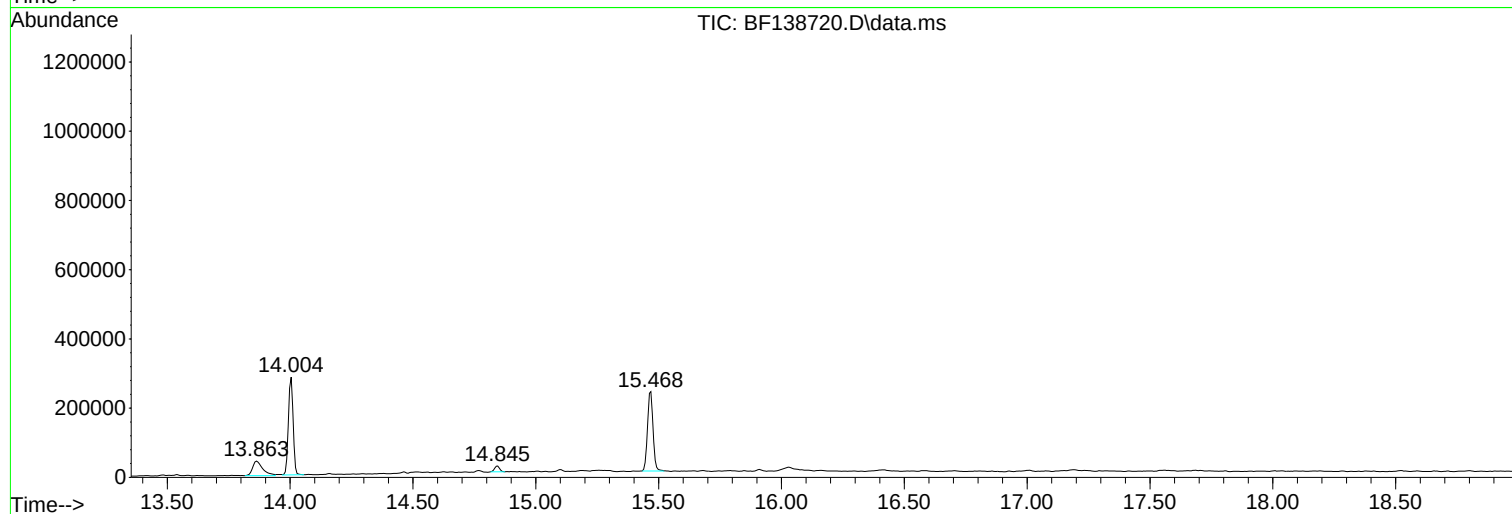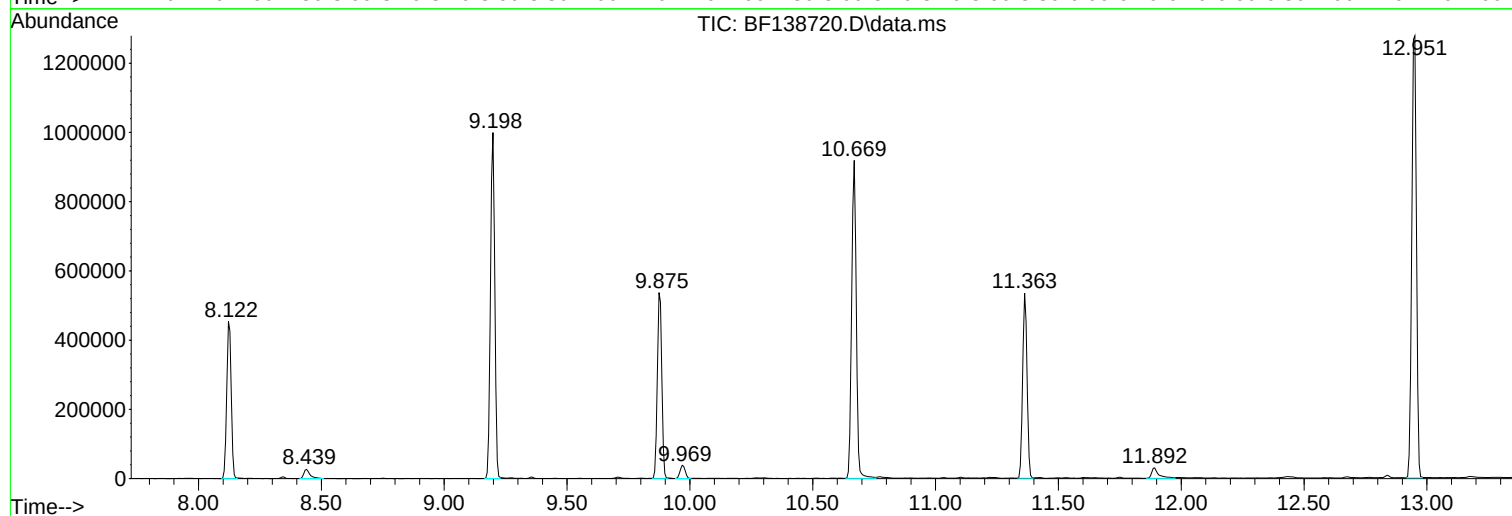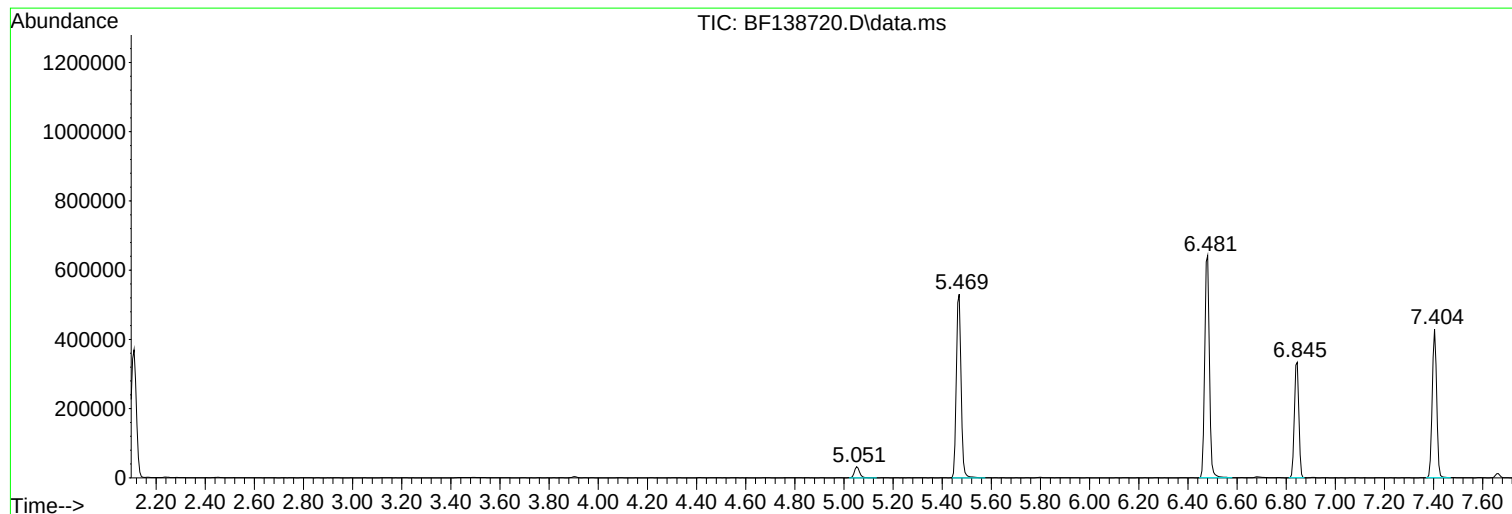

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138720.D
Acq On : 01 Aug 2024 12:51
Operator : RC/JU
Sample : P3379-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138720.D
Acq On : 01 Aug 2024 12:51
Operator : RC/JU
Sample : P3379-03
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-02-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------