

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138721.D
 Acq On : 01 Aug 2024 13:21
 Operator : RC/JU
 Sample : P3379-05
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-03-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138721.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	5	12	rVB	757999	894397	49.58%	6.917%
2	3.381	214	219	235	rBV2	6476	25790	1.43%	0.199%
3	5.063	500	505	515	rVB	70796	106826	5.92%	0.826%
4	5.469	569	574	590	rBV	1089297	1407835	78.05%	10.888%
5	6.481	740	746	767	rVB	1147064	1508059	83.60%	11.664%
6	6.845	803	808	813	rBV	349108	434683	24.10%	3.362%
7	7.404	897	903	912	rBV	736733	977992	54.22%	7.564%
8	7.657	942	946	952	rBV	19710	25130	1.39%	0.194%
9	8.122	1020	1025	1036	rBV	471287	599574	33.24%	4.637%
10	8.439	1074	1079	1087	rBV	29558	46892	2.60%	0.363%
11	9.198	1202	1208	1213	rBV	1470423	1803820	100.00%	13.951%
12	9.874	1318	1323	1329	rBV	544884	700733	38.85%	5.420%
13	9.969	1334	1339	1348	rBV	46552	69296	3.84%	0.536%
14	10.669	1452	1458	1473	rBV	816494	1066793	59.14%	8.251%
15	11.363	1571	1576	1584	rBV	563463	699424	38.77%	5.409%
16	11.892	1661	1666	1680	rBV2	24546	48676	2.70%	0.376%
17	12.951	1840	1846	1851	rBV	1204454	1578527	87.51%	12.209%
18	13.862	1994	2001	2018	rBV	51144	144686	8.02%	1.119%
19	14.004	2020	2025	2032	rVB	295371	377982	20.95%	2.923%
20	15.468	2268	2274	2284	rBV	243541	374211	20.75%	2.894%
21	16.033	2362	2370	2379	rBV6	11218	38255	2.12%	0.296%




Sum of corrected areas: 12929581

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138721.D
Acq On : 01 Aug 2024 13:21
Operator : RC/JU
Sample : P3379-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-03-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

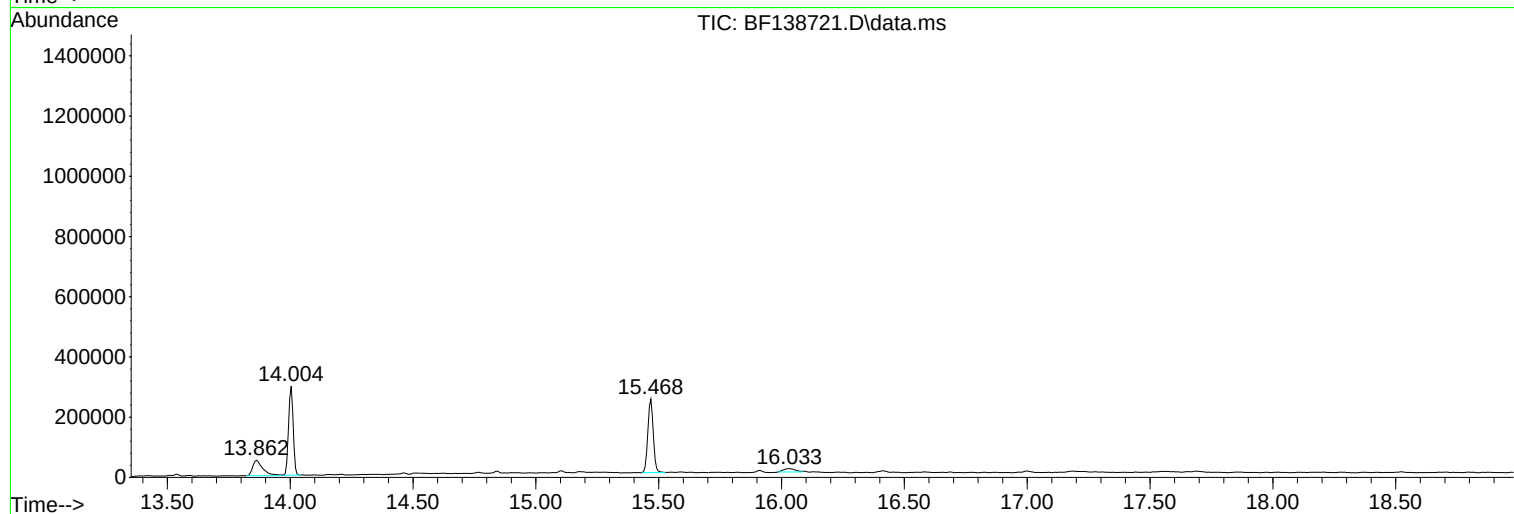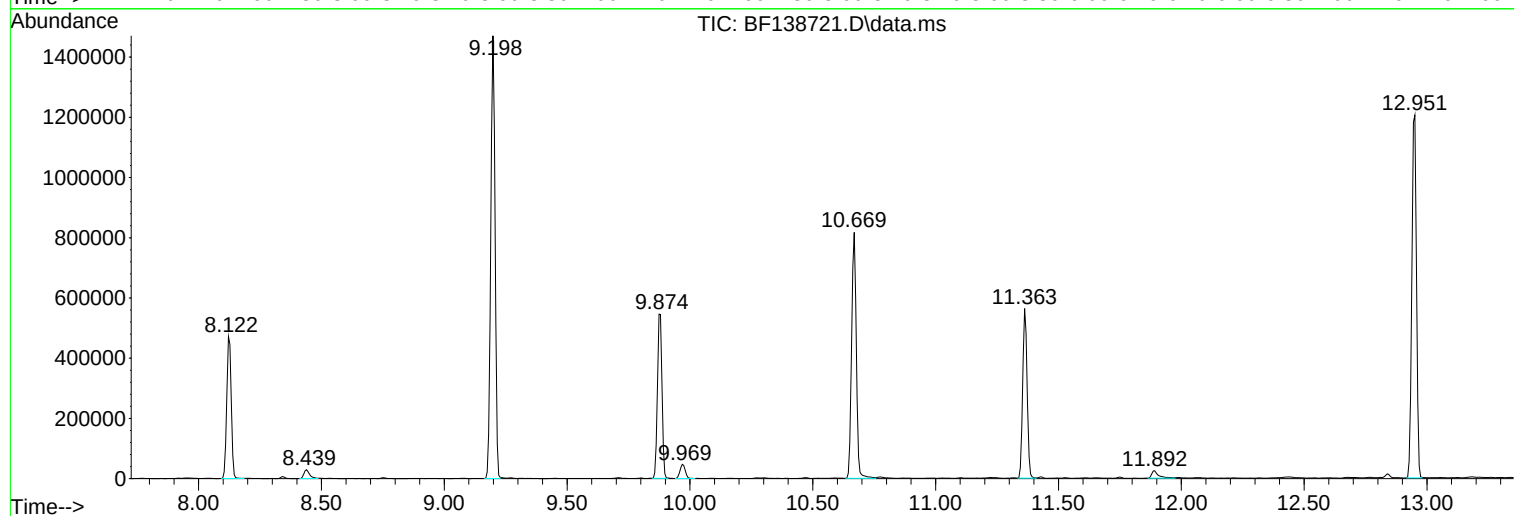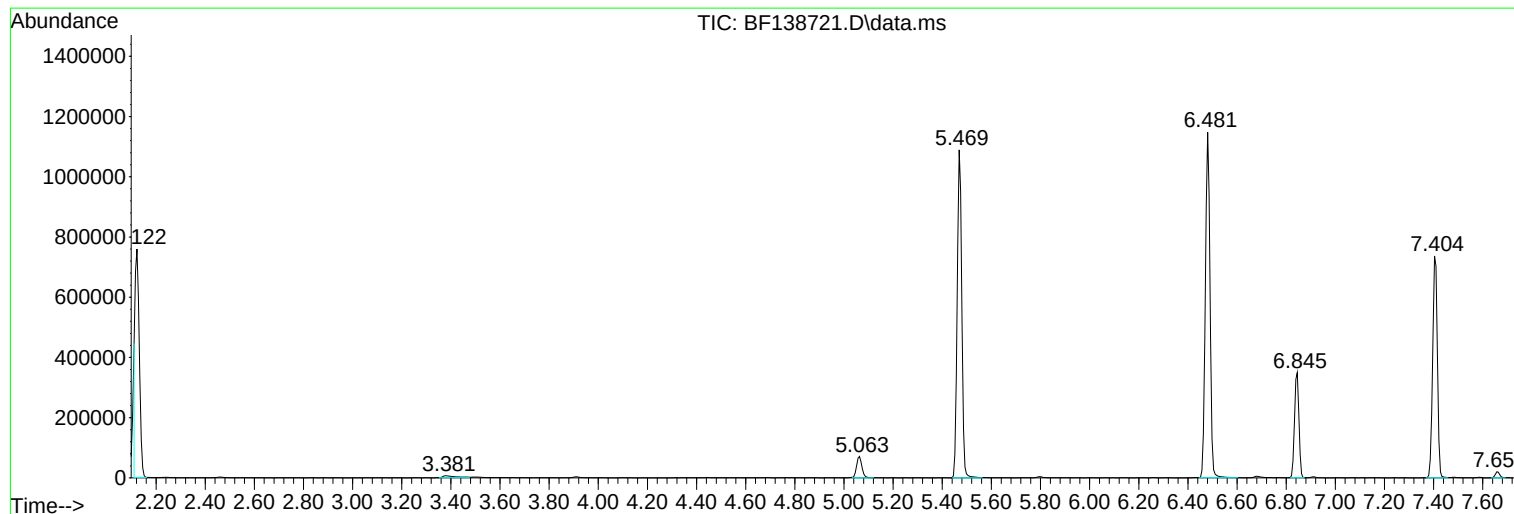

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138721.D
Acq On : 01 Aug 2024 13:21
Operator : RC/JU
Sample : P3379-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-03-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138721.D
Acq On : 01 Aug 2024 13:21
Operator : RC/JU
Sample : P3379-05
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-03-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------