

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138722.D
 Acq On : 01 Aug 2024 13:53
 Operator : RC/JU
 Sample : P3379-07
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-04-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138722.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	5	12	rVB	831648	968720	50.91%	6.989%
2	3.369	213	217	235	rBV	8901	31909	1.68%	0.230%
3	5.063	500	505	518	rVB	74226	110771	5.82%	0.799%
4	5.469	569	574	590	rBV	1152431	1492026	78.41%	10.765%
5	6.481	740	746	764	rBV	1223500	1615699	84.91%	11.657%
6	6.846	802	808	813	rBV	370636	471565	24.78%	3.402%
7	7.404	897	903	908	rBV	794359	1042258	54.77%	7.520%
8	7.657	942	946	955	rVB	21266	27212	1.43%	0.196%
9	8.122	1020	1025	1031	rBV	519809	657835	34.57%	4.746%
10	8.440	1074	1079	1089	rBV	31084	51854	2.72%	0.374%
11	9.198	1202	1208	1213	rBV	1533782	1902944	100.00%	13.729%
12	9.875	1318	1323	1334	rVB	601405	764814	40.19%	5.518%
13	9.969	1334	1339	1347	rVB	42368	64760	3.40%	0.467%
14	10.669	1452	1458	1472	rBV	881102	1156174	60.76%	8.342%
15	11.363	1571	1576	1583	rBV	619585	757163	39.79%	5.463%
16	11.892	1661	1666	1680	rBV2	30167	58059	3.05%	0.419%
17	12.945	1840	1845	1850	rBV	1325596	1701467	89.41%	12.276%
18	13.863	1993	2001	2016	rBV3	46711	138212	7.26%	0.997%
19	14.004	2020	2025	2030	rVB	315323	403411	21.20%	2.911%
20	15.468	2267	2274	2282	rVB	259956	404462	21.25%	2.918%
21	16.033	2363	2370	2383	rVB	10640	38971	2.05%	0.281%




Sum of corrected areas: 13860286

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138722.D
Acq On : 01 Aug 2024 13:53
Operator : RC/JU
Sample : P3379-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-04-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

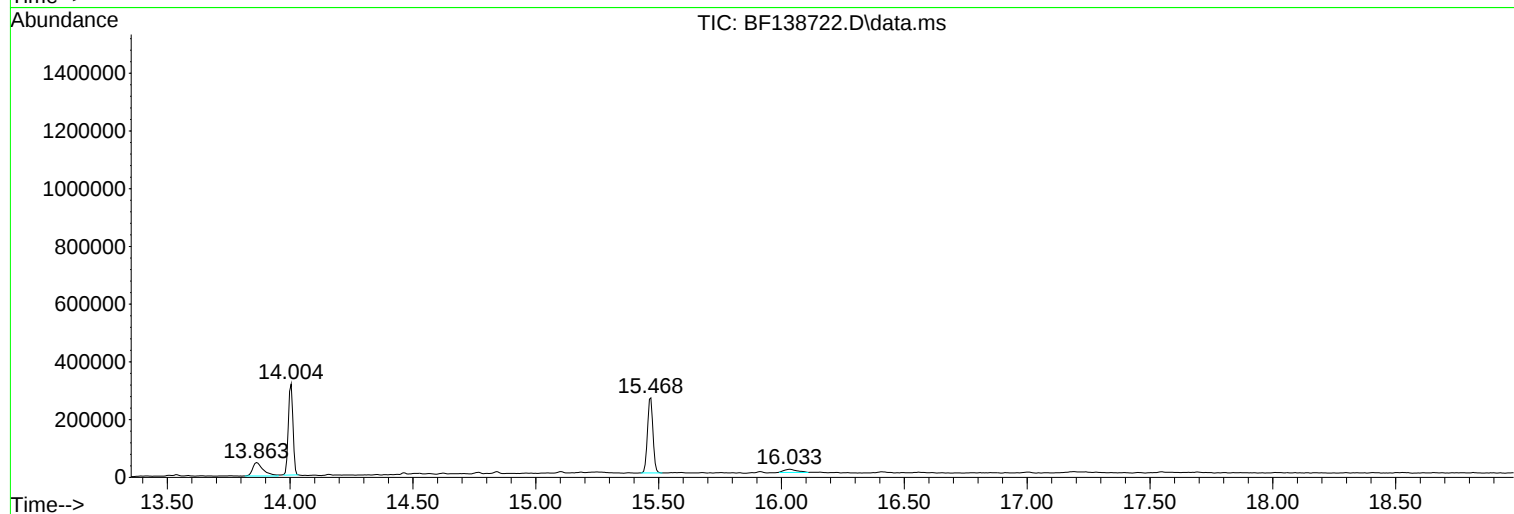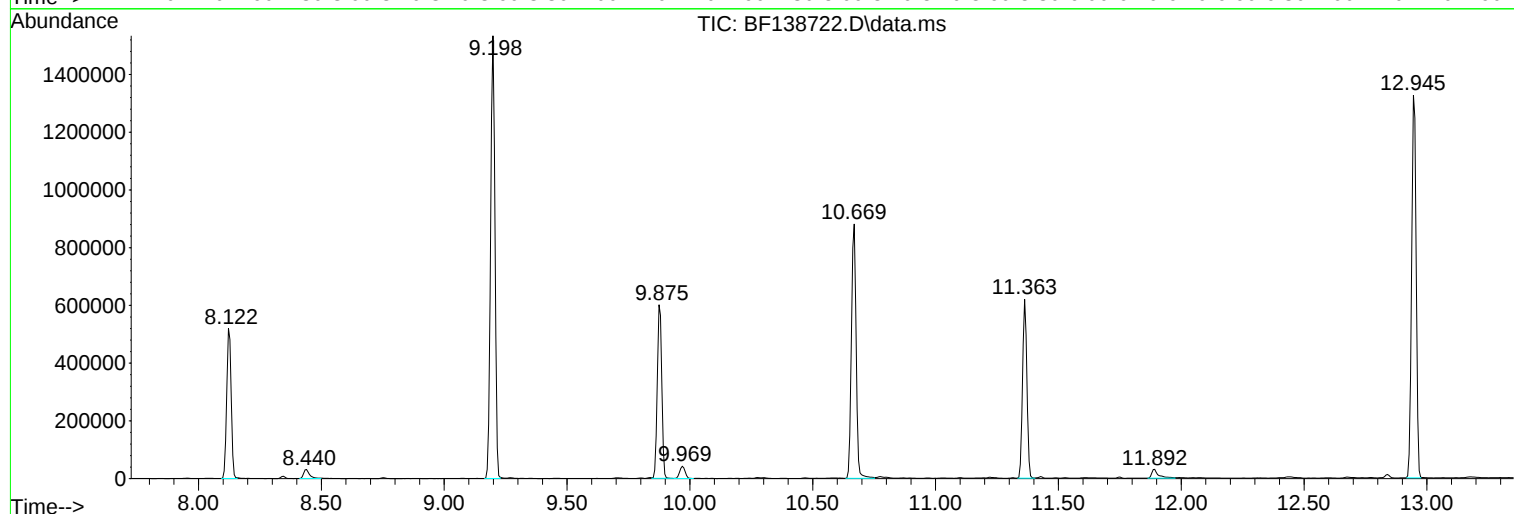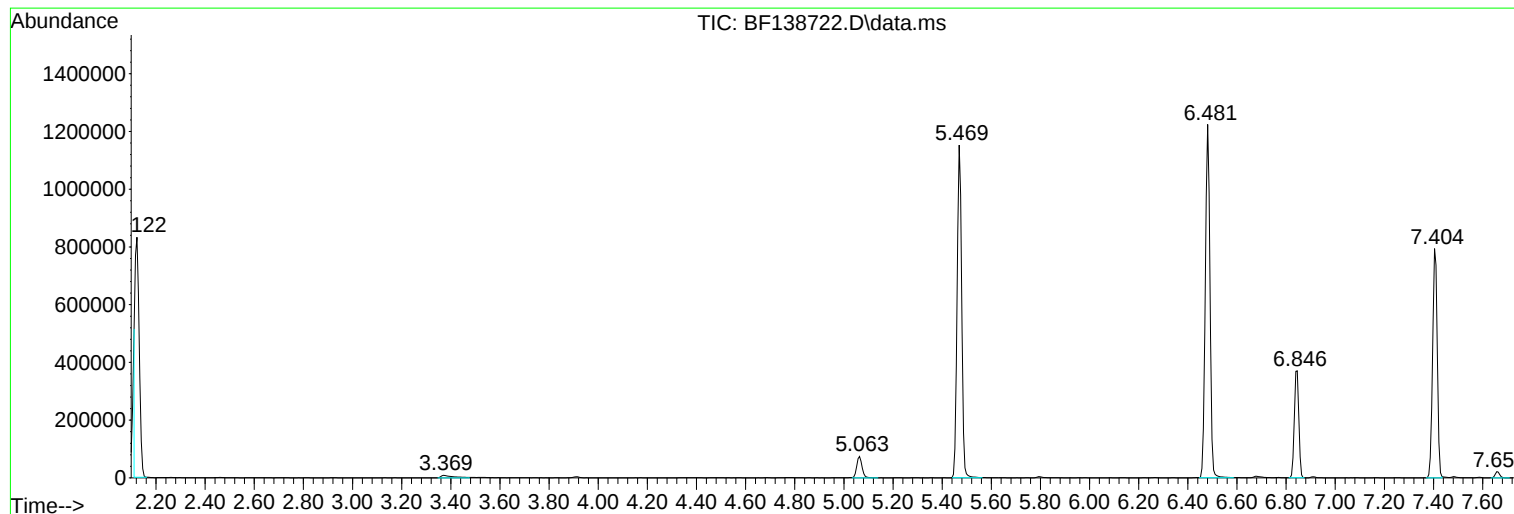

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138722.D
Acq On : 01 Aug 2024 13:53
Operator : RC/JU
Sample : P3379-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-04-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138722.D
Acq On : 01 Aug 2024 13:53
Operator : RC/JU
Sample : P3379-07
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-04-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------