

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138724.D
 Acq On : 01 Aug 2024 14:54
 Operator : RC/JU
 Sample : P3379-11
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-01-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138724.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	5	20	rVB	795413	954637	49.14%	7.203%
2	3.369	213	217	235	rBV	8930	30464	1.57%	0.230%
3	5.063	500	505	524	rVB	78017	117070	6.03%	0.883%
4	5.469	569	574	590	rBV	1188759	1564500	80.53%	11.805%
5	6.481	740	746	766	rBV	1262292	1683518	86.65%	12.703%
6	6.845	803	808	813	rVB	352919	444020	22.85%	3.350%
7	7.404	897	903	913	rBV	831800	1113930	57.34%	8.405%
8	7.657	942	946	954	rVB	23851	30930	1.59%	0.233%
9	8.122	1020	1025	1034	rBV	492396	620016	31.91%	4.678%
10	8.439	1074	1079	1093	rBV	34685	59945	3.09%	0.452%
11	9.198	1202	1208	1213	rBV	1562763	1942800	100.00%	14.659%
12	9.875	1318	1323	1329	rBV	554435	695708	35.81%	5.249%
13	9.969	1334	1339	1348	rBV	43481	65557	3.37%	0.495%
14	10.669	1452	1458	1473	rBV	806865	1058259	54.47%	7.985%
15	11.363	1571	1576	1585	rBV	513869	634988	32.68%	4.791%
16	11.892	1661	1666	1679	rBV2	28203	52253	2.69%	0.394%
17	12.839	1821	1827	1834	rVB	19831	25262	1.30%	0.191%
18	12.945	1840	1845	1850	rBV	1003727	1276484	65.70%	9.632%
19	13.863	1995	2001	2018	rBV2	33497	107463	5.53%	0.811%
20	14.004	2020	2025	2032	rVB	284138	359731	18.52%	2.714%
21	14.839	2164	2167	2175	rVB	13535	20652	1.06%	0.156%
22	15.468	2268	2274	2280	rBV	260511	394682	20.32%	2.978%




Sum of corrected areas: 13252869

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138724.D
Acq On : 01 Aug 2024 14:54
Operator : RC/JU
Sample : P3379-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-01-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

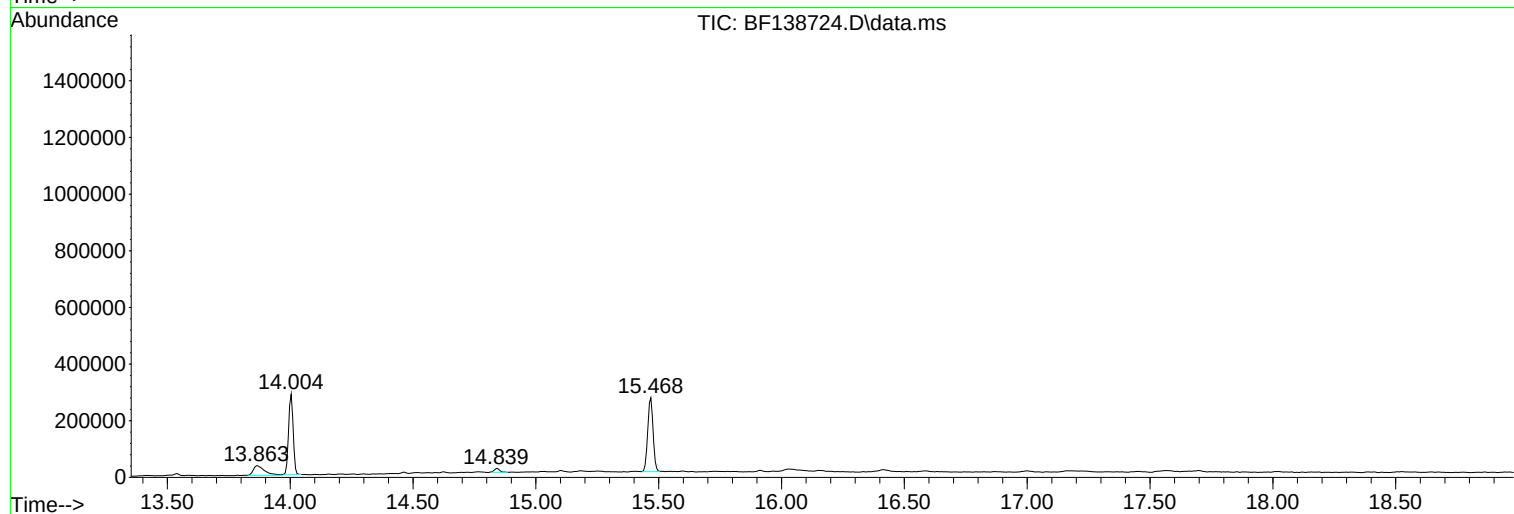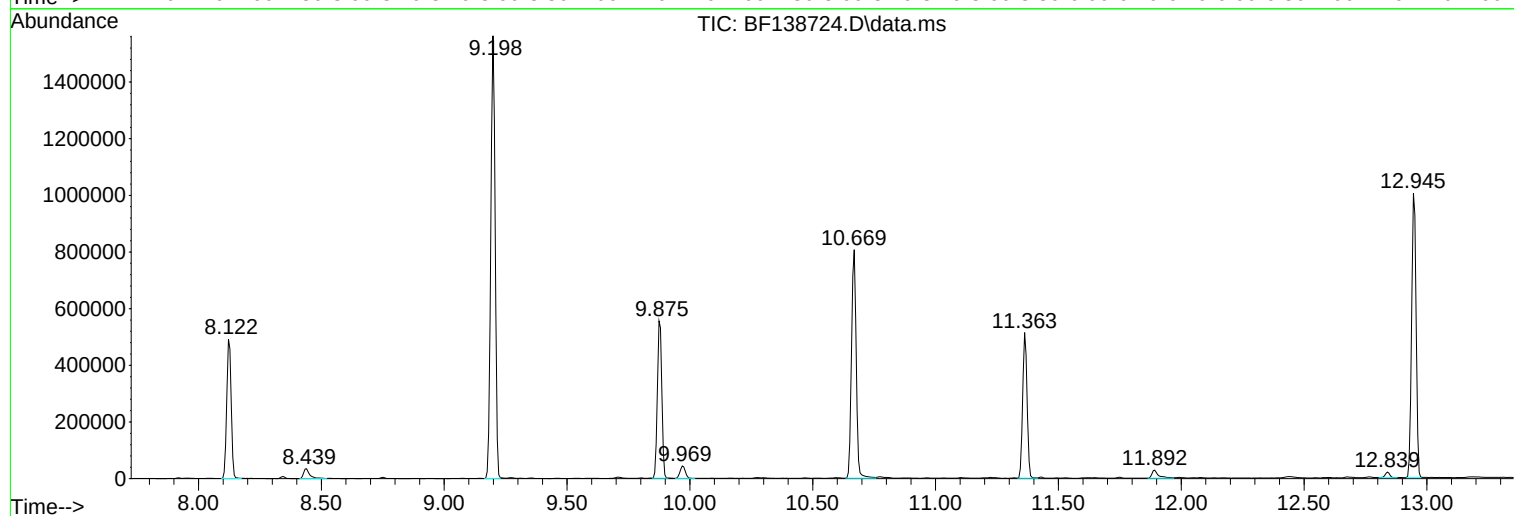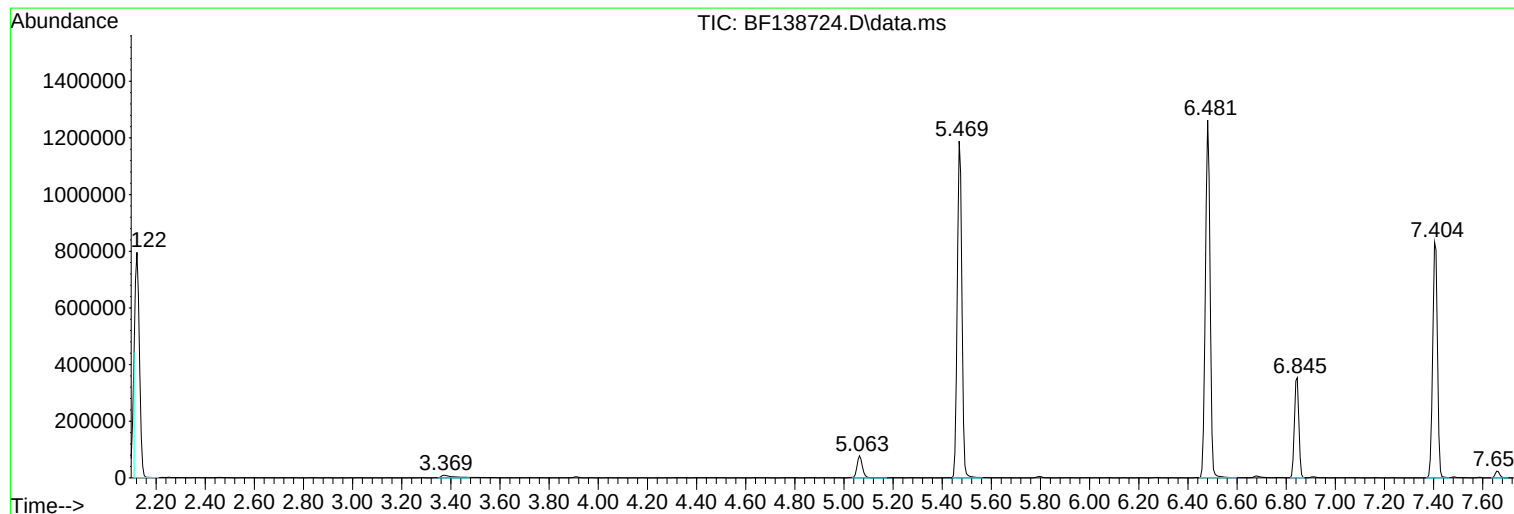

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138724.D
Acq On : 01 Aug 2024 14:54
Operator : RC/JU
Sample : P3379-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-01-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138724.D
Acq On : 01 Aug 2024 14:54
Operator : RC/JU
Sample : P3379-11
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-01-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------