

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138725.D
 Acq On : 01 Aug 2024 15:25
 Operator : RC/JU
 Sample : P3379-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-02-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138725.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	3	6	17	rVB	832377	1154797	57.95%	8.442%
2	3.387	215	220	233	rBV	5746	20416	1.02%	0.149%
3	5.063	495	505	513	rBV	80359	129942	6.52%	0.950%
4	5.469	569	574	590	rBV	1227643	1669976	83.80%	12.208%
5	6.481	740	746	769	rVB	1325719	1771235	88.88%	12.948%
6	6.845	803	808	813	rBV	358281	451551	22.66%	3.301%
7	7.410	897	904	913	rBV	859404	1170652	58.75%	8.558%
8	7.657	942	946	957	rVB	25565	32577	1.63%	0.238%
9	8.122	1020	1025	1031	rBV	491515	622171	31.22%	4.548%
10	8.439	1074	1079	1093	rBV	33163	59126	2.97%	0.432%
11	9.198	1202	1208	1213	rBV	1616646	1992728	100.00%	14.567%
12	9.875	1318	1323	1334	rVB	551877	694539	34.85%	5.077%
13	9.969	1334	1339	1346	rVB	39492	58735	2.95%	0.429%
14	10.669	1452	1458	1473	rBV	823761	1069810	53.69%	7.820%
15	11.363	1571	1576	1582	rBV	497867	605959	30.41%	4.430%
16	11.892	1661	1666	1678	rBV2	30470	60158	3.02%	0.440%
17	12.945	1840	1845	1850	rBV	982081	1232172	61.83%	9.007%
18	13.869	1995	2002	2016	rBV2	37141	113636	5.70%	0.831%
19	14.004	2020	2025	2032	rVB	270637	350660	17.60%	2.563%
20	14.839	2163	2167	2173	rVB	14978	22225	1.12%	0.162%
21	15.468	2268	2274	2283	rBV	252573	396541	19.90%	2.899%




Sum of corrected areas: 13679606

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138725.D
Acq On : 01 Aug 2024 15:25
Operator : RC/JU
Sample : P3379-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-02-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

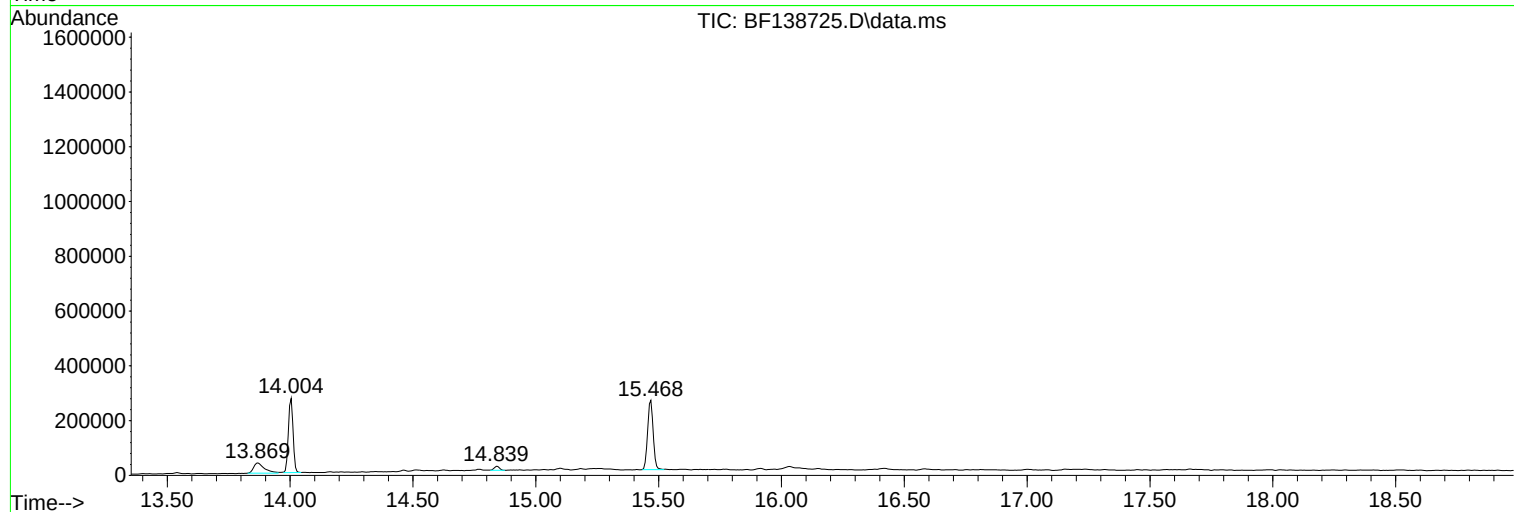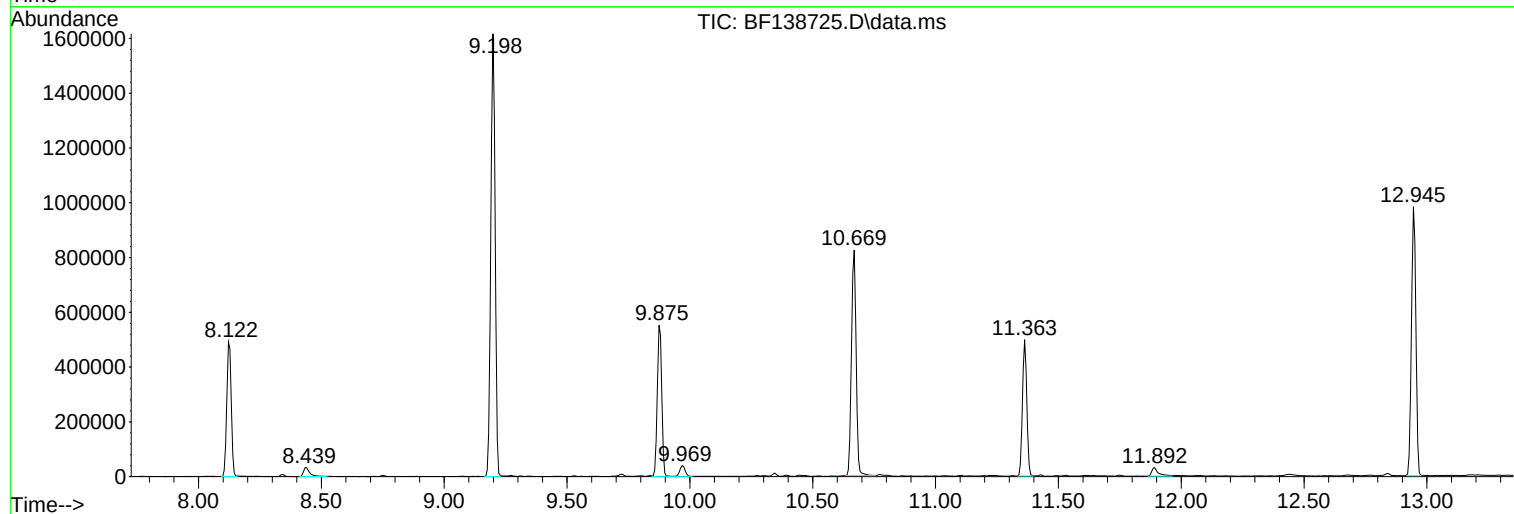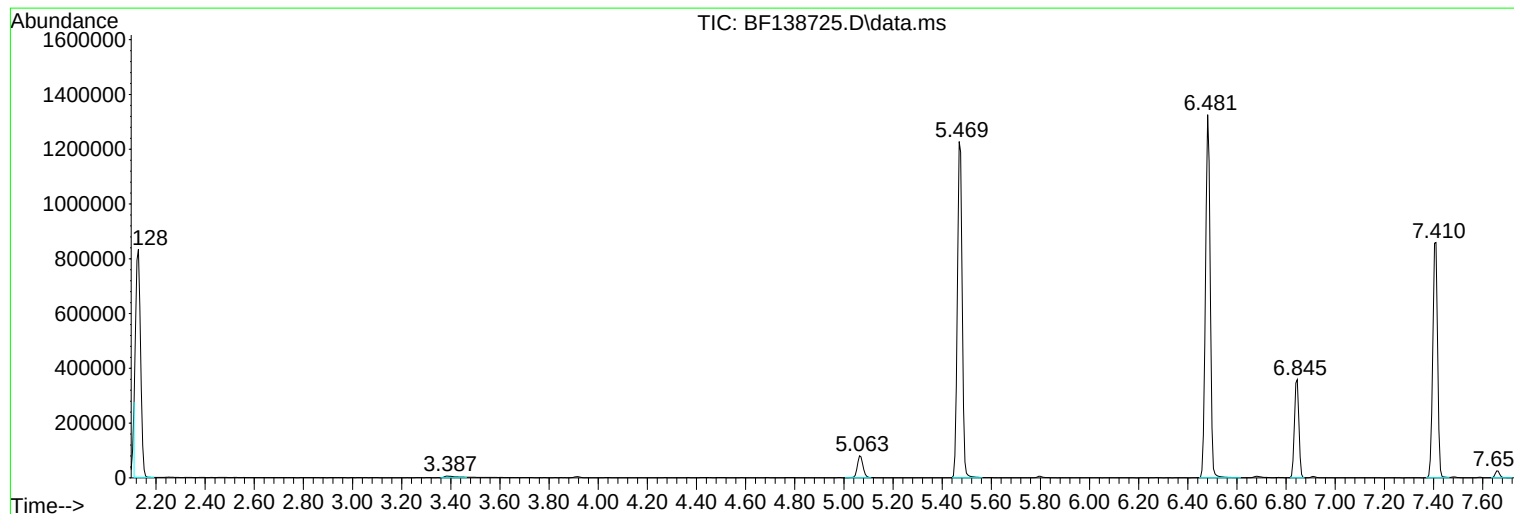

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138725.D
Acq On : 01 Aug 2024 15:25
Operator : RC/JU
Sample : P3379-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-02-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138725.D
Acq On : 01 Aug 2024 15:25
Operator : RC/JU
Sample : P3379-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-02-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------