

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138726.D
 Acq On : 01 Aug 2024 15:57
 Operator : RC/JU
 Sample : P3379-15
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-03-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138726.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.057	499	504	512	rVB	66375	96139	6.24%	0.950%
2	5.469	568	574	592	rBV	995249	1281429	83.19%	12.666%
3	6.481	740	746	767	rBV	1039494	1346251	87.39%	13.307%
4	6.840	803	807	813	rBV	346174	441684	28.67%	4.366%
5	7.404	897	903	908	rBV	700162	888867	57.70%	8.786%
6	7.657	942	946	954	rVB	20067	25810	1.68%	0.255%
7	8.122	1020	1025	1031	rBV	486220	605427	39.30%	5.984%
8	8.440	1074	1079	1088	rBV	28416	49486	3.21%	0.489%
9	9.198	1202	1208	1213	rBV	1254571	1540427	100.00%	15.226%
10	9.875	1318	1323	1332	rVB	529706	659389	42.81%	6.518%
11	9.969	1334	1339	1348	rVB	34078	50184	3.26%	0.496%
12	10.669	1452	1458	1473	rBV	588058	795023	51.61%	7.858%
13	11.363	1571	1576	1581	rBV	452114	553918	35.96%	5.475%
14	11.886	1661	1665	1684	rBV3	13784	28355	1.84%	0.280%
15	12.945	1840	1845	1850	rBV	755043	931644	60.48%	9.209%
16	13.869	1994	2002	2016	rBV3	25076	83805	5.44%	0.828%
17	14.004	2020	2025	2033	rVB	267934	350240	22.74%	3.462%
18	15.469	2268	2274	2282	rVB	256100	389039	25.26%	3.845%




Sum of corrected areas: 10117117

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138726.D
Acq On : 01 Aug 2024 15:57
Operator : RC/JU
Sample : P3379-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-03-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

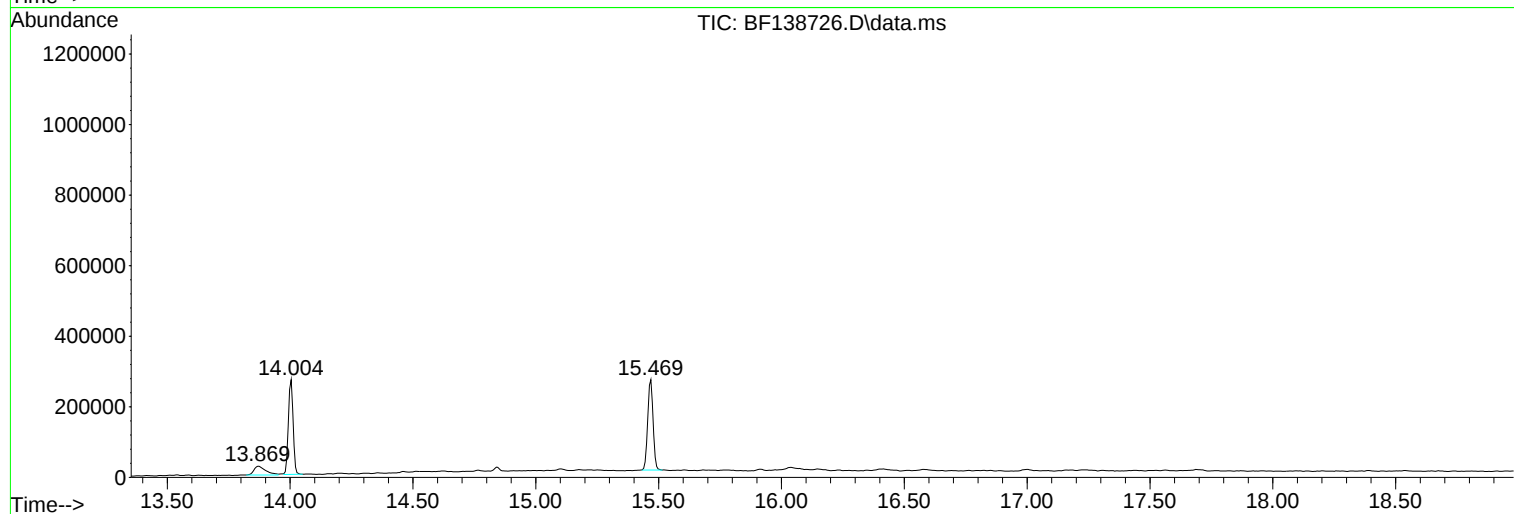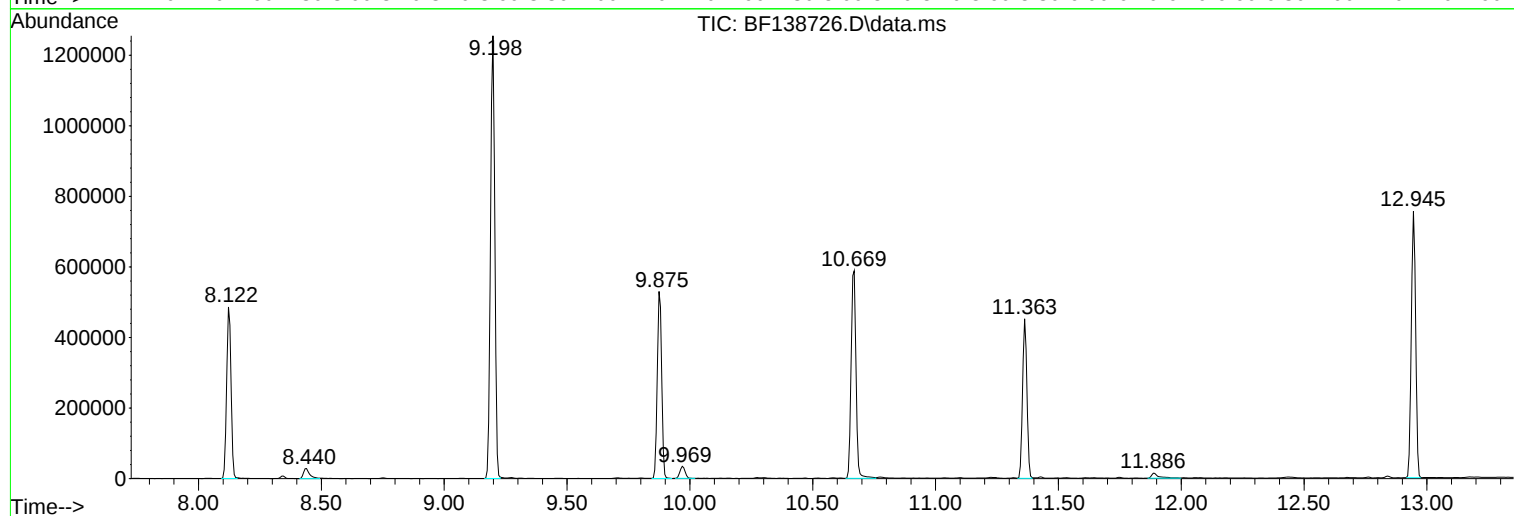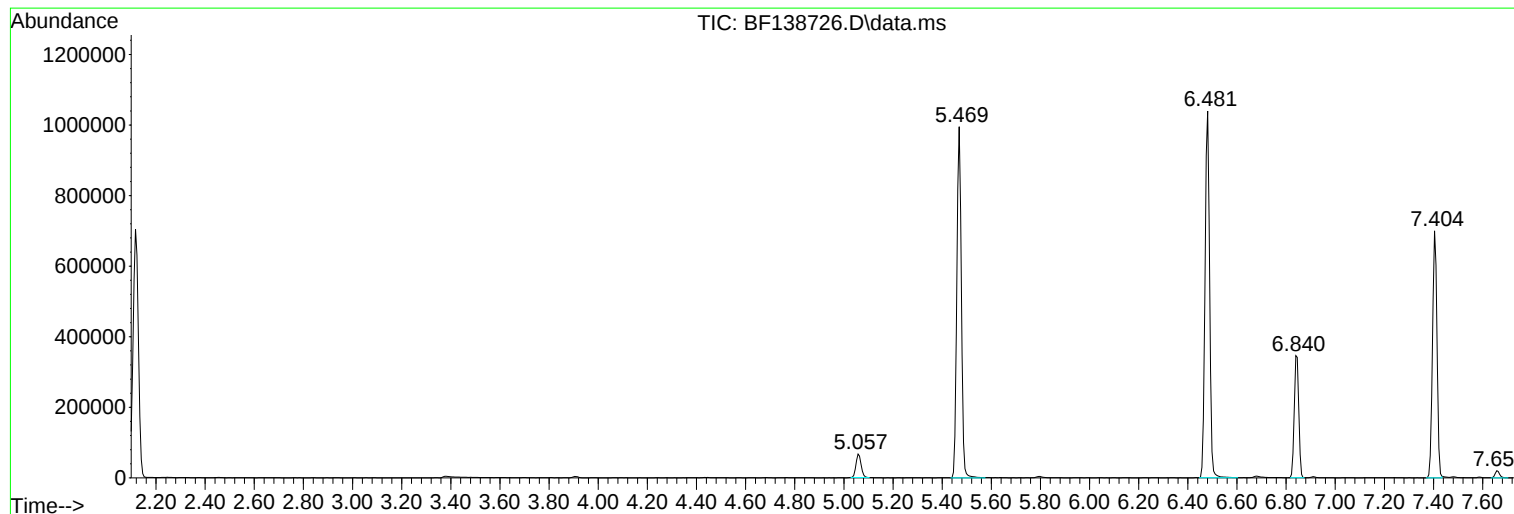

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138726.D
Acq On : 01 Aug 2024 15:57
Operator : RC/JU
Sample : P3379-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-03-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138726.D
Acq On : 01 Aug 2024 15:57
Operator : RC/JU
Sample : P3379-15
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-03-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------