

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138727.D
 Acq On : 01 Aug 2024 16:29
 Operator : RC/JU
 Sample : P3379-17
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-04-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138727.D\data.ms




peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.116	3	4	12	rVB	693161	782219	51.15%	7.289%
2	5.057	499	504	518	rVB	61644	95121	6.22%	0.886%
3	5.469	569	574	594	rBV	1023728	1317826	86.18%	12.280%
4	6.481	740	746	762	rBV	1053579	1366752	89.38%	12.736%
5	6.845	802	808	813	rBV	321201	404921	26.48%	3.773%
6	7.404	897	903	908	rBV	707831	901842	58.97%	8.404%
7	7.657	942	946	958	rVB	18697	25173	1.65%	0.235%
8	8.122	1020	1025	1034	rBV	439768	555867	36.35%	5.180%
9	8.439	1074	1079	1092	rBV	26607	46241	3.02%	0.431%
10	9.198	1202	1208	1213	rBV	1247396	1529215	100.00%	14.250%
11	9.875	1318	1323	1334	rVB	478261	602808	39.42%	5.617%
12	9.969	1334	1339	1346	rBV	36313	55427	3.62%	0.516%
13									

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138727.D
Acq On : 01 Aug 2024 16:29
Operator : RC/JU
Sample : P3379-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-04-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

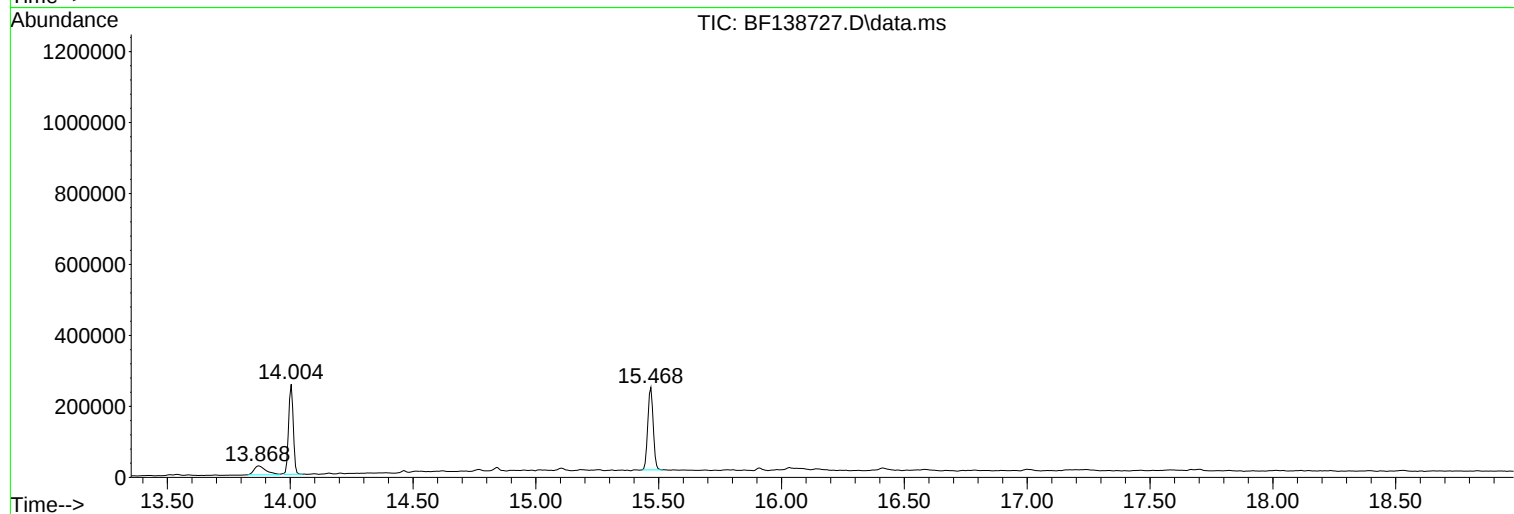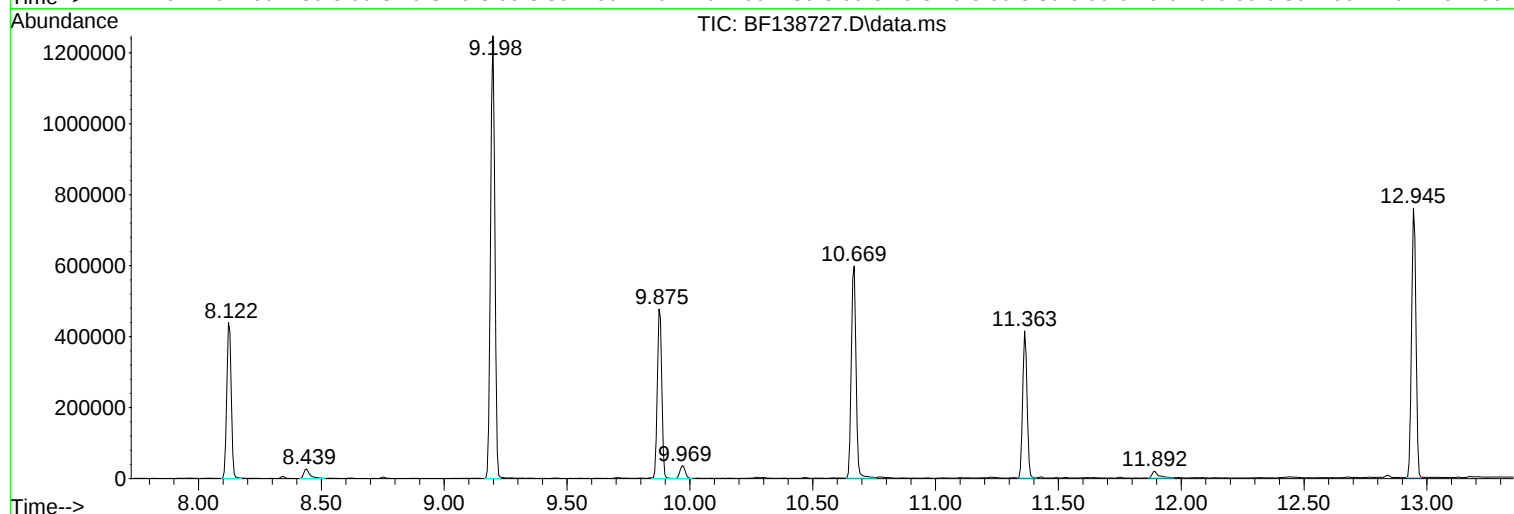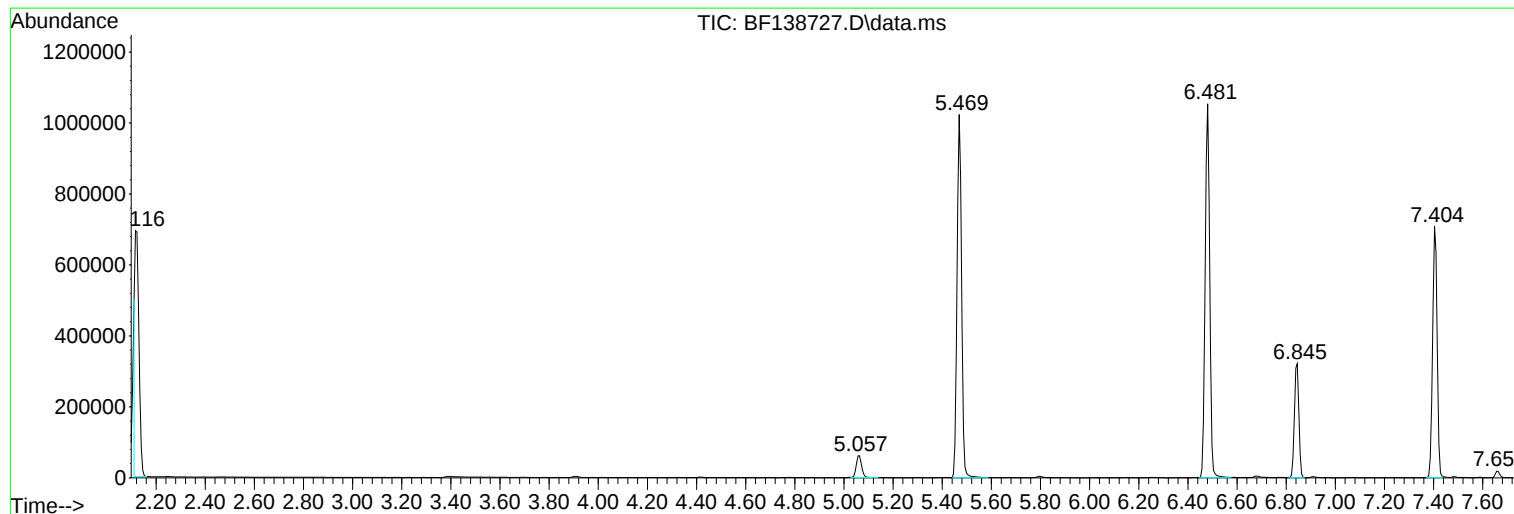

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138727.D
Acq On : 01 Aug 2024 16:29
Operator : RC/JU
Sample : P3379-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-04-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138727.D
Acq On : 01 Aug 2024 16:29
Operator : RC/JU
Sample : P3379-17
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-04-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------