

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
 Data File : BF138728.D
 Acq On : 01 Aug 2024 17:00
 Operator : RC/JU
 Sample : P3379-19
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-VSL-05-072324

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF138728.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.128	3	6	13	rVB	848070	1175514	70.92%	9.470%
2	5.063	500	505	516	rVB	71247	107051	6.46%	0.862%
3	5.469	569	574	595	rBV	1128057	1472083	88.82%	11.859%
4	6.481	740	746	762	rBV	1169692	1533140	92.50%	12.351%
5	6.845	803	808	813	rBV	375205	472777	28.53%	3.809%
6	7.404	897	903	912	rBV	765806	996023	60.10%	8.024%
7	7.657	942	946	955	rBV	22266	28844	1.74%	0.232%
8	8.122	1020	1025	1038	rBV	507518	640694	38.66%	5.161%
9	8.439	1074	1079	1093	rBV	31243	56160	3.39%	0.452%
10	9.198	1202	1208	1213	rBV	1364293	1657409	100.00%	13.352%
11	9.875	1318	1323	1329	rBV	539491	683016	41.21%	5.502%
12	9.969	1334	1339	1346	rBV	47271	72048	4.35%	0.580%
13	10.669	1452	1458	1473	rBV	657332	872685	52.65%	7.030%
14	11.363	1571	1576	1584	rBV	479595	588067	35.48%	4.737%
15	11.892	1661	1666	1679	rBV3	19154	41081	2.48%	0.331%
16	12.945	1840	1845	1850	rBV	848900	1089588	65.74%	8.778%
17	13.874	1995	2003	2017	rBV2	29329	103665	6.25%	0.835%
18	14.004	2020	2025	2035	rVB	306043	390733	23.57%	3.148%
19	15.468	2268	2274	2285	rBV	288458	432780	26.11%	3.486%




Sum of corrected areas: 12413358

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138728.D
Acq On : 01 Aug 2024 17:00
Operator : RC/JU
Sample : P3379-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-05-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

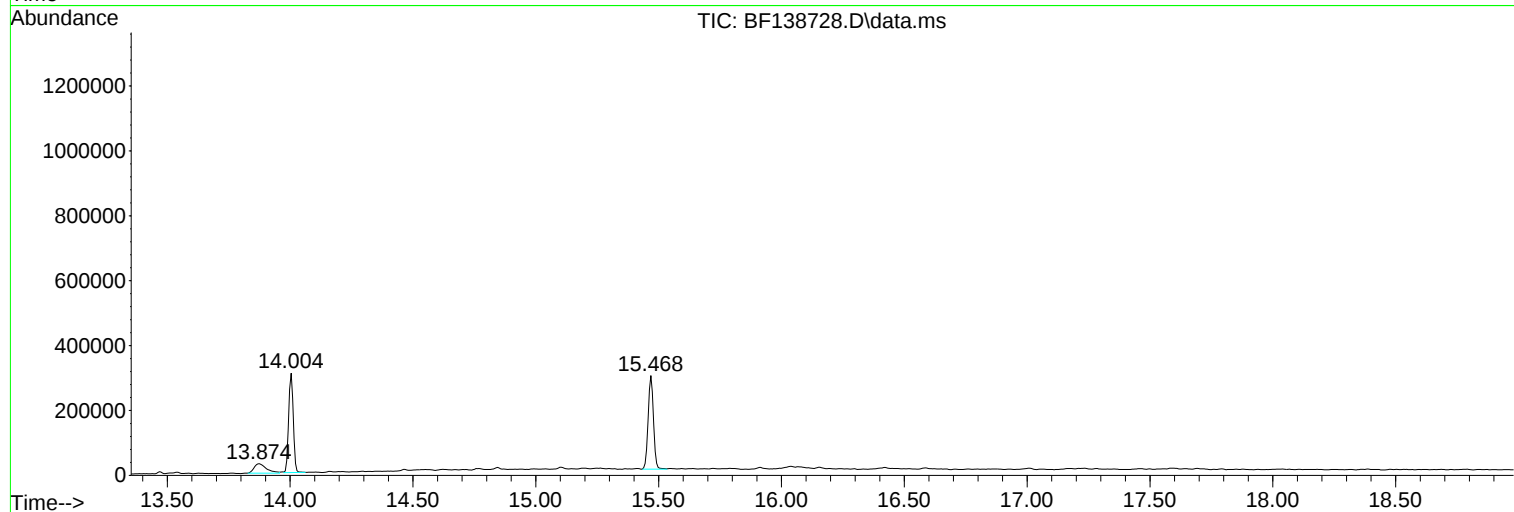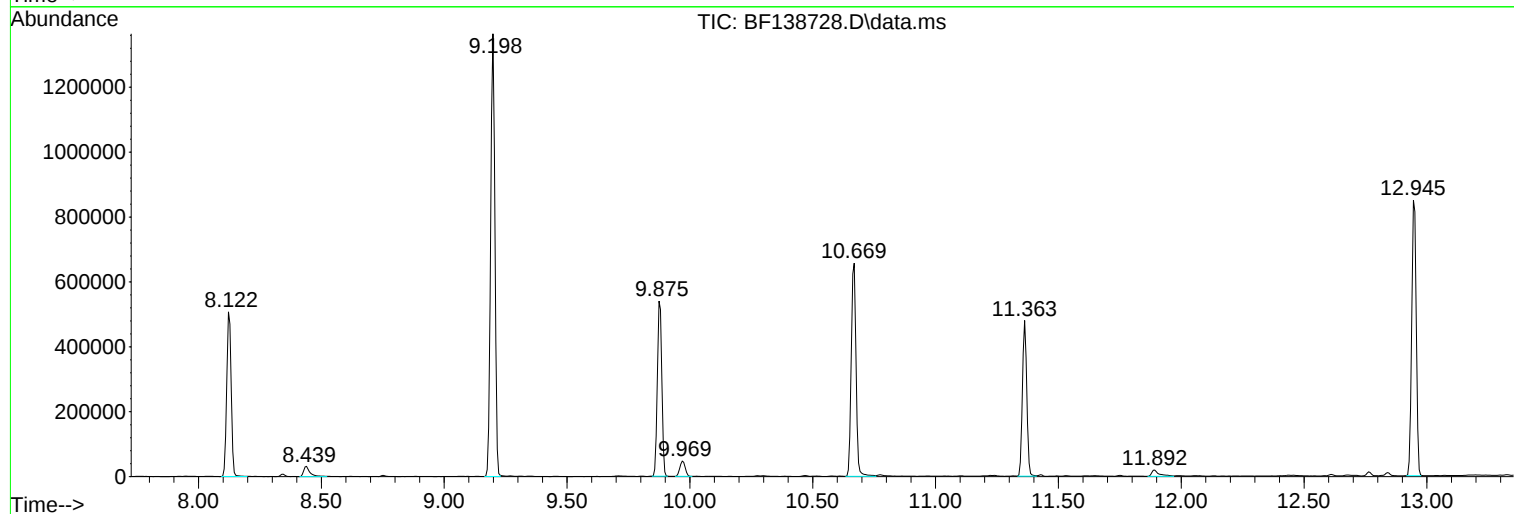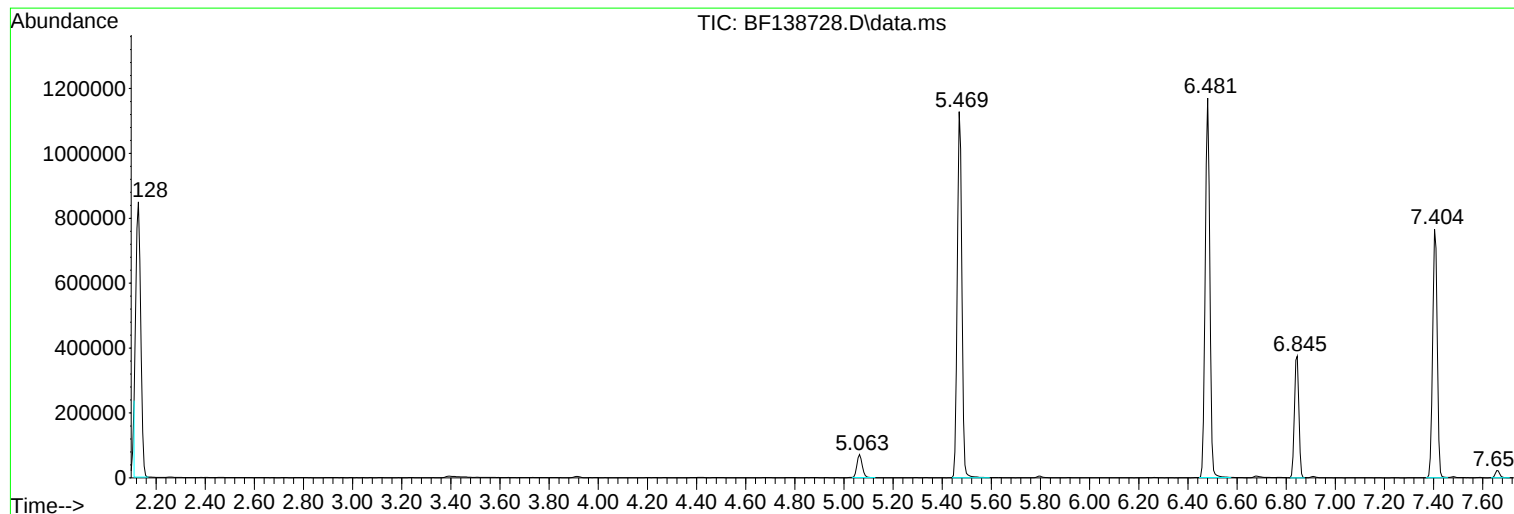

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138728.D
Acq On : 01 Aug 2024 17:00
Operator : RC/JU
Sample : P3379-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-05-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138728.D
Acq On : 01 Aug 2024 17:00
Operator : RC/JU
Sample : P3379-19
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-VSL-05-072324

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------