


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138713.D
Acq On : 01 Aug 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 30 17:50:01 2024

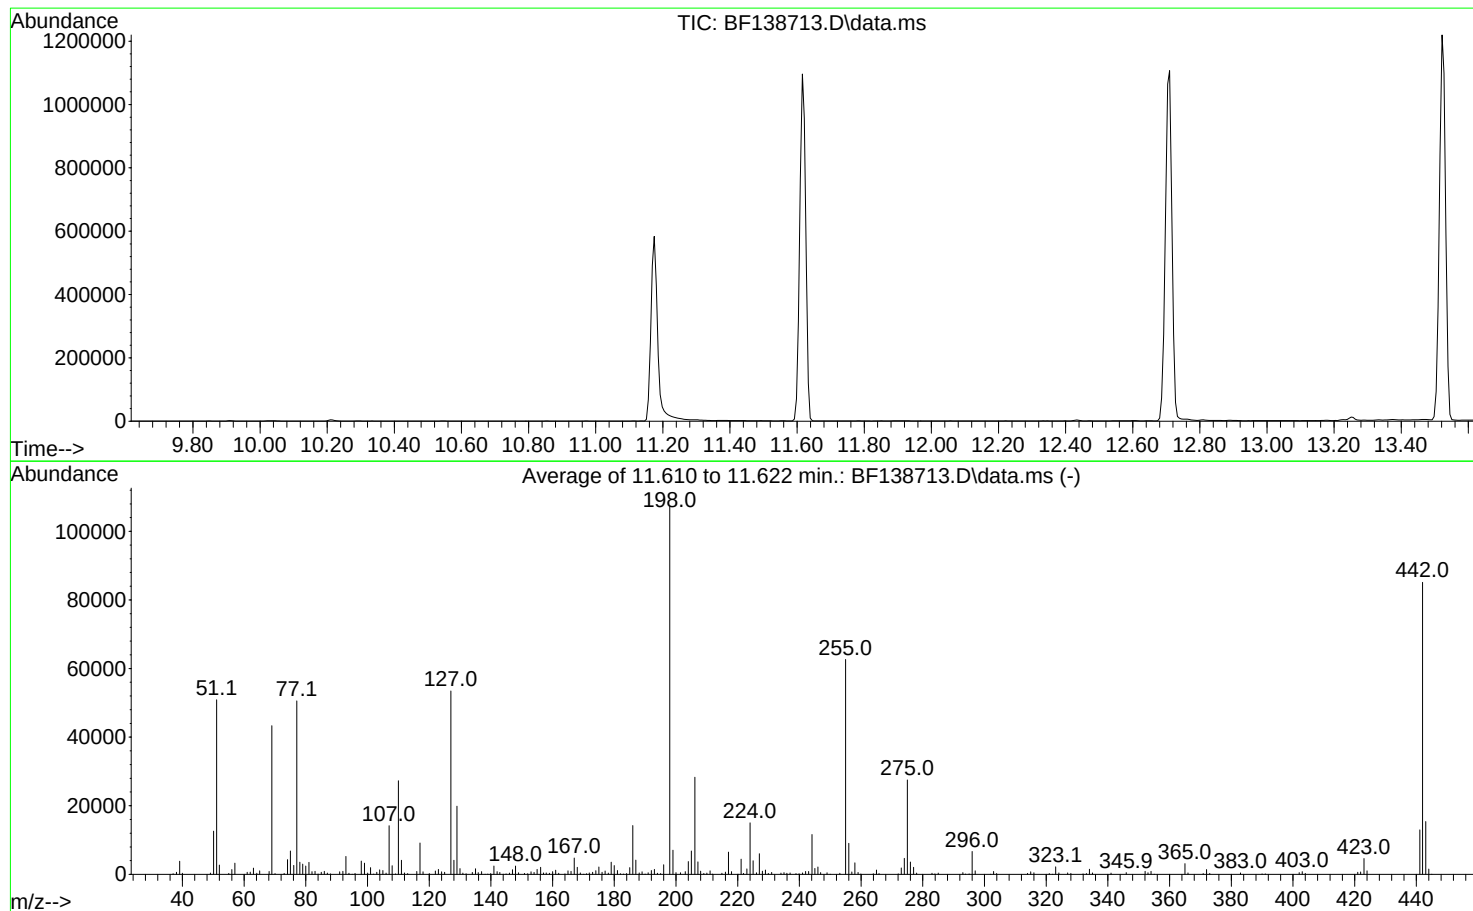




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1612

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	47.4	50880	PASS
68	69	0.00	2	1.9	835	PASS
69	198	0.00	100	40.4	43312	PASS
70	69	0.00	2	0.5	213	PASS
127	198	10	80	49.8	53437	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107237	PASS
199	198	5	9	6.6	7054	PASS
275	198	10	60	25.7	27515	PASS
365	198	1	100	2.9	3124	PASS
441	198	0.01	100	12.1	12979	PASS
442	442	50	100	100.0	85147	PASS
443	442	15	24	18.1	15392	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138713.D
Acq On : 01 Aug 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 01 11:04:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

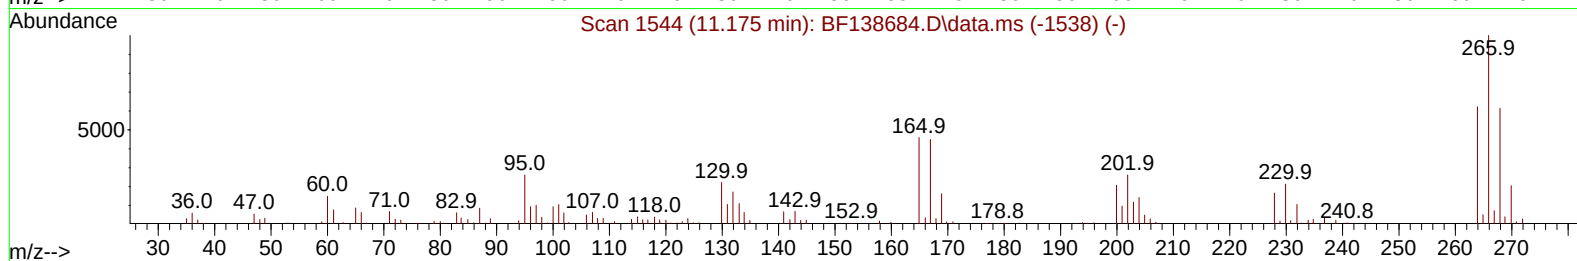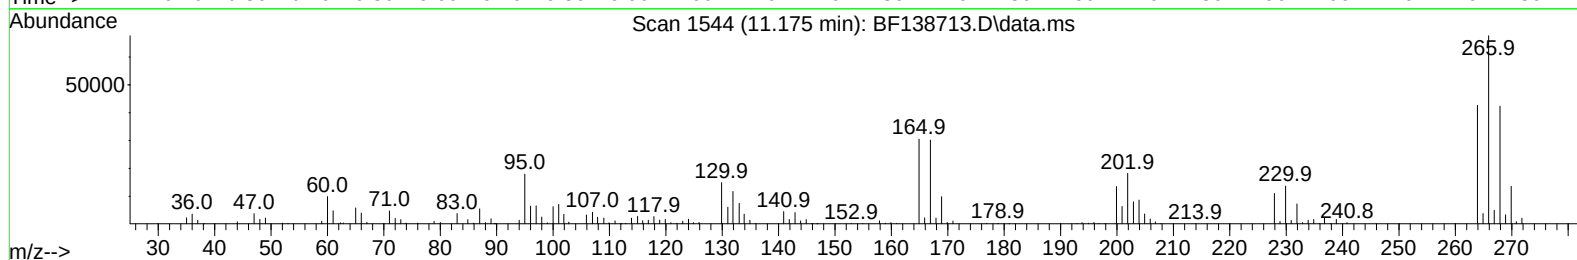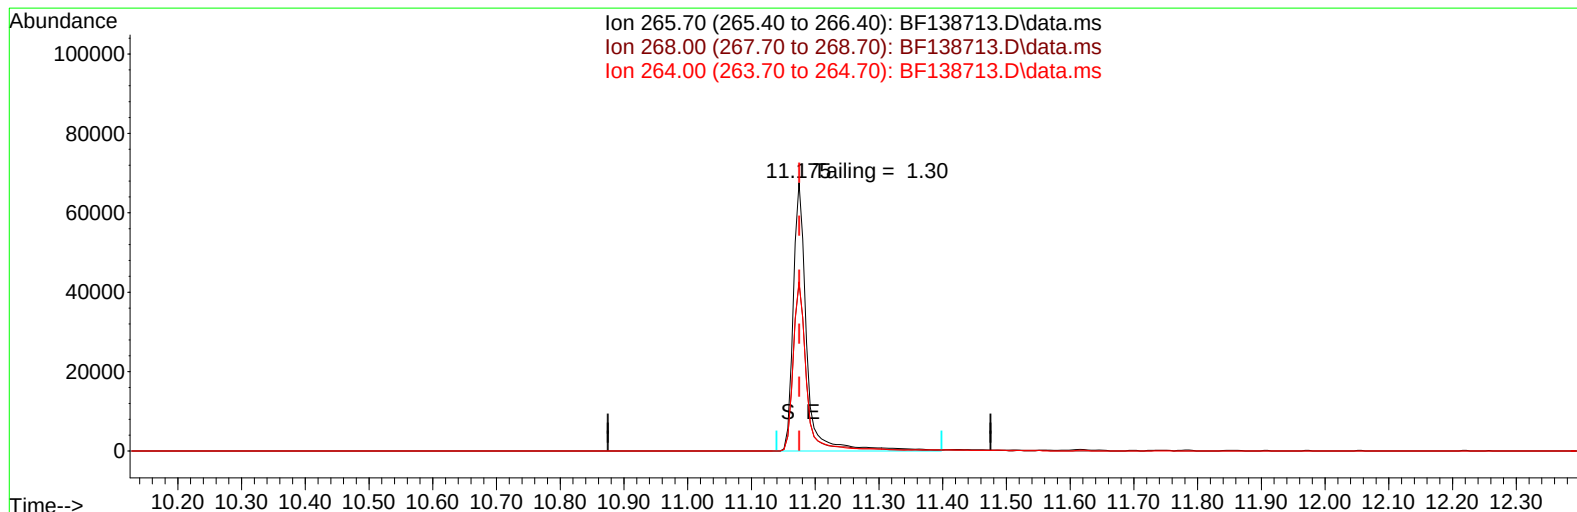

TIC: BF138713.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.000) 35881.22 ng




response 99981

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.50	62.64
264.00	62.20	63.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF080124\
Data File : BF138713.D
Acq On : 01 Aug 2024 09:13
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Aug 01 11:04:30 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF073024.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 17:50:01 2024
Response via : Initial Calibration

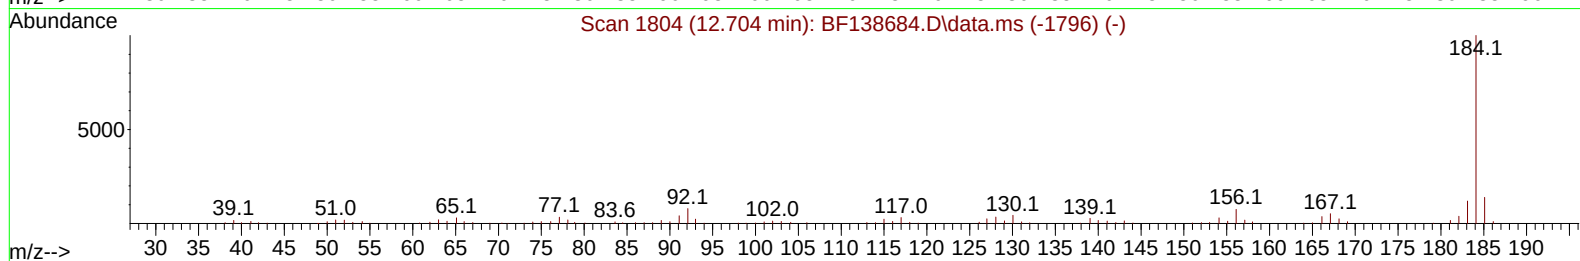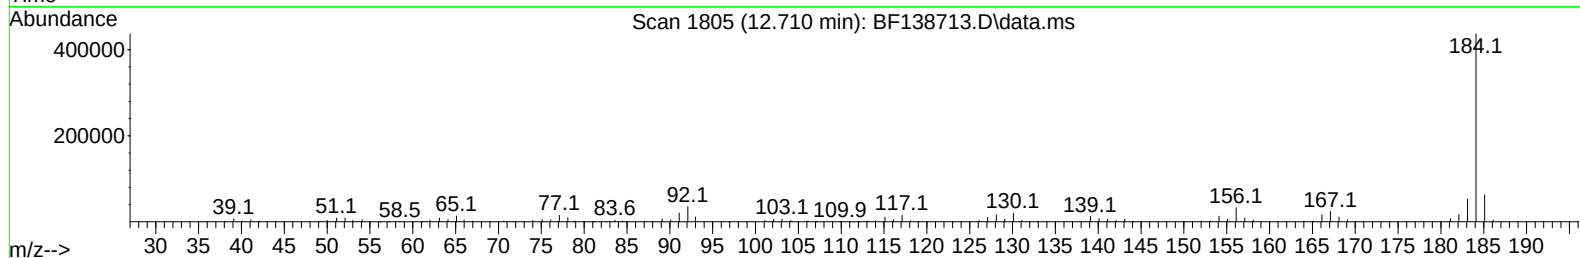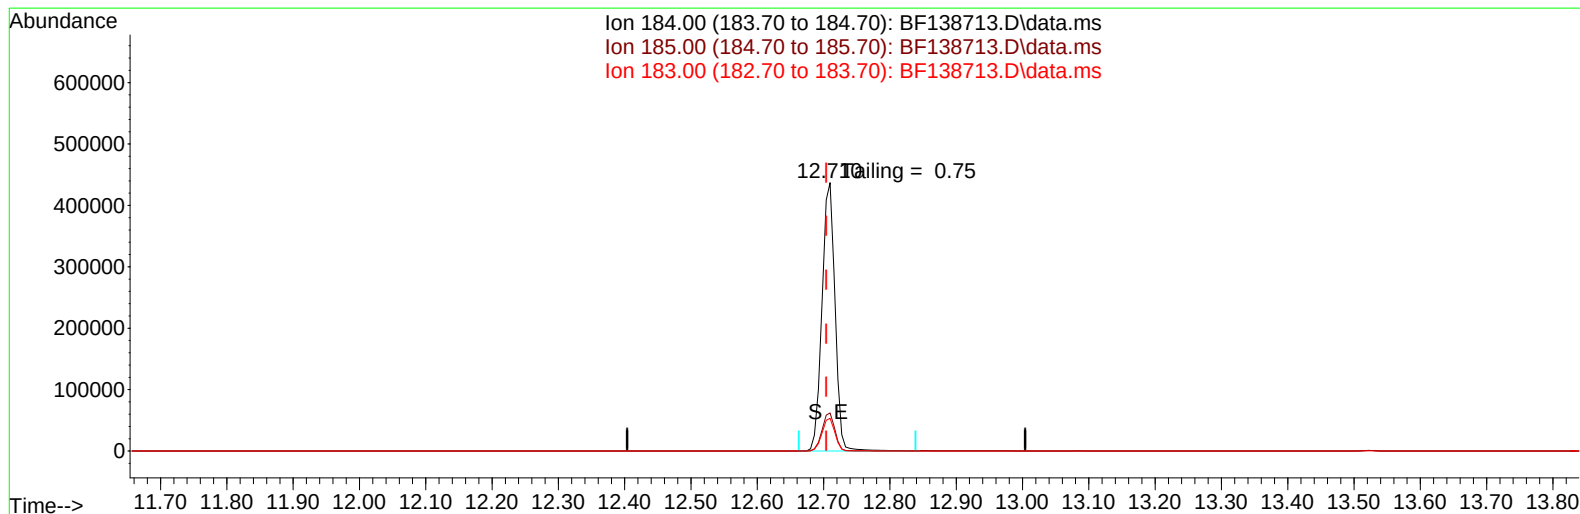

TIC: BF138713.D\data.ms

(77) Benzidine

12.710min (+ 0.006) 0.00 ng

response 598499

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.90	14.21
183.00	12.00	12.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
8/1/2024	BNA_F	<u>BF138713.D</u>
Compound Name	Response	Retention Time
DDT	297106	13.521
DDD	4492	13.251
DDE	513	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5005	302111	1.66

Instrument :
BNA_F
ClientSampleId :
DFTPP