


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080215\
Data File : BF080803.D
Acq On : 2 Aug 2015 11:52
Operator : TP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF073015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Aug 03 14:00:36 2015

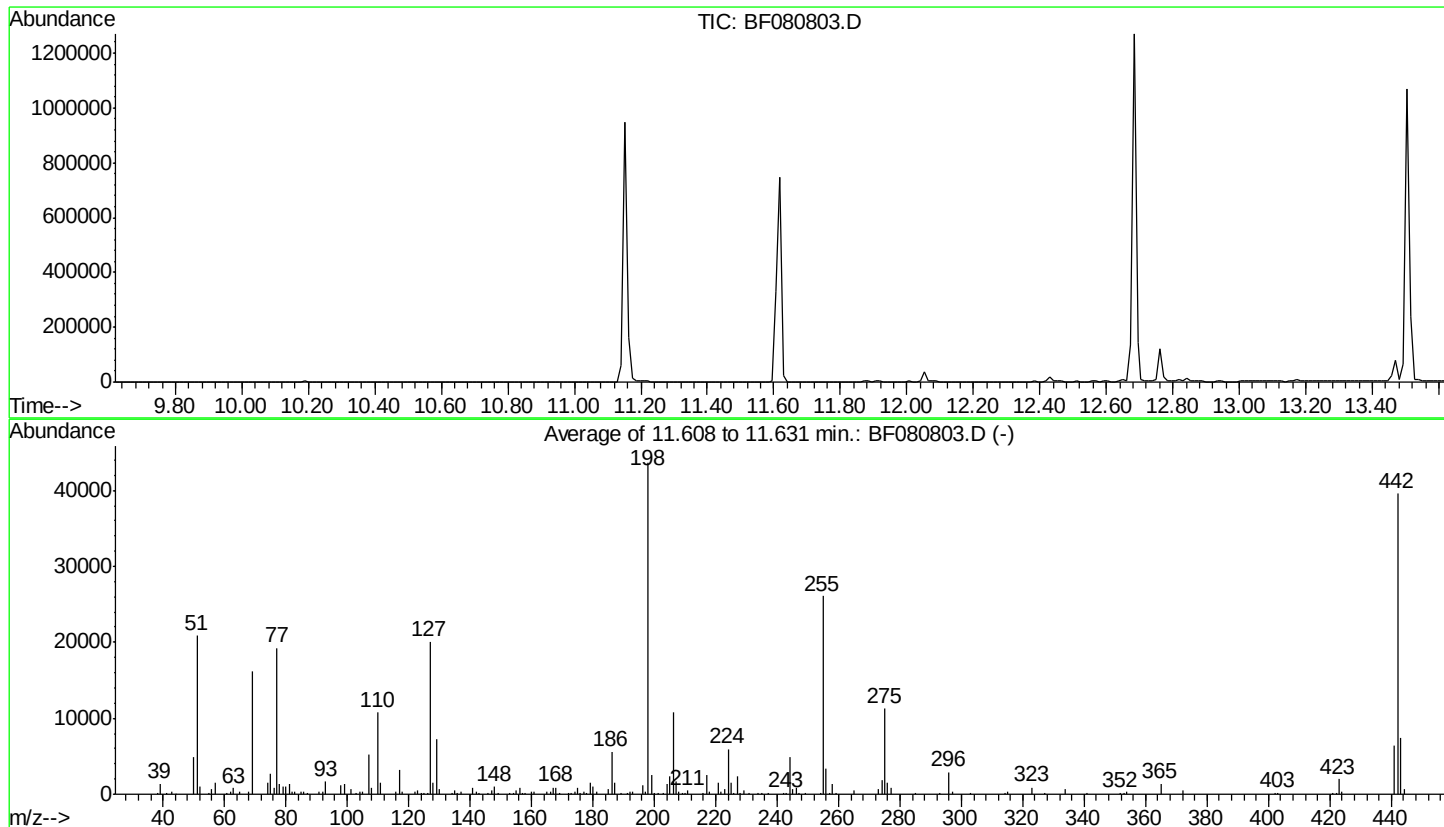

AutoFind: Scans 833, 834, 835; Background Corrected with Scan 830

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	20821	PASS
68	69	0.00	2	1.7	281	PASS
69	198	0.00	100	37.0	16170	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.1	20106	PASS
197	198	0.00	2	0.6	275	PASS
198	198	100	100	100.0	43652	PASS
199	198	5	9	5.8	2540	PASS
275	198	10	60	25.8	11268	PASS
365	198	1	100	3.2	1411	PASS
441	442	0.01	24	16.4	6467	PASS
442	198	50	100	90.6	39552	PASS
443	442	15	24	18.7	7378	PASS