
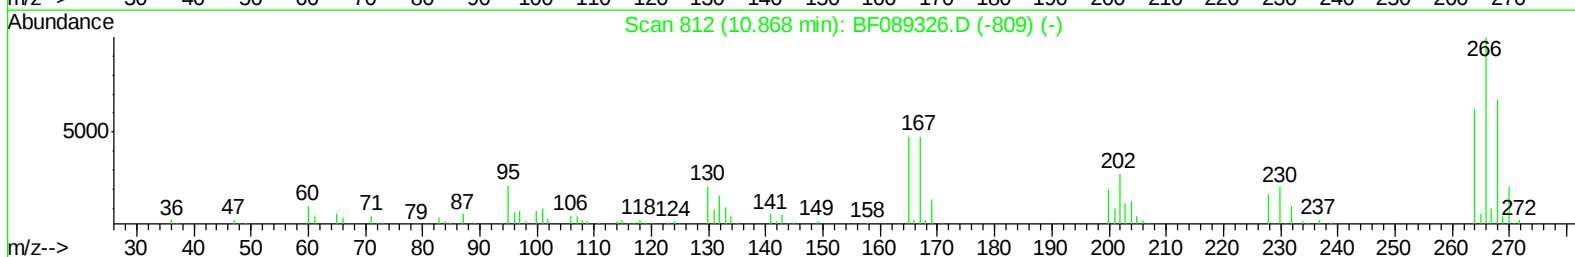
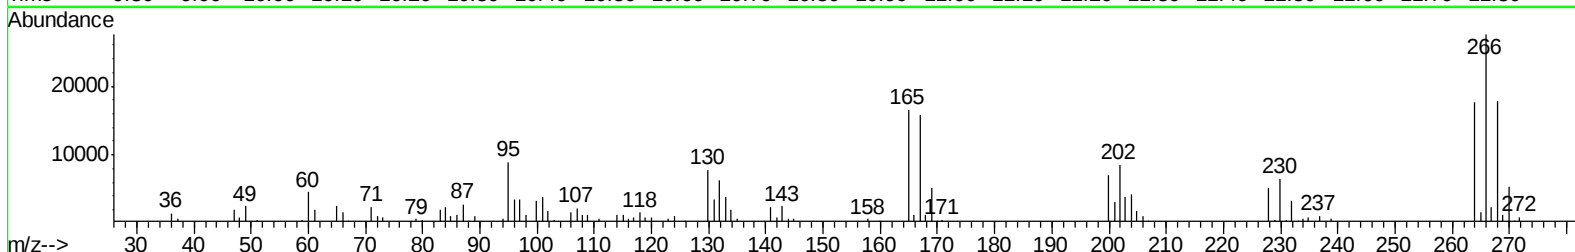


Data Path : Z:\HPCHEM1\BNA_F\Data\BF080216\
Data File : BF089539.D
Acq On : 2 Aug 2016 11:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 08:03:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

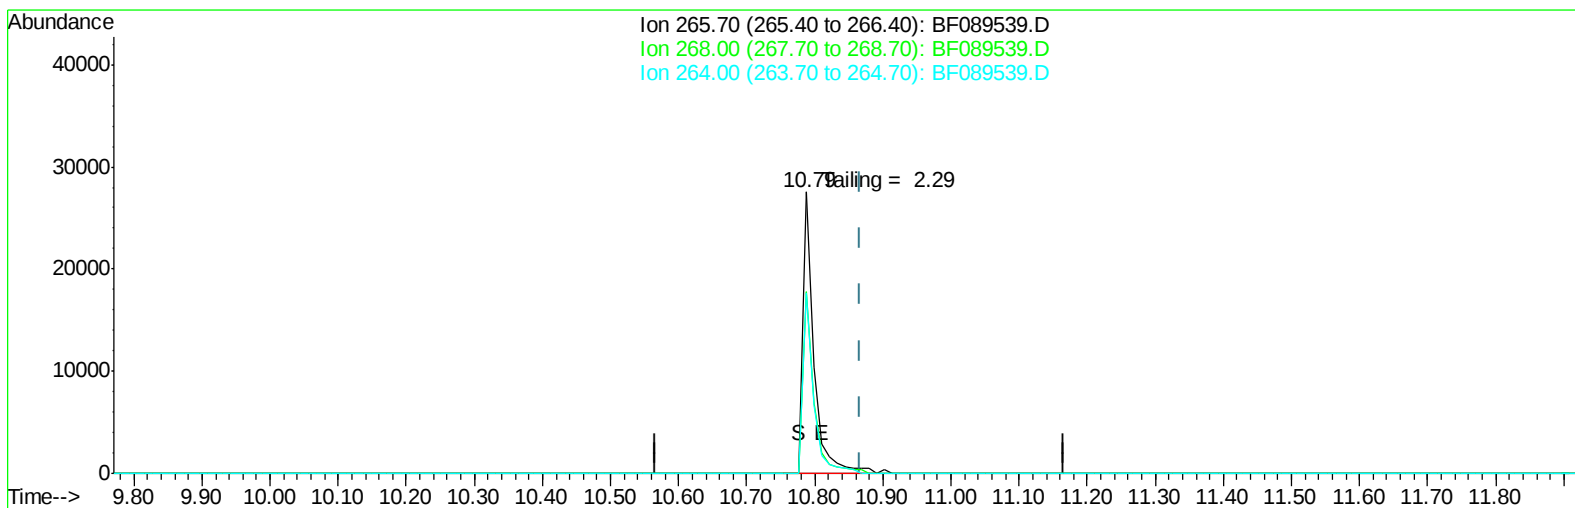

TIC: BF089539.D

(69) Pentachlorophenol (C)




10.788min (-0.079) 0.00ng

response 31470

Ion	Exp%	Act%
265.70	100	100
268.00	61.80	64.67
264.00	62.70	64.30
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF080216\
Data File : BF089539.D
Acq On : 2 Aug 2016 11:16
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 03 08:03:04 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 28 16:02:32 2016
Response via : Initial Calibration

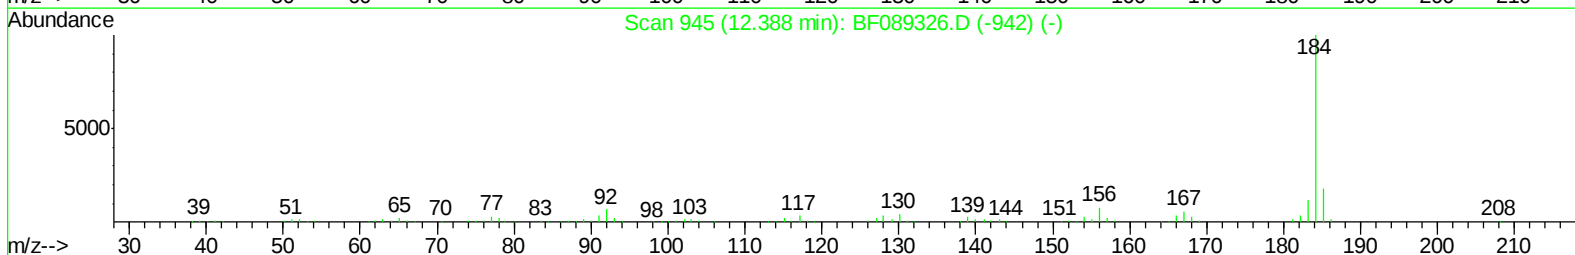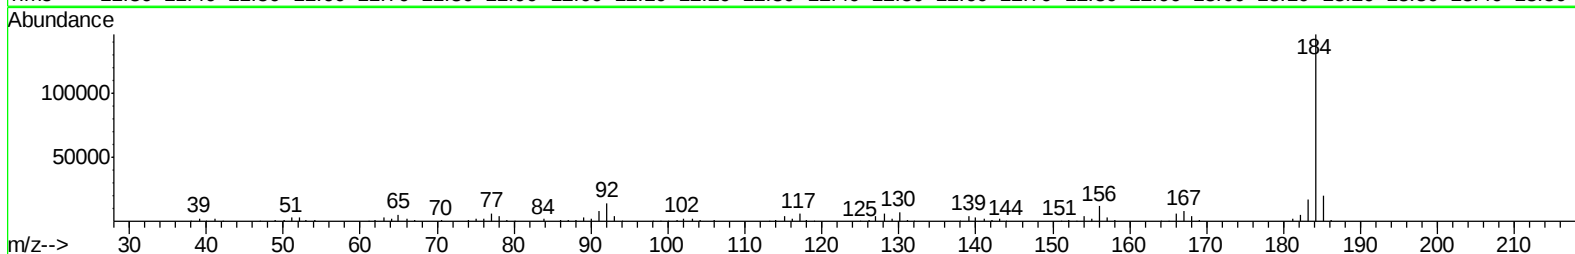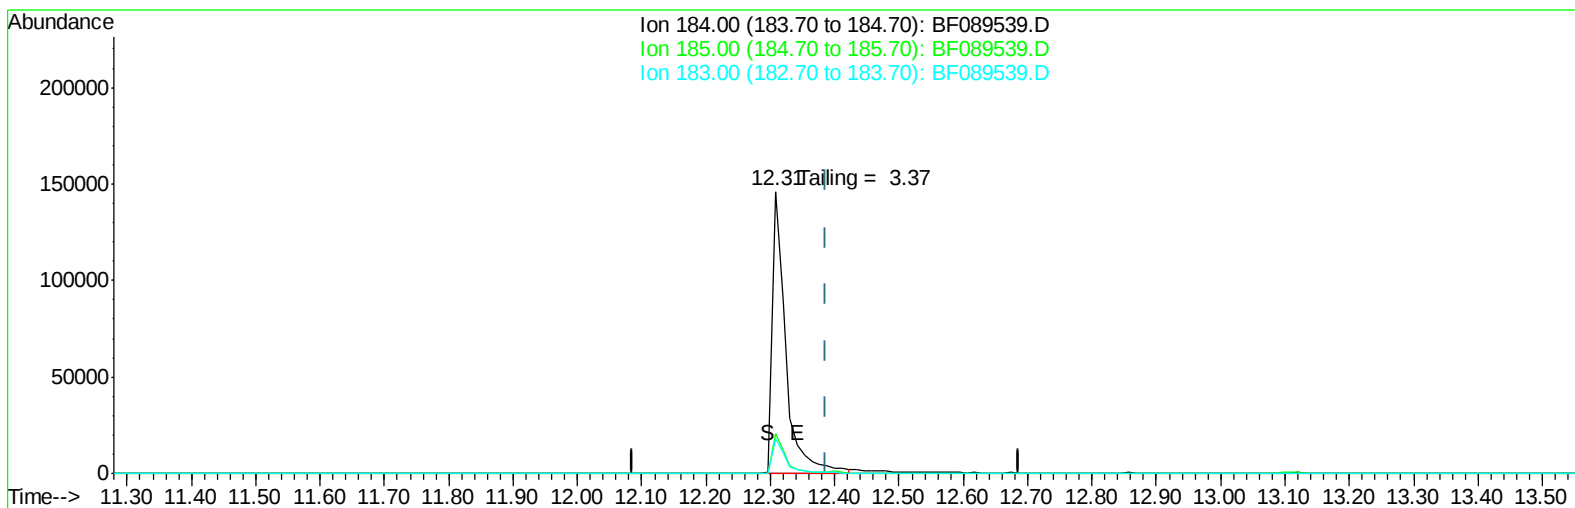

TIC: BF089539.D

(76) Benzidine

12.308min (-0.079) 0.00ng

response 220493

Ion	Exp%	Act%
184.00	100	100
185.00	16.90	14.08
183.00	12.20	12.09
0.00	0.00	0.00