

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080216\
 Data File : BF089556.D
 Acq On : 2 Aug 2016 19:40
 Operator : UM/SJ
 Sample : H4269-15
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-55-17.0-18.0

Quant Time: Aug 03 02:01:12 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 03 01:32:56 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.47	152	41970	20.00	ng	0.00
21) Naphthalene-d8	7.76	136	161553	20.00	ng	0.00
38) Acenaphthene-d10	9.50	164	74083	20.00	ng	-0.01
63) Phenanthrene-d10	10.97	188	122366	20.00	ng	0.00
75) Chrysene-d12	13.59	240	87102	20.00	ng	-0.01
86) Perylene-d12	14.91	264	79985	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.04	112	335124	127.50	ng	0.01
7) Phenol-d6	6.14	99	482203	138.82	ng	0.00
23) Nitrobenzene-d5	7.05	82	284015	103.77	ng	0.00
41) 2,4,6-Tribromophenol	10.28	330	76849	125.25	ng	-0.01
44) 2-Fluorobiphenyl	8.83	172	425617	84.31	ng	-0.01
78) Terphenyl-d14	12.55	244	298727	80.27	ng	-0.01
Target Compounds						Qvalue
49) Dimethylphthalate	9.23	163	98478	17.47	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080216\
Data File : BF089556.D
Acq On : 2 Aug 2016 19:40
Operator : UM/SJ
Sample : H4269-15
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-55-17.0-18.0

Quant Time: Aug 03 02:01:12 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 03 01:32:56 2016
Response via : Initial Calibration

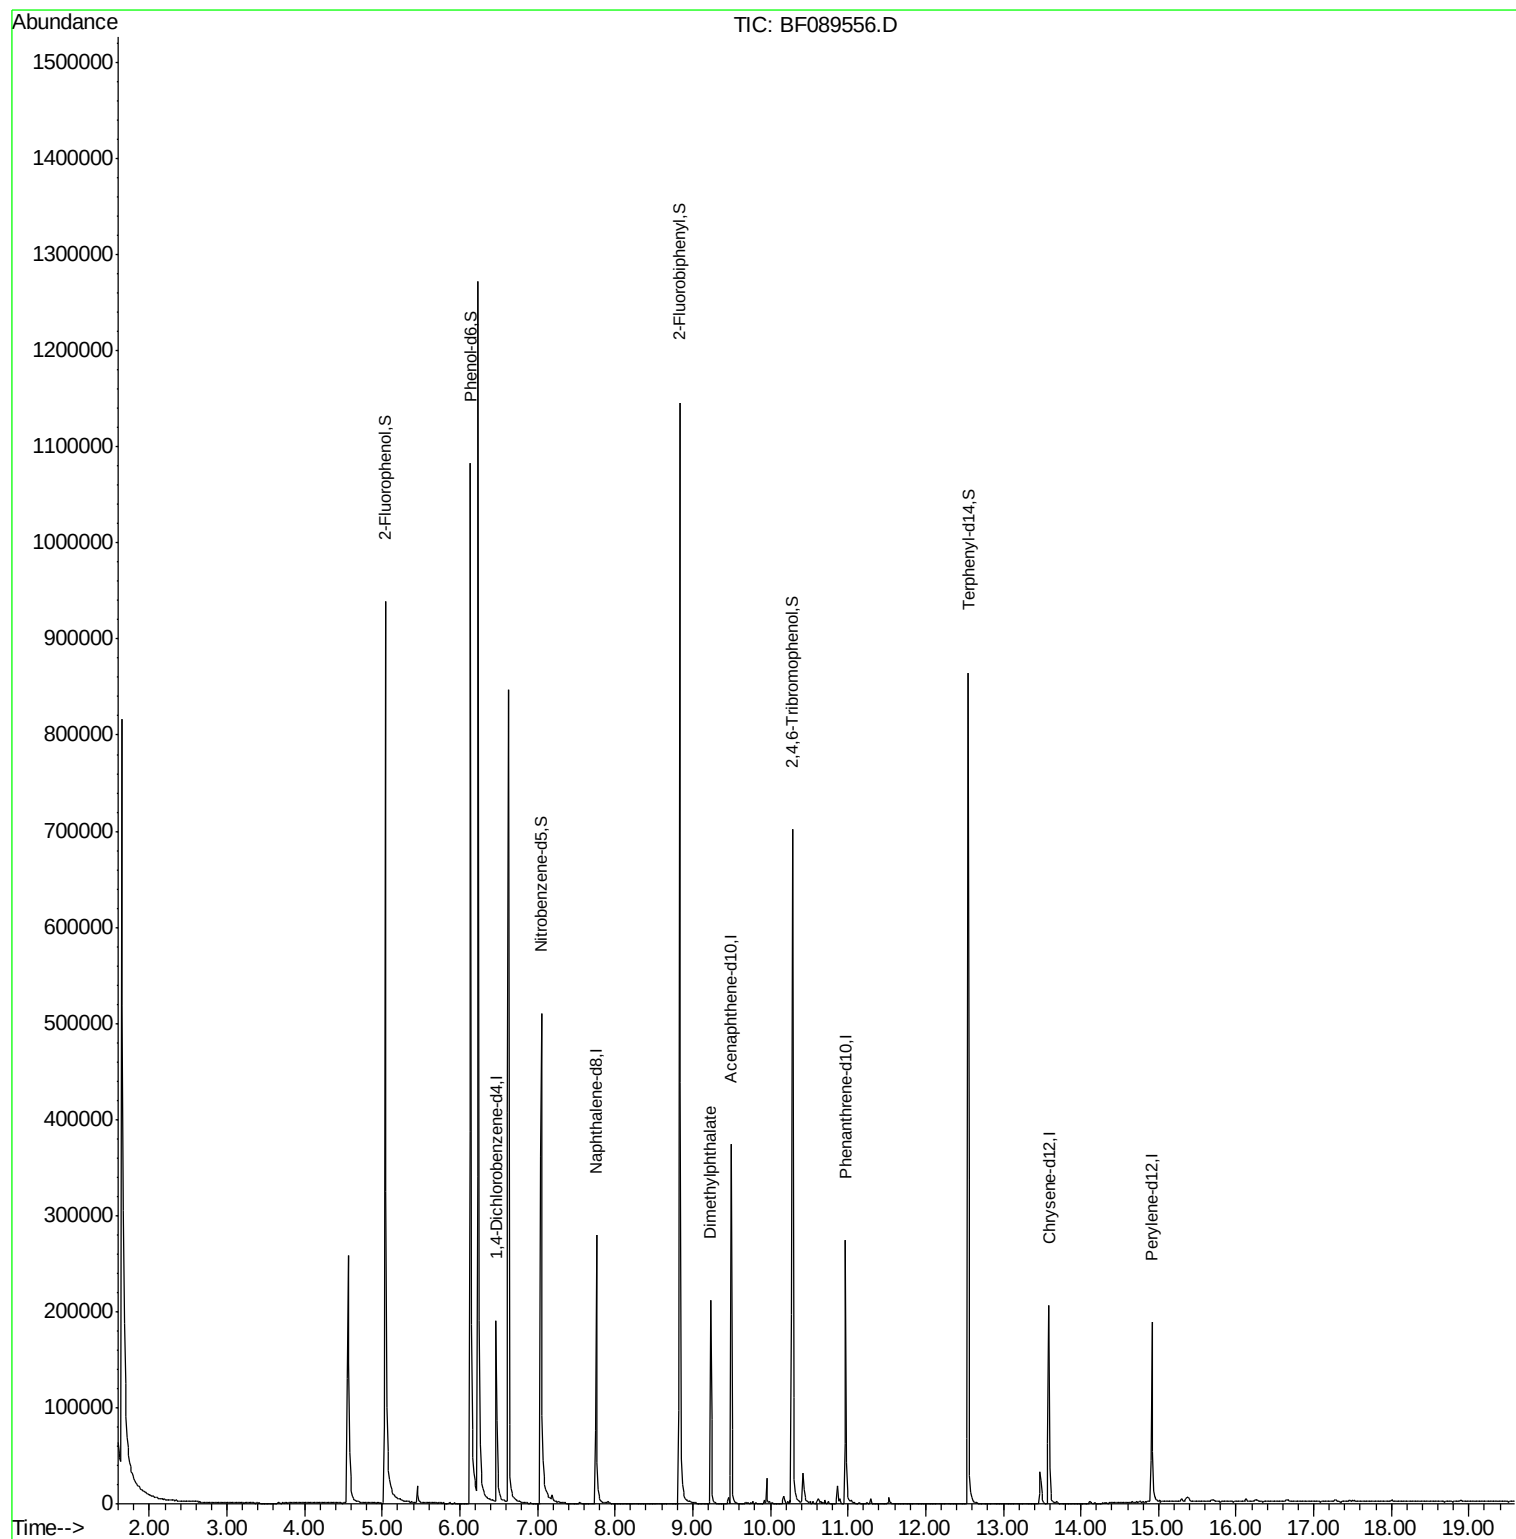

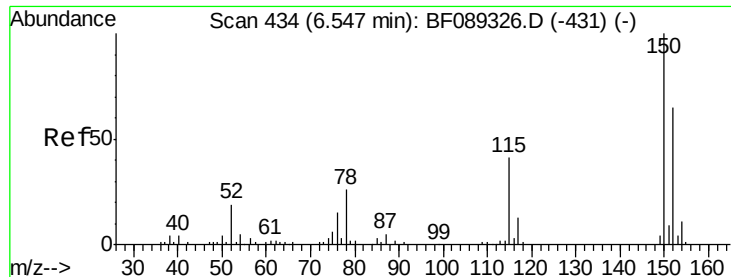


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.47 min Scan# 427
Delta R.T. -0.00 min
Lab File: BF089556.D
Acq: 2 Aug 2016 19:40

Instrument :
BNA_F
ClientSampleId :
SB-55-17.0-18.0

Tot Ion:152 Resp: 41970
Ion Ratio Lower Upper
152 100
150 157.2 129.5 194.3
115 70.6 51.4 77.2

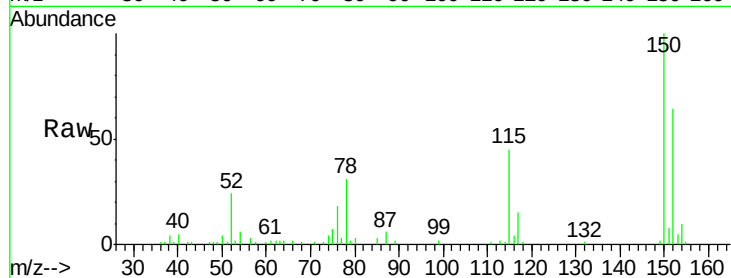


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

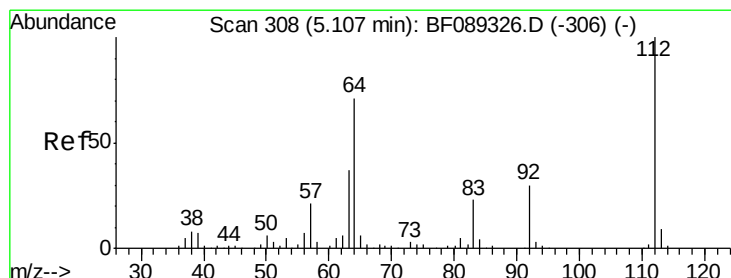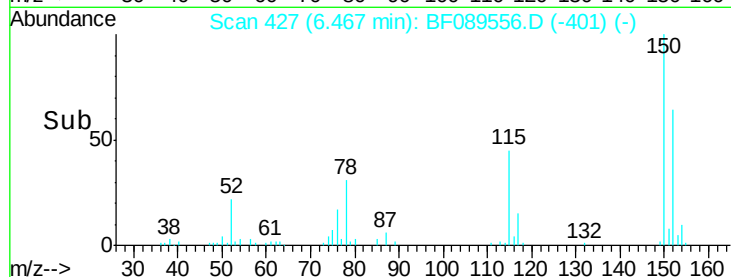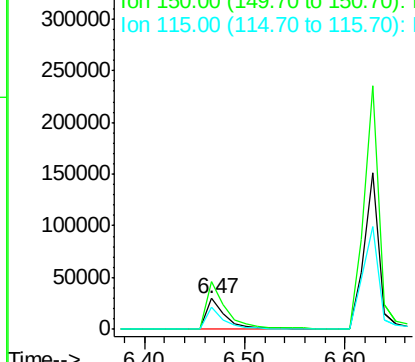



#5


2-Fluorophenol
Concen: 127.50 ng
RT: 5.04 min Scan# 302
Delta R.T. 0.01 min
Lab File: BF089556.D
Acq: 2 Aug 2016 19:40

Tgt Ion:112 Resp: 335124
Ion Ratio Lower Upper
112 100
64 60.3 55.0 82.6
63 32.2 29.4 44.2

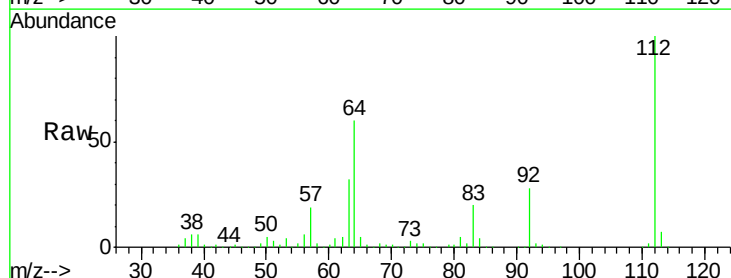

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

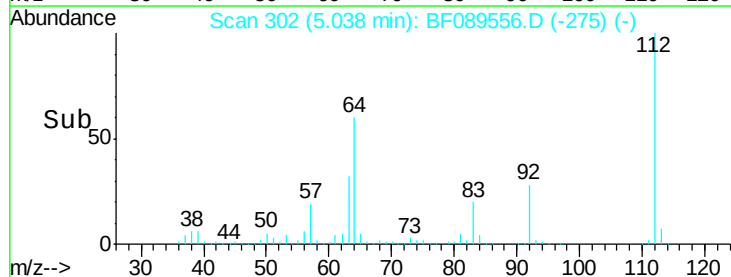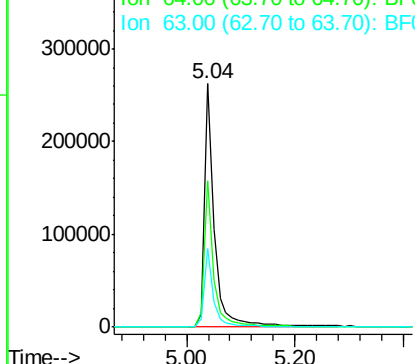

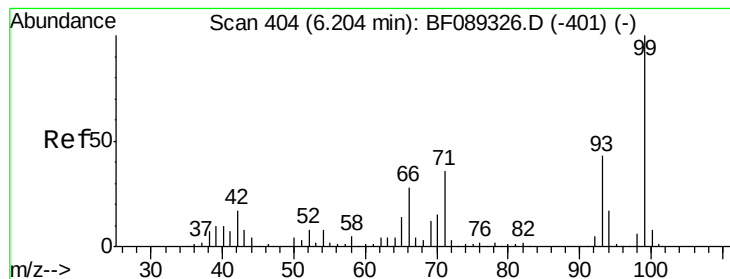

#7

Phenol-d6

Concen: 138.82 ng

RT: 6.14 min Scan# 398

Delta R.T. -0.00 min

Lab File: BF089556.D

Acq: 2 Aug 2016 19:40

Instrument :

BNA_F

ClientSampleId :

SB-55-17.0-18.0


Tot Ion: 99 Resp: 482203

Ion Ratio Lower Upper

99 100

42 17.3 13.6 20.4




71 37.4 29.4 44.2

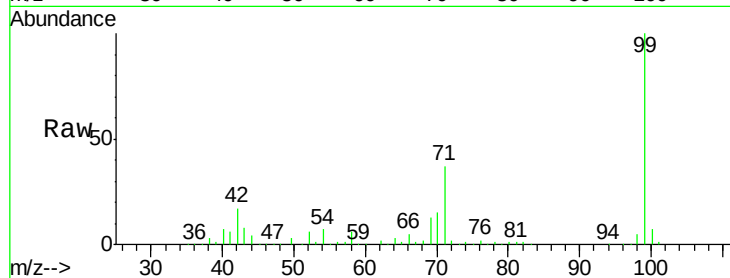

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

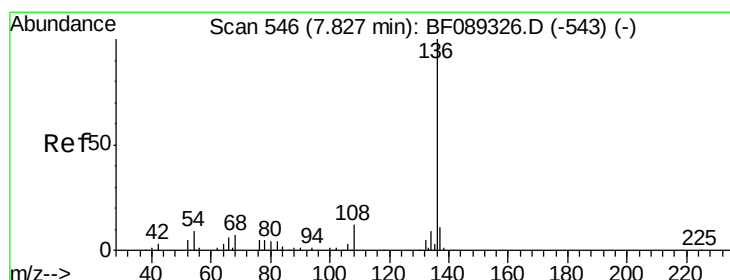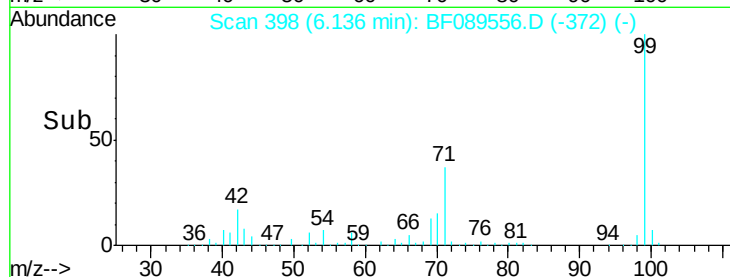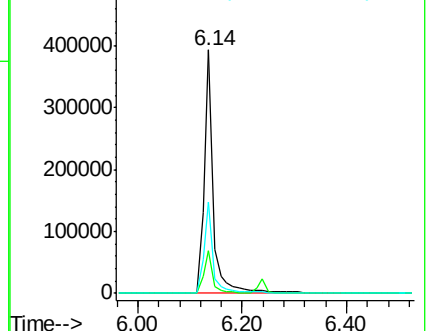

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 7.76 min Scan# 540

Delta R.T. -0.00 min

Lab File: BF089556.D

Acq: 2 Aug 2016 19:40

Tgt Ion: 136 Resp: 161553


Ion Ratio Lower Upper

136 100

137 10.7 8.6 13.0

54 6.0 7.0 10.4

68 5.1 4.9 7.3


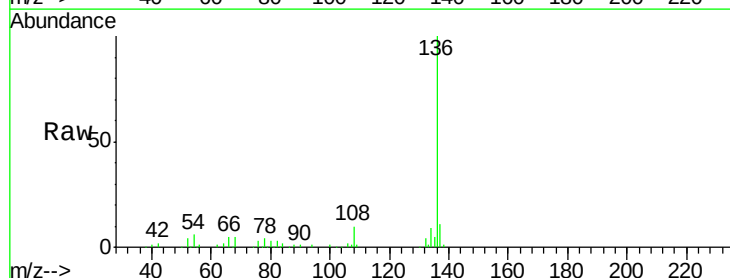



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

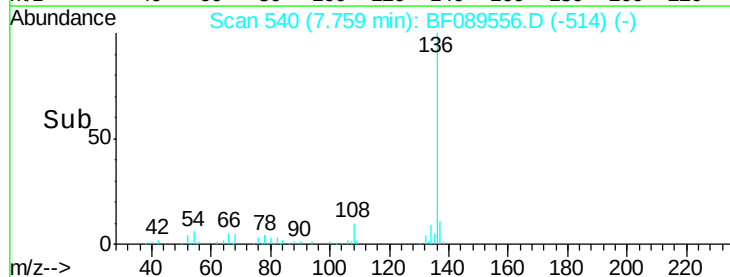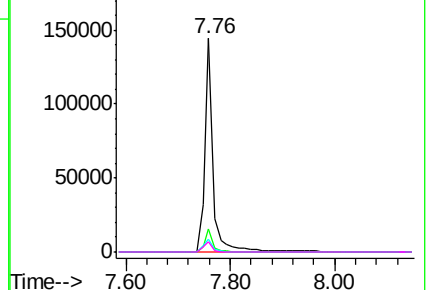


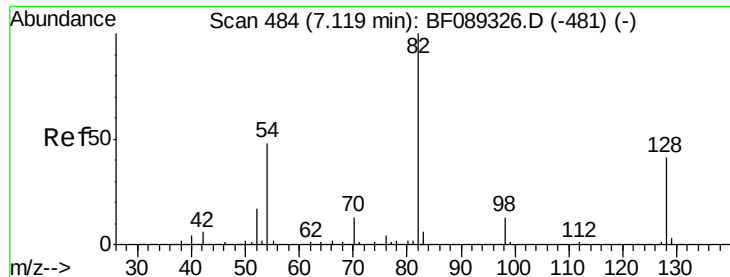




#23
 Nitrobenzene-d5
 Concen: 103.77 ng
 RT: 7.05 min Scan# 478
 Delta R.T. -0.00 min
 Lab File: BF089556.D
 Acq: 2 Aug 2016 19:40

Instrument :
 BNA_F
 ClientSampleId :
 SB-55-17.0-18.0

Tot Ion	82	Resp	284015
Ion Ratio	100		
Lower	32.5		
Upper	48.7		
54	43.0		58.2

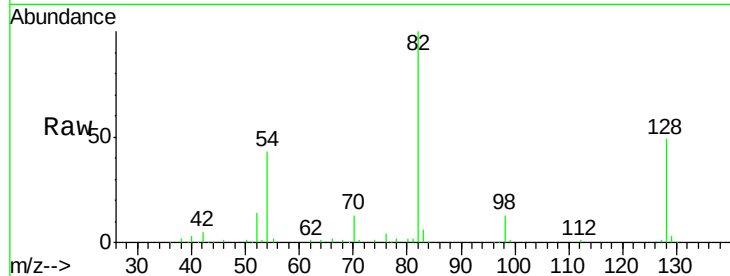


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): BF0
 Ion 54.00 (53.70 to 54.70): BF0

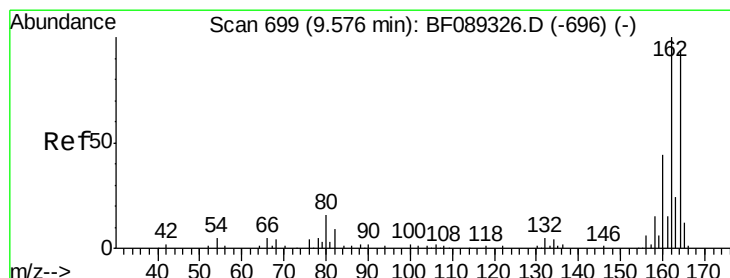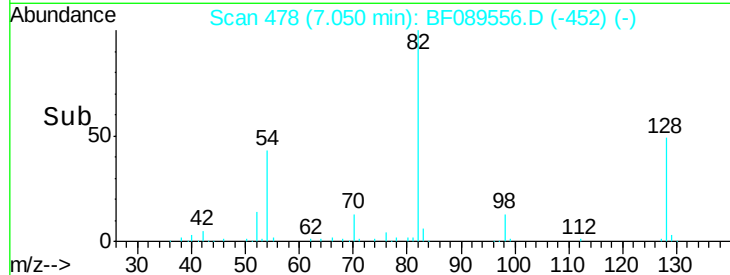
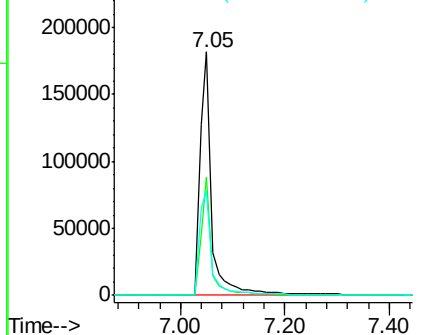



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.50 min Scan# 692
 Delta R.T. -0.01 min
 Lab File: BF089556.D
 Acq: 2 Aug 2016 19:40

Tgt Ion	164	Resp	74083
Ion Ratio	100		
Lower	83.7		
Upper	125.5		
162	104.8		56.6
160	46.7		

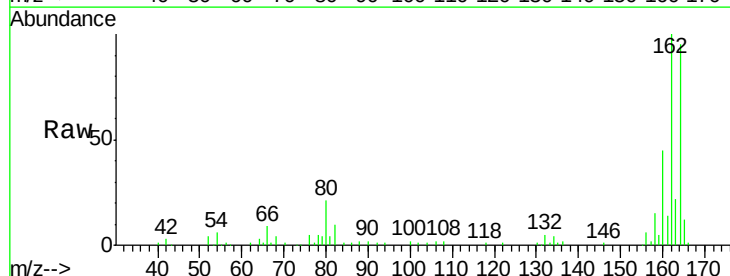

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

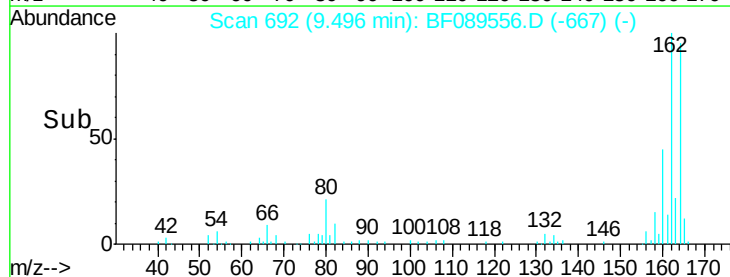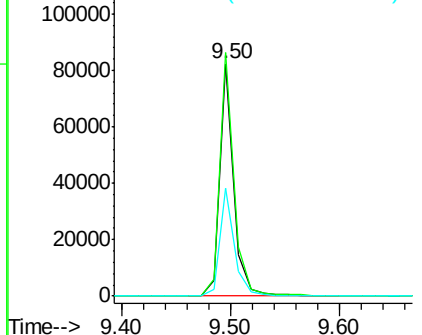


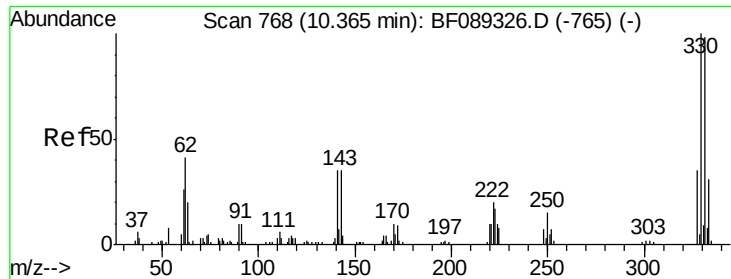

#41
 2,4,6-Tribromophenol
 Concen: 125.25 ng
 RT: 10.28 min Scan# 761
 Delta R.T. -0.01 min
 Lab File: BF089556.D
 Acq: 2 Aug 2016 19:40

Instrument :
 BNA_F
 ClientSampleId :
 SB-55-17.0-18.0

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	76.8	115.2
141	49.4	37.3	55.9



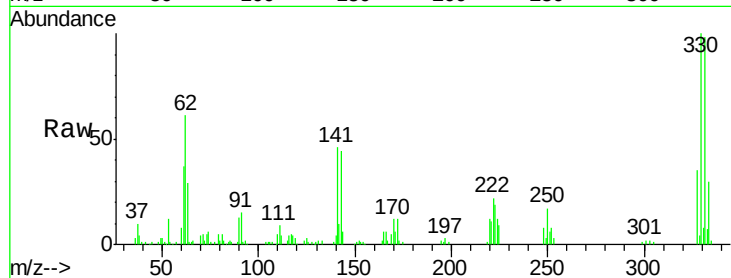


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

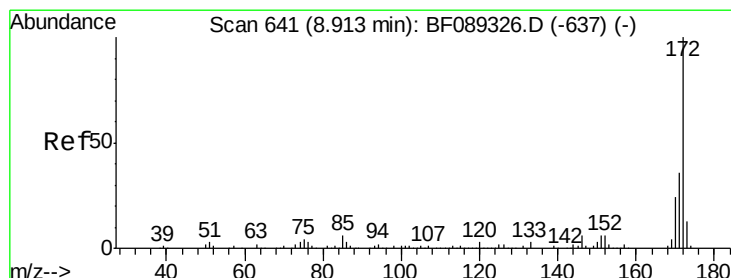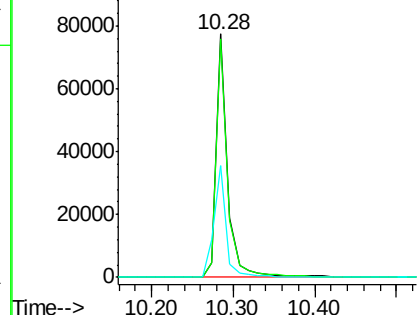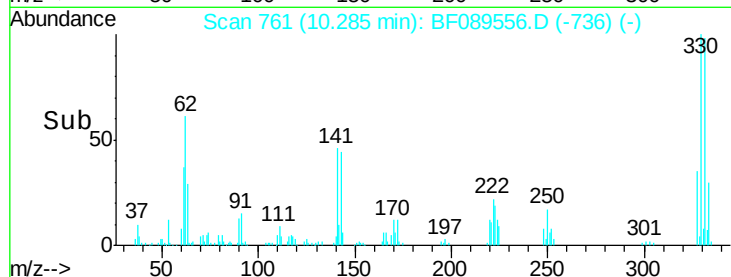

#44
 2-Fluorobiphenyl
 Concen: 84.31 ng
 RT: 8.83 min Scan# 634
 Delta R.T. -0.01 min
 Lab File: BF089556.D
 Acq: 2 Aug 2016 19:40

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.8	29.2	43.8
170	23.5	19.2	28.8


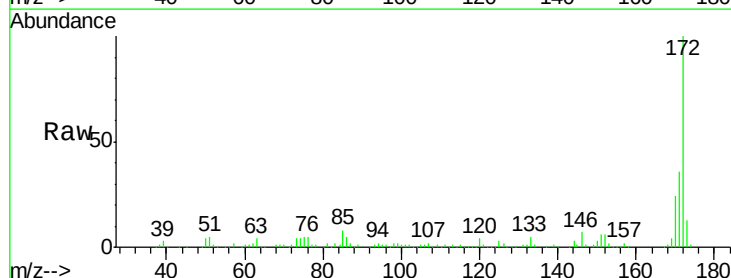



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E



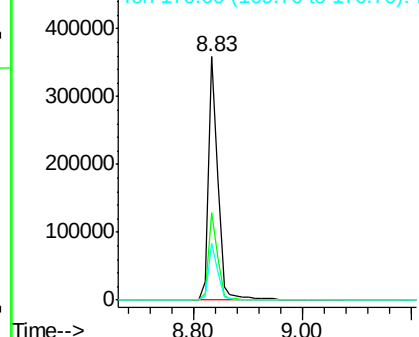
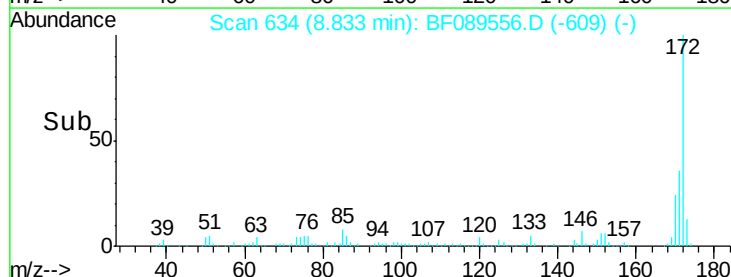


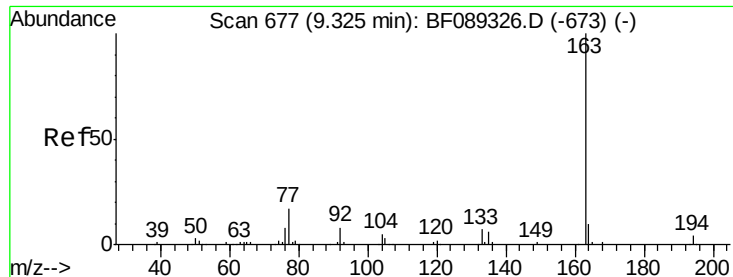

#49
Dimethylphthalate
Concen: 17.47 ng
RT: 9.23 min Scan# 669
Delta R.T. -0.02 min
Lab File: BF089556.D
Acq: 2 Aug 2016 19:40




Instrument :
BNA_F
ClientSampleId :
SB-55-17.0-18.0


Tot Ion:163 Resp: 98478
Ion Ratio Lower Upper
163 100
194 3.0 2.8 4.2
164 10.4 7.8 11.8

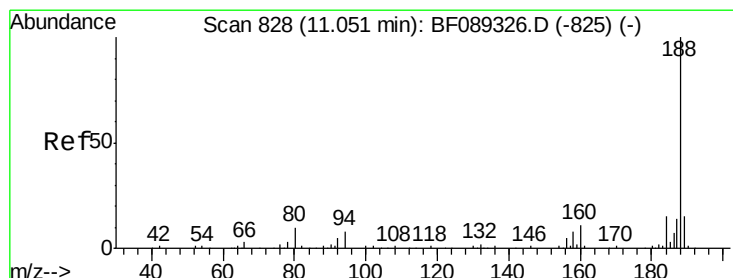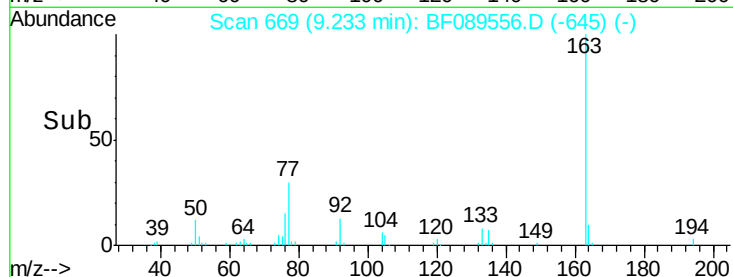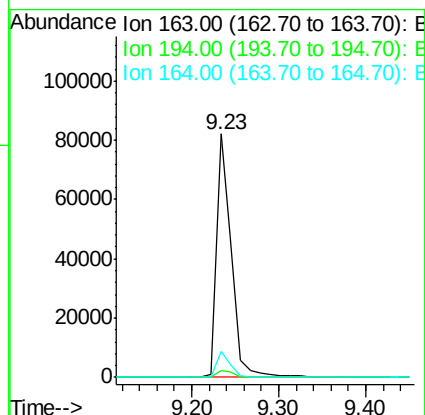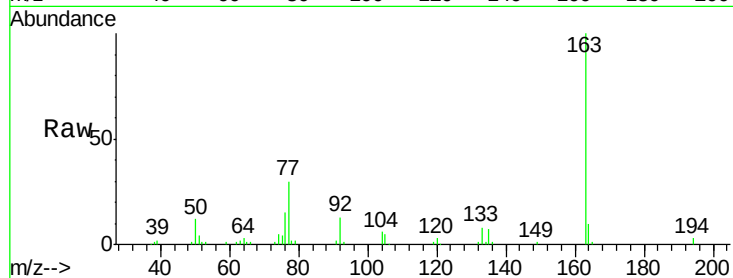

#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 10.97 min Scan# 821
Delta R.T. -0.00 min
Lab File: BF089556.D
Acq: 2 Aug 2016 19:40

Tgt Ion:188 Resp: 122366
Ion Ratio Lower Upper
188 100
94 8.4 6.5 9.7
80 9.3 7.2 10.8

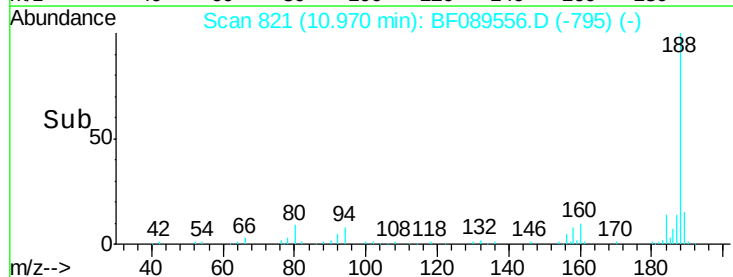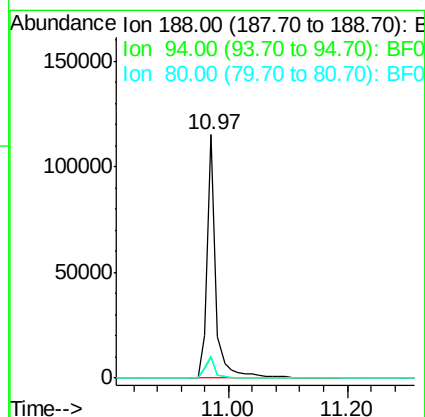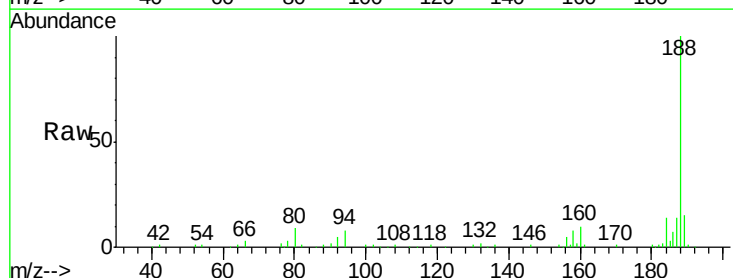

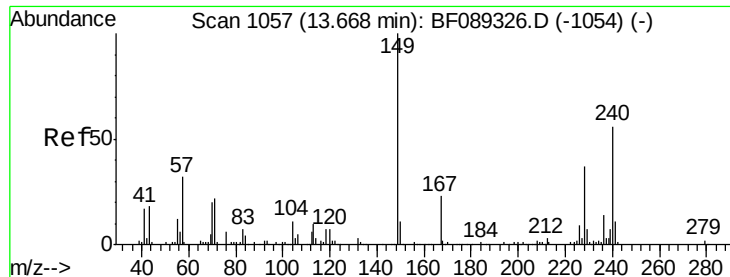

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.59 min Scan# 1050

Delta R.T. -0.01 min

Lab File: BF089556.D

Acq: 2 Aug 2016 19:40

Instrument :

BNA_F

ClientSampleId :

SB-55-17.0-18.0


Tot Ion:240 Resp: 87102

Ion Ratio Lower Upper

240 100

120 10.1 9.1 13.7




236 24.6 20.6 30.8

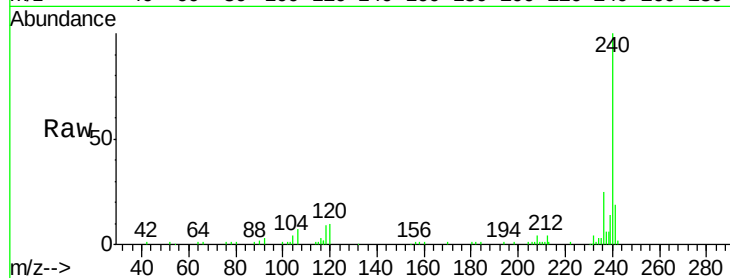

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

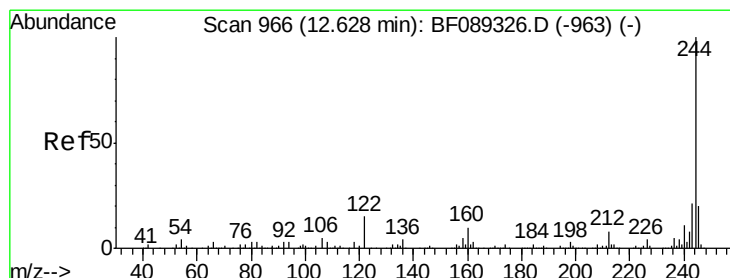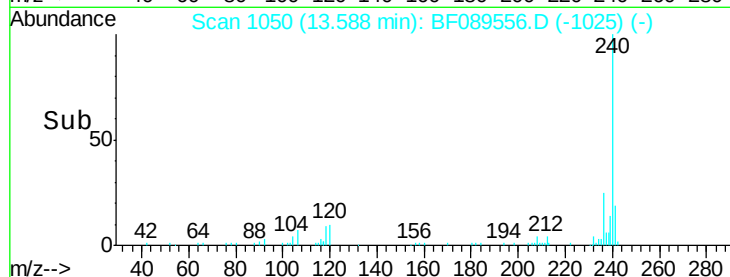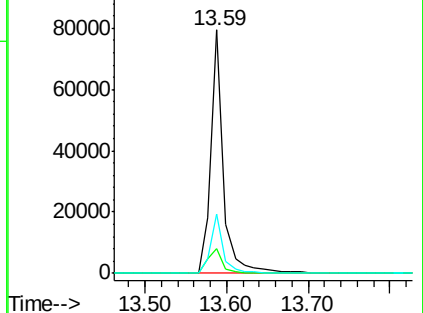

#78

Terphenyl-d14

Concen: 80.27 ng

RT: 12.55 min Scan# 959

Delta R.T. -0.01 min

Lab File: BF089556.D

Acq: 2 Aug 2016 19:40


Tgt Ion:244 Resp: 298727

Ion Ratio Lower Upper

244 100

212 8.2 6.5 9.7



122 17.0 11.4 17.0

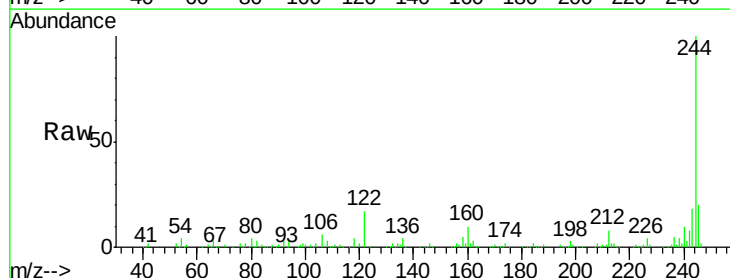


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

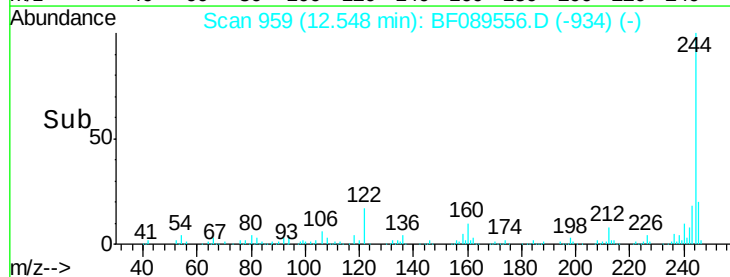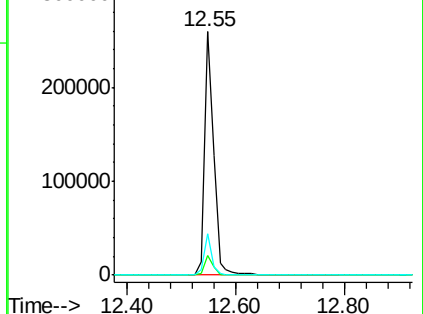


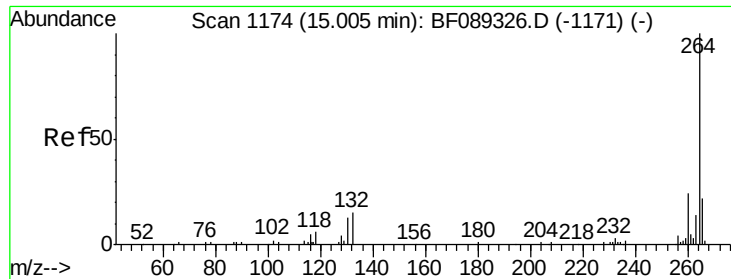

#86
 Pervlene-d12
 Concen: 20.00 ng
 RT: 14.91 min Scan# 1166
 Delta R.T. -0.01 min
 Lab File: BF089556.D
 Acq: 2 Aug 2016 19:40

Instrument :
 BNA_F
 ClientSampleId :
 SB-55-17.0-18.0

Tot Ion	Ratio	Lower	Upper
264	100		
260	22.9	19.0	28.4
265	20.7	17.5	26.3

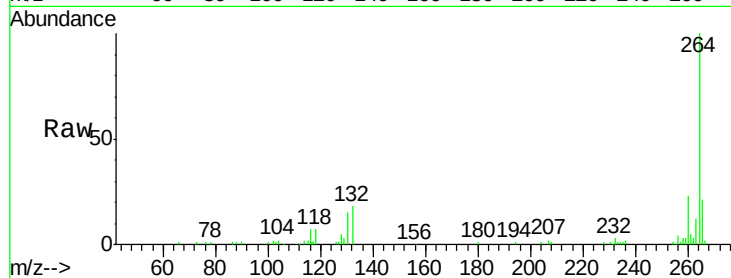

Abundance Ion 264.00 (263.70 to 264.70): E
 Ion 260.00 (259.70 to 260.70): E
 Ion 265.00 (264.70 to 265.70): E

