

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\
 Data File : BF097305.D
 Acq On : 3 Aug 2017 7:49
 Operator : SJ/JU
 Sample : I4537-04
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Aug 03 11:59:08 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 25 14:11:51 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.45	152	108091	20.00	ng	-0.05
21) Naphthalene-d8	7.73	136	407479	20.00	ng	-0.05
38) Acenaphthene-d10	9.47	164	186829	20.00	ng	-0.06
63) Phenanthrene-d10	10.95	188	283491	20.00	ng	-0.05
75) Chrysene-d12	13.57	240	185258	20.00	ng	-0.06
86) Perylene-d12	14.92	264	169659	20.00	ng	-0.06
System Monitoring Compounds						
5) 2-Fluorophenol	5.05	112	506407	70.63	ng	-0.05
7) Phenol-d6	6.12	99	664590	81.19	ng	-0.05
23) Nitrobenzene-d5	7.02	82	434397	62.54	ng	-0.06
41) 2,4,6-Tribromophenol	10.26	330	113675	77.01	ng	-0.06
44) 2-Fluorobiphenyl	8.81	172	729010	66.22	ng	-0.06
78) Terphenyl-d14	12.53	244	458404	50.45	ng	-0.05
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.02	70	57557	10.682	ng	# 85
25) Isophorone	7.02	82	421360	30.976	ng	# 67
49) Dimethylphthalate	9.21	163	56153	3.958	ng	# 97
50) 2,6-Dinitrotoluene	9.47	165	23861	7.930	ng	# 34
56) 2,4-Dinitrotoluene	9.47	165	23861	6.898	ng	# 33
66) 4-Bromophenyl-phenylether	10.26	248	7096	2.508	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\
Data File : BF097305.D
Acq On : 3 Aug 2017 7:49
Operator : SJ/JU
Sample : I4537-04
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Aug 03 11:59:08 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 14:11:51 2017
Response via : Initial Calibration

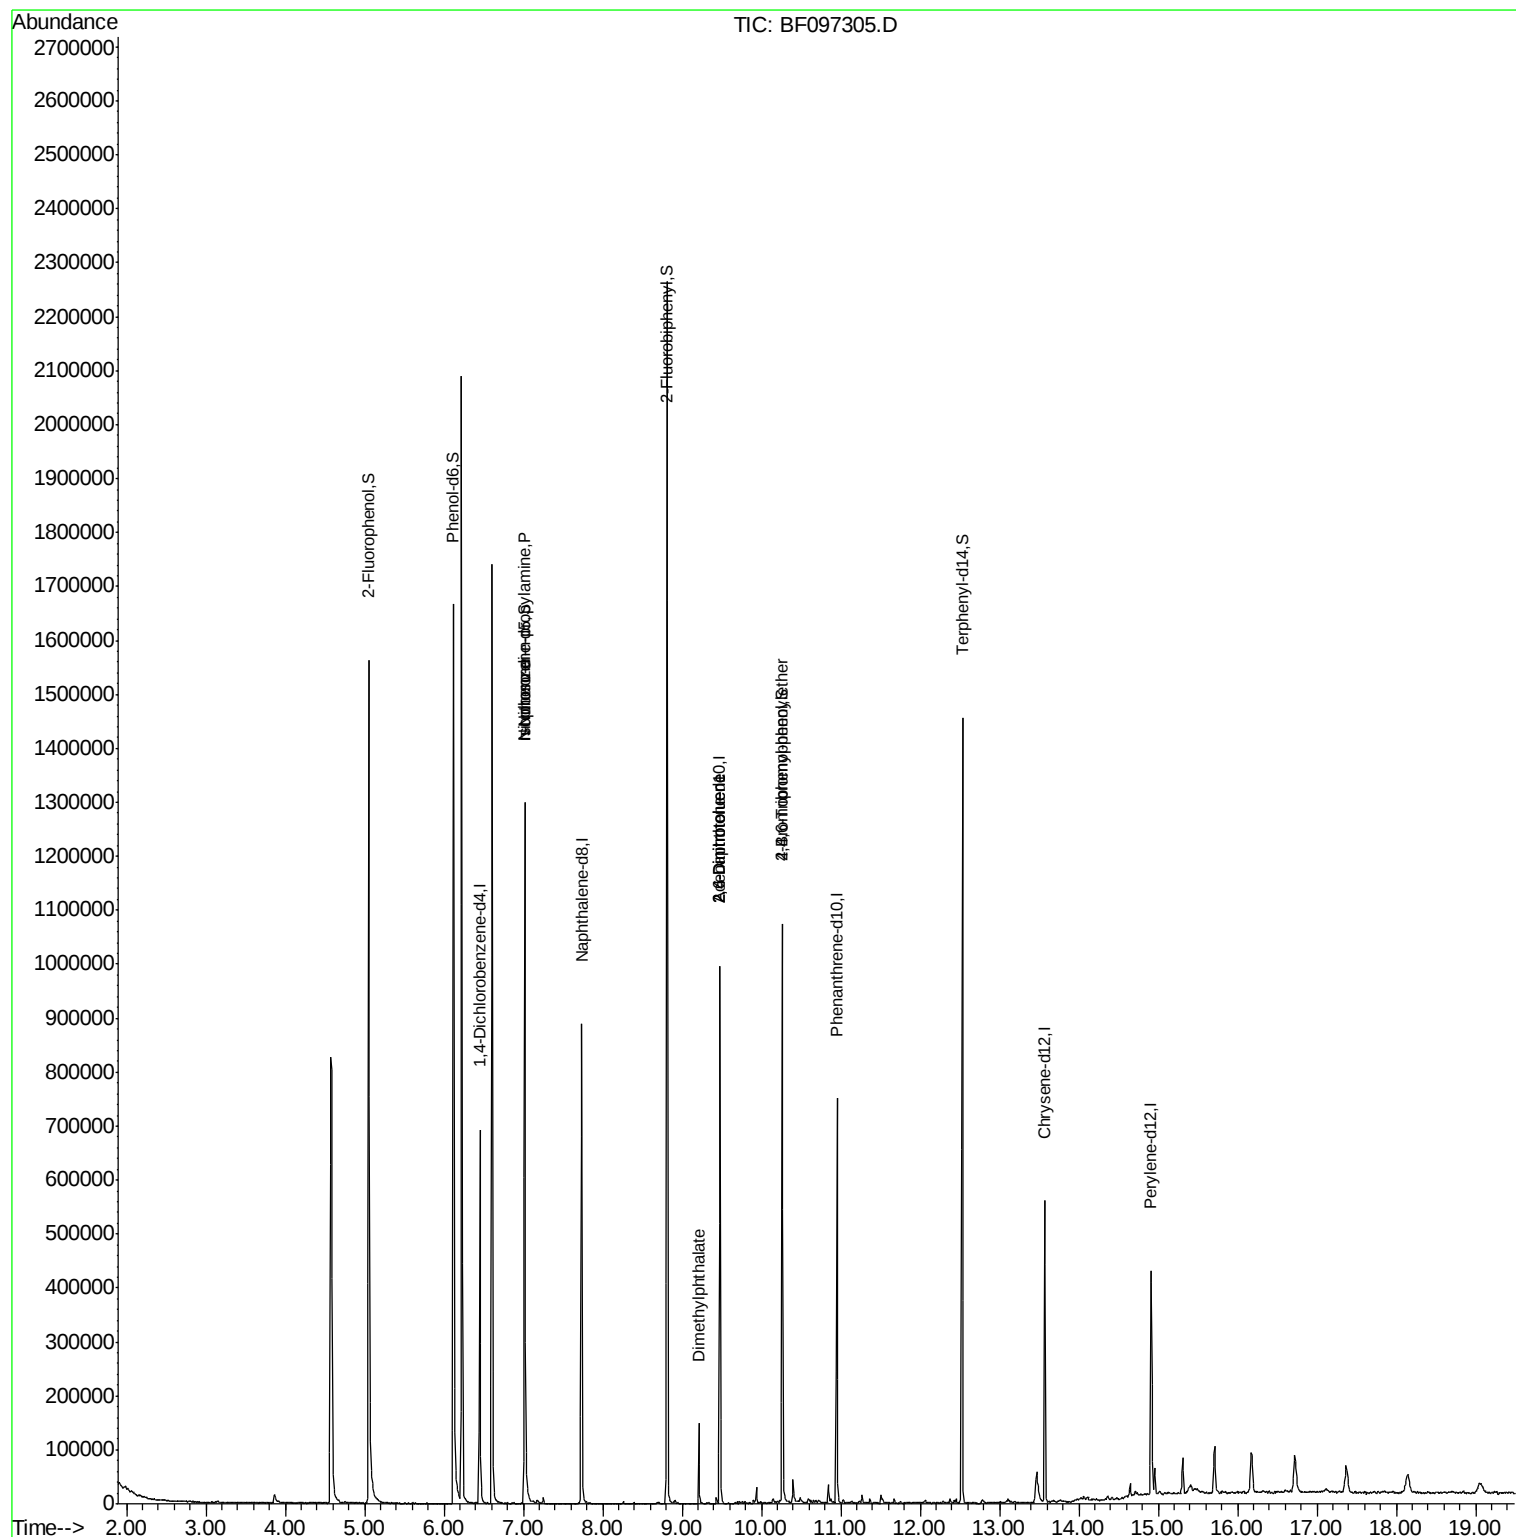

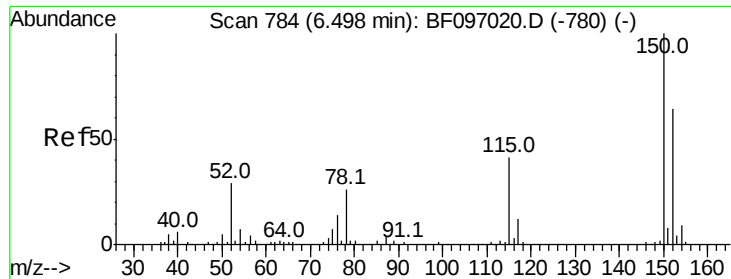


#1



1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.45 min Scan# 776
Delta R.T. -0.05 min
Lab File: BF097305.D
Acq: 3 Aug 2017 7:49

Instrument :
BNA_F
ClientSampled :

Tot Ion:152 Resp: 108091
Ion Ratio Lower Upper
152 100
150 158.7 126.2 189.2
115 62.2 52.2 78.2

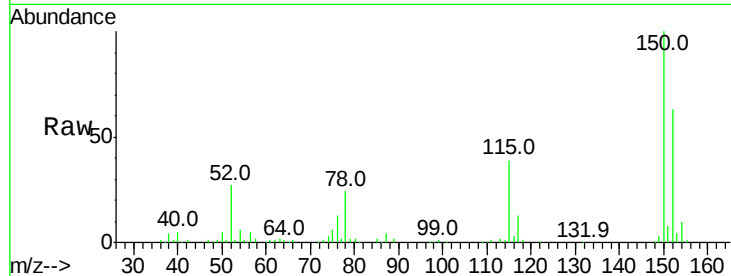


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

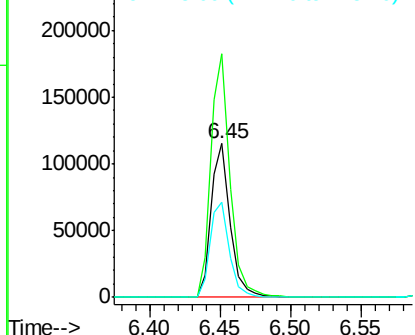



#5


2-Fluorophenol
Concen: 70.626 ng
RT: 5.05 min Scan# 538
Delta R.T. -0.05 min
Lab File: BF097305.D
Acq: 3 Aug 2017 7:49

Tgt Ion:112 Resp: 506407
Ion Ratio Lower Upper
112 100
64 64.7 46.0 69.0
63 33.2 23.4 35.0



Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

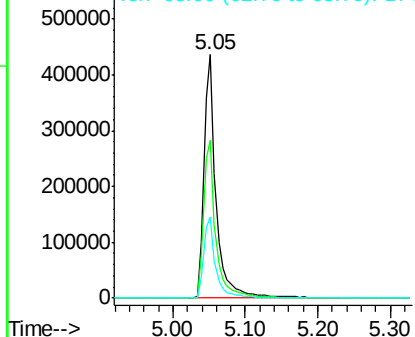

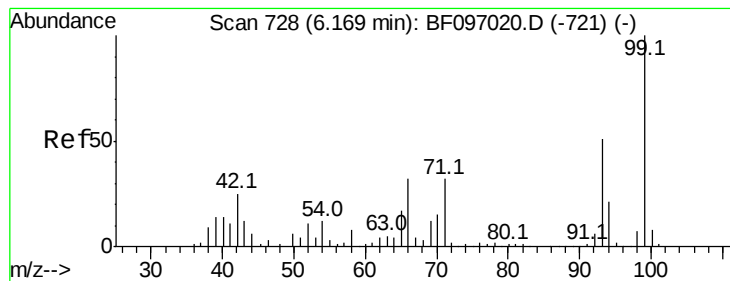

#7

Phenol-d6

Concen: 81.189 ng

RT: 6.12 min Scan# 720

Delta R.T. -0.05 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 99 Resp: 664590

Ion Ratio Lower Upper

99 100

42 21.9 13.5 20.3#




71 30.3 24.5 36.7

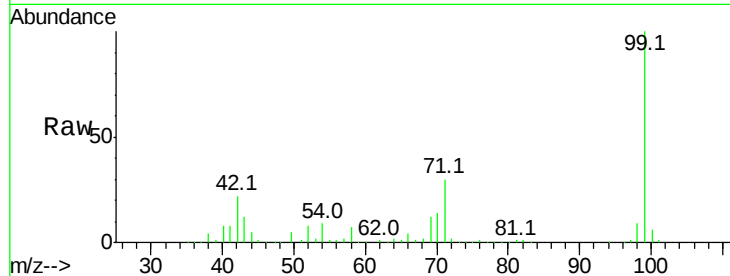

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

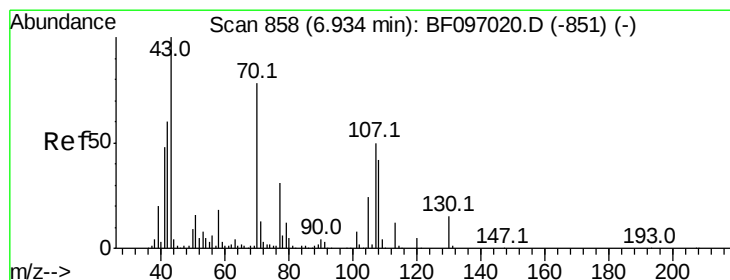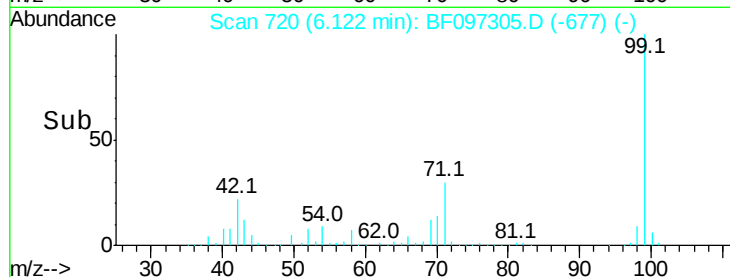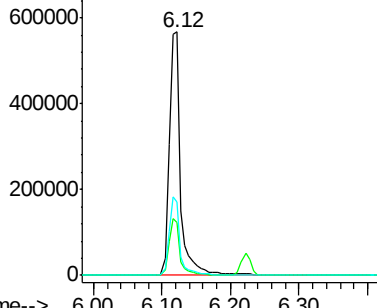

#19

n-Nitroso-di-n-propylamine

Concen: 10.682 ng

RT: 7.02 min Scan# 873

Delta R.T. 0.09 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49

Tgt Ion: 70 Resp: 57557


Ion Ratio Lower Upper

70 100

42 55.1 47.2 70.8

101 0.0 7.2 10.8#

130 2.3 15.9 23.9#


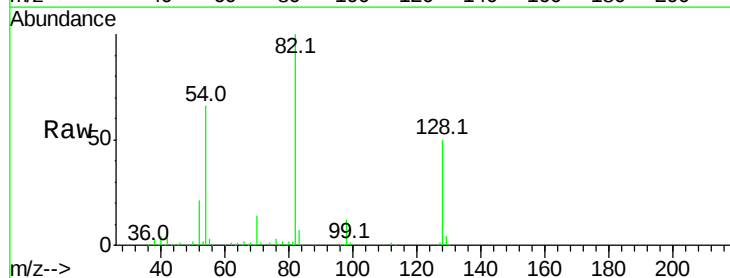


Abundance Ion 70.00 (69.70 to 70.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 101.00 (100.70 to 101.70): BF0

Ion 130.00 (129.70 to 130.70): BF0

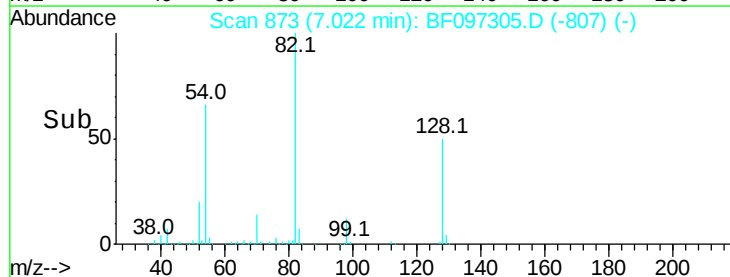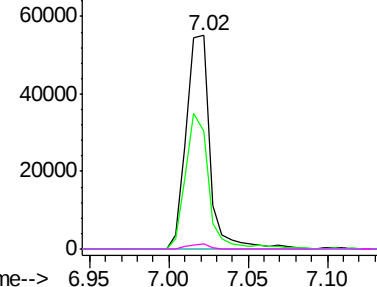



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.73 min Scan# 994

Delta R.T. -0.05 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 407479


Ion Ratio Lower Upper

136 100

137 11.3 8.5 12.7

54 10.3 4.9 7.3#

68 4.8 4.1 6.1






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

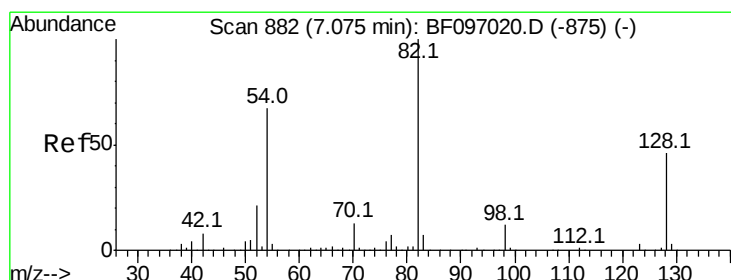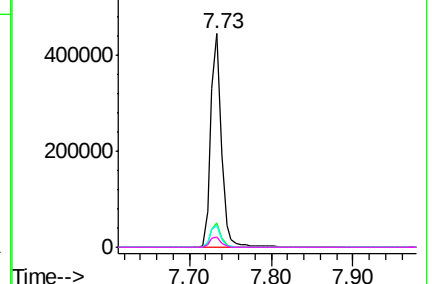

#23

Nitrobenzene-d5

Concen: 62.539 ng

RT: 7.02 min Scan# 872

Delta R.T. -0.06 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49


Tgt Ion: 82 Resp: 434397

Ion Ratio Lower Upper

82 100

128 44.0 34.0 51.0



54 67.3 42.2 63.2#




Abundance Ion 82.00 (81.70 to 82.70): BF0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF0

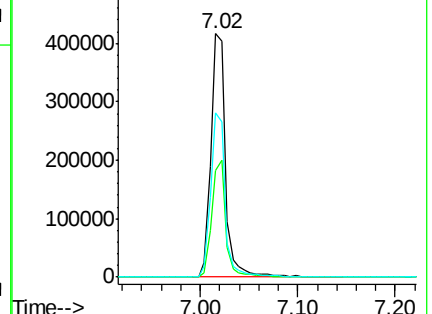



#25

Isophorone

Concen: 30.976 ng

RT: 7.02 min Scan# 872

Delta R.T. -0.32 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 421360

Ion Ratio Lower Upper




82 100

95 0.0 5.3 7.9#

138 0.0 13.1 19.7#

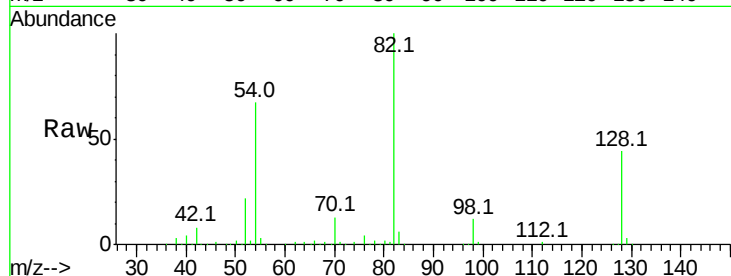

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 95.00 (94.70 to 95.70): BF0
Ion 138.00 (137.70 to 138.70): E

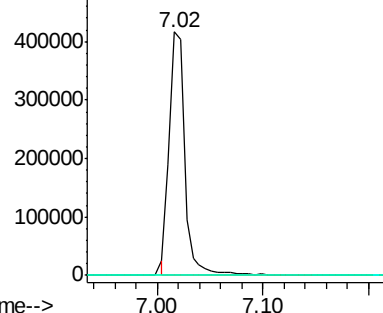

#38

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.47 min Scan# 1290

Delta R.T. -0.06 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49


Tgt Ion:164 Resp: 186829

Ion Ratio Lower Upper



164 100


162 104.2 82.6 123.8

160 48.3 36.2 54.2



Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

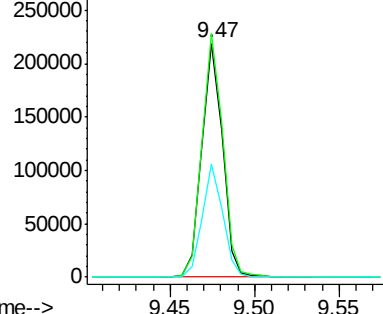


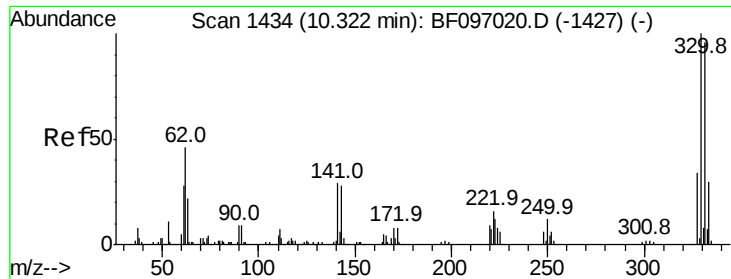




#41
 2,4,6-Tribromophenol
 Concen: 77.009 ng
 RT: 10.26 min Scan# 1424
 Delta R.T. -0.06 min
 Lab File: BF097305.D
 Acq: 3 Aug 2017 7:49

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:330 Resp: 113675
 Ion Ratio Lower Upper
 330 100
 332 96.3 76.6 115.0
 141 37.7 31.4 47.2

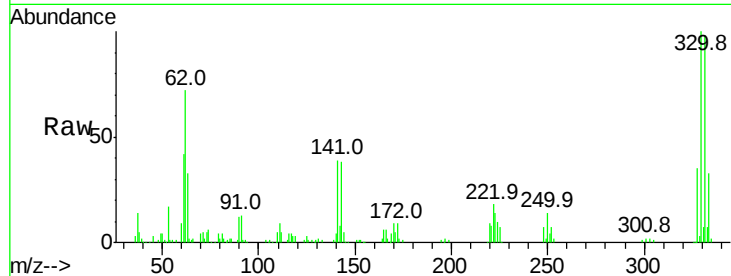


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

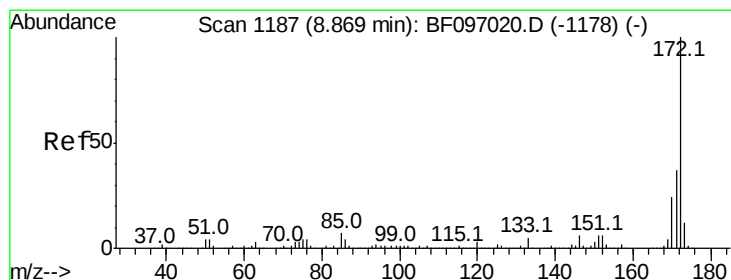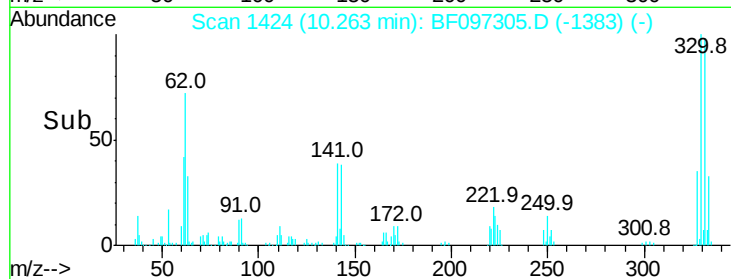
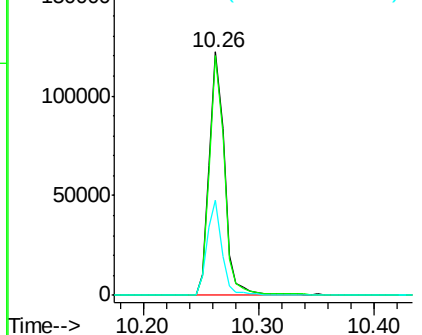



#44
 2-Fluorobiphenyl
 Concen: 66.221 ng
 RT: 8.81 min Scan# 1177
 Delta R.T. -0.06 min
 Lab File: BF097305.D
 Acq: 3 Aug 2017 7:49

Tgt Ion:172 Resp: 729010
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.6 44.4
 170 24.2 19.8 29.8



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E


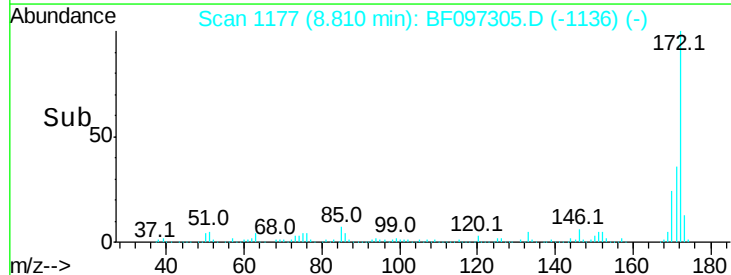
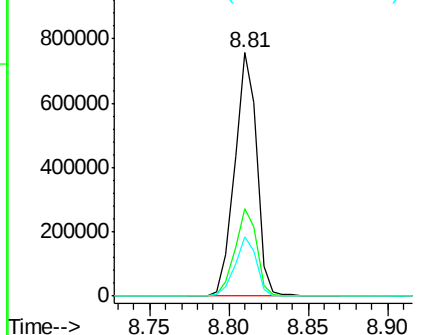


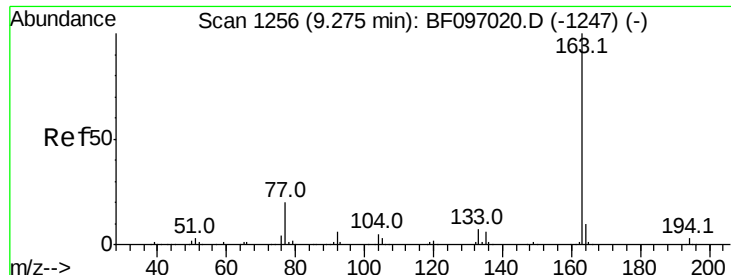

#49
Dimethylphthalate
Concen: 3.958 ng
RT: 9.21 min Scan# 1245
Delta R.T. -0.06 min
Lab File: BF097305.D
Acq: 3 Aug 2017 7:49





Instrument :
BNA_F
ClientSampleId :

Tot Ion:163 Resp: 56153
Ion Ratio Lower Upper
163 100
194 2.7 2.6 4.0
164 9.4 8.4 12.6

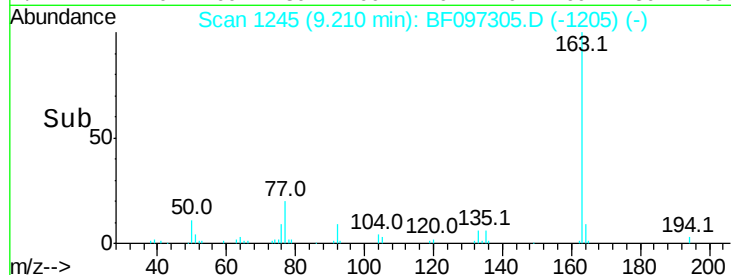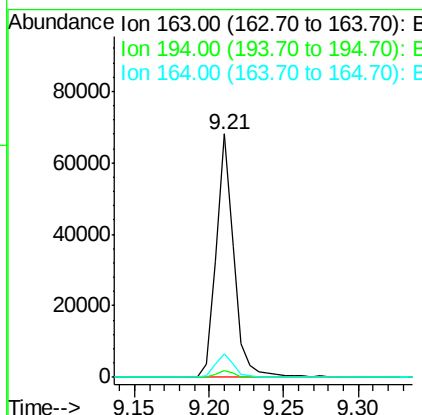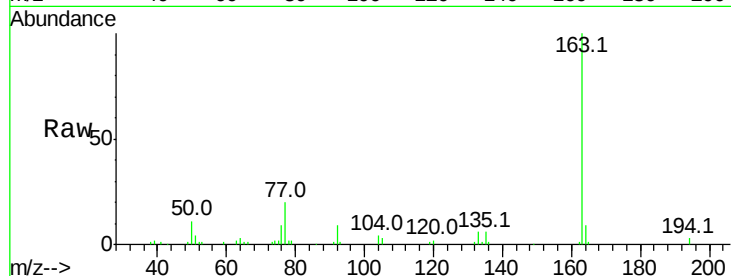

#50
2,6-Dinitrotoluene
Concen: 7.930 ng
RT: 9.47 min Scan# 1290
Delta R.T. 0.14 min
Lab File: BF097305.D
Acq: 3 Aug 2017 7:49

Tgt Ion:165 Resp: 23861
Ion Ratio Lower Upper
165 100
63 1.5 34.3 51.5#
89 1.2 37.1 55.7#

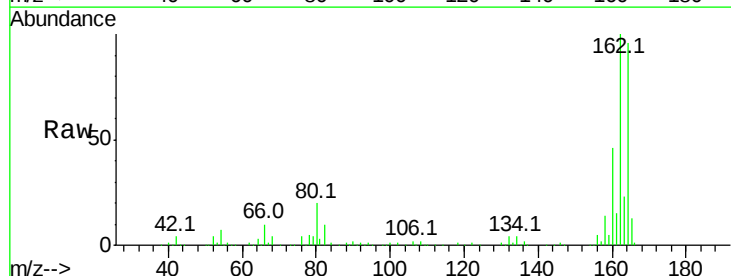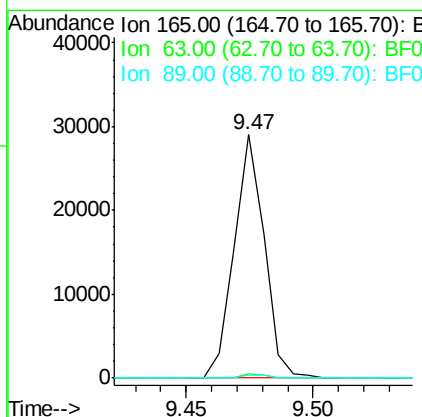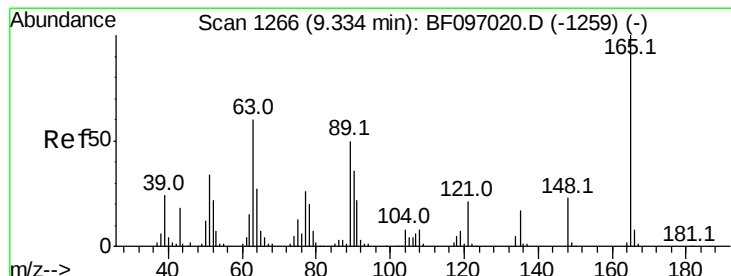







#56
 2,4-Dinitrotoluene
 Concen: 6.898 ng
 RT: 9.47 min Scan# 1290
 Delta R.T. -0.26 min
 Lab File: BF097305.D
 Acq: 3 Aug 2017 7:49

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:165 Resp: 23861
 Ion Ratio Lower Upper
 165 100
 63 1.5 25.4 38.0#
 89 1.2 46.4 69.6#
 182 0.0 1.8 2.6#




Abundance Ion 165.00 (164.70 to 165.70): E
 Ion 63.00 (62.70 to 63.70): BF0
 Ion 89.00 (88.70 to 89.70): BF0
 Ion 182.00 (181.70 to 182.70): E

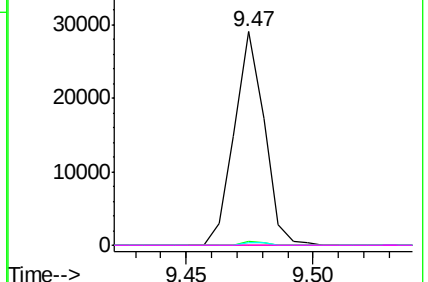




#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 10.95 min Scan# 1541
 Delta R.T. -0.05 min
 Lab File: BF097305.D
 Acq: 3 Aug 2017 7:49

Tgt Ion:188 Resp: 283491
 Ion Ratio Lower Upper
 188 100
 94 9.6 9.4 14.2
 80 10.2 10.2 15.2



Abundance Ion 188.00 (187.70 to 188.70): E
 Ion 94.00 (93.70 to 94.70): BF0
 Ion 80.00 (79.70 to 80.70): BF0

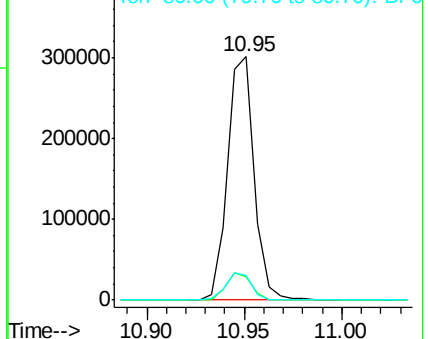


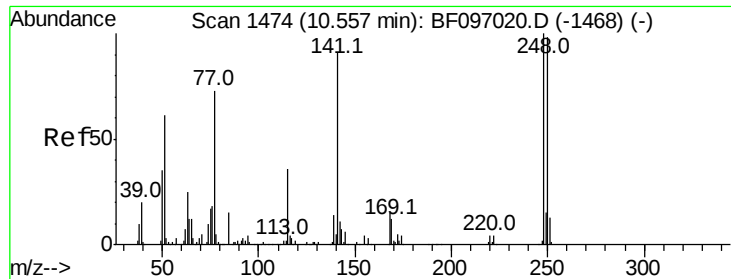




#66
4-Bromophenyl-phenylether
Concen: 2.508 ng
RT: 10.26 min Scan# 1424
Delta R.T. -0.29 min
Lab File: BF097305.D
Acq: 3 Aug 2017 7:49

Instrument :
BNA_F
ClientSampleId :

Tot Ion:248 Resp: 7096
Ion Ratio Lower Upper
248 100
250 207.9 76.8 115.2#
141 574.3 68.6 103.0#

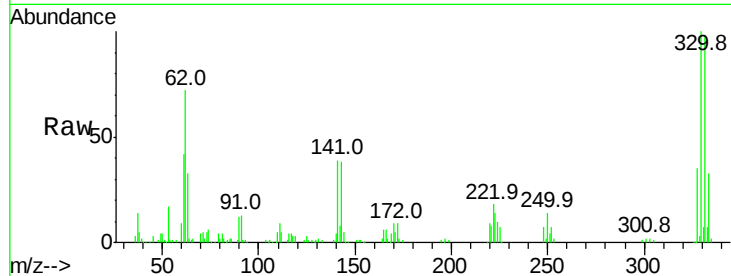


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E


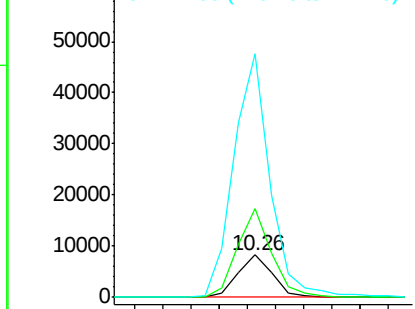



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.57 min Scan# 1986
Delta R.T. -0.06 min
Lab File: BF097305.D
Acq: 3 Aug 2017 7:49

Tgt Ion:240 Resp: 185258
Ion Ratio Lower Upper
240 100
120 17.1 5.8 8.8#
236 24.8 20.5 30.7



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

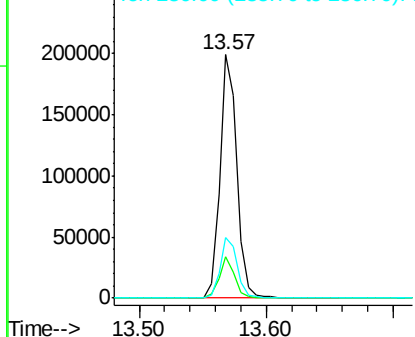

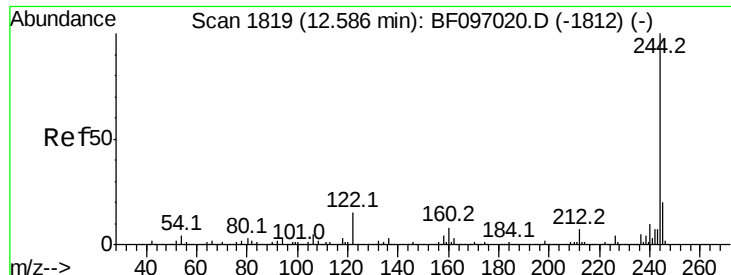

#78

Terphenyl-d14

Concen: 50.450 ng

RT: 12.53 min Scan# 1810

Delta R.T. -0.05 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49

Instrument :

BNA_F

ClientSampleId :


Tot Ion:244 Resp: 458404

Ion Ratio Lower Upper

244 100

212 6.6 6.0 9.0

122 12.6 10.3 15.5



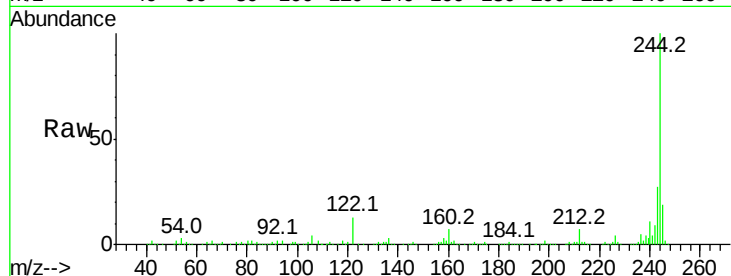


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

12.53

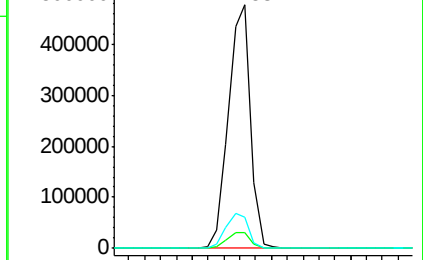

#86

Perylene-d12

Concen: 20.000 ng

RT: 14.92 min Scan# 2215

Delta R.T. -0.06 min

Lab File: BF097305.D

Acq: 3 Aug 2017 7:49


Tgt Ion:264 Resp: 169659

Ion Ratio Lower Upper

264 100

260 22.9 19.5 29.3

265 20.7 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

14.92

