

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\
 Data File : BF097275.D
 Acq On : 2 Aug 2017 16:06
 Operator : SJ/JU
 Sample : PB101142BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB101142BL

Quant Time: Aug 02 17:10:02 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 02 17:05:06 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.45	152	92092	20.00	ng	0.00
21) Naphthalene-d8	7.73	136	451630	20.00	ng	0.00
38) Acenaphthene-d10	9.47	164	177496	20.00	ng	0.00
63) Phenanthrene-d10	10.95	188	330139	20.00	ng	0.00
75) Chrysene-d12	13.57	240	256645	20.00	ng	-0.01
86) Perylene-d12	14.91	264	170547	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.06	112	833888	136.50	ng	0.01
7) Phenol-d6	6.12	99	1050924	150.69	ng	0.00
23) Nitrobenzene-d5	7.02	82	571435	74.23	ng	0.00
41) 2,4,6-Tribromophenol	10.27	330	198657	141.66	ng	0.00
44) 2-Fluorobiphenyl	8.81	172	974657	93.19	ng	0.00
78) Terphenyl-d14	12.53	244	826654	65.67	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\
Data File : BF097275.D
Acq On : 2 Aug 2017 16:06
Operator : SJ/JU
Sample : PB101142BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB101142BL

Quant Time: Aug 02 17:10:02 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 02 17:05:06 2017
Response via : Initial Calibration

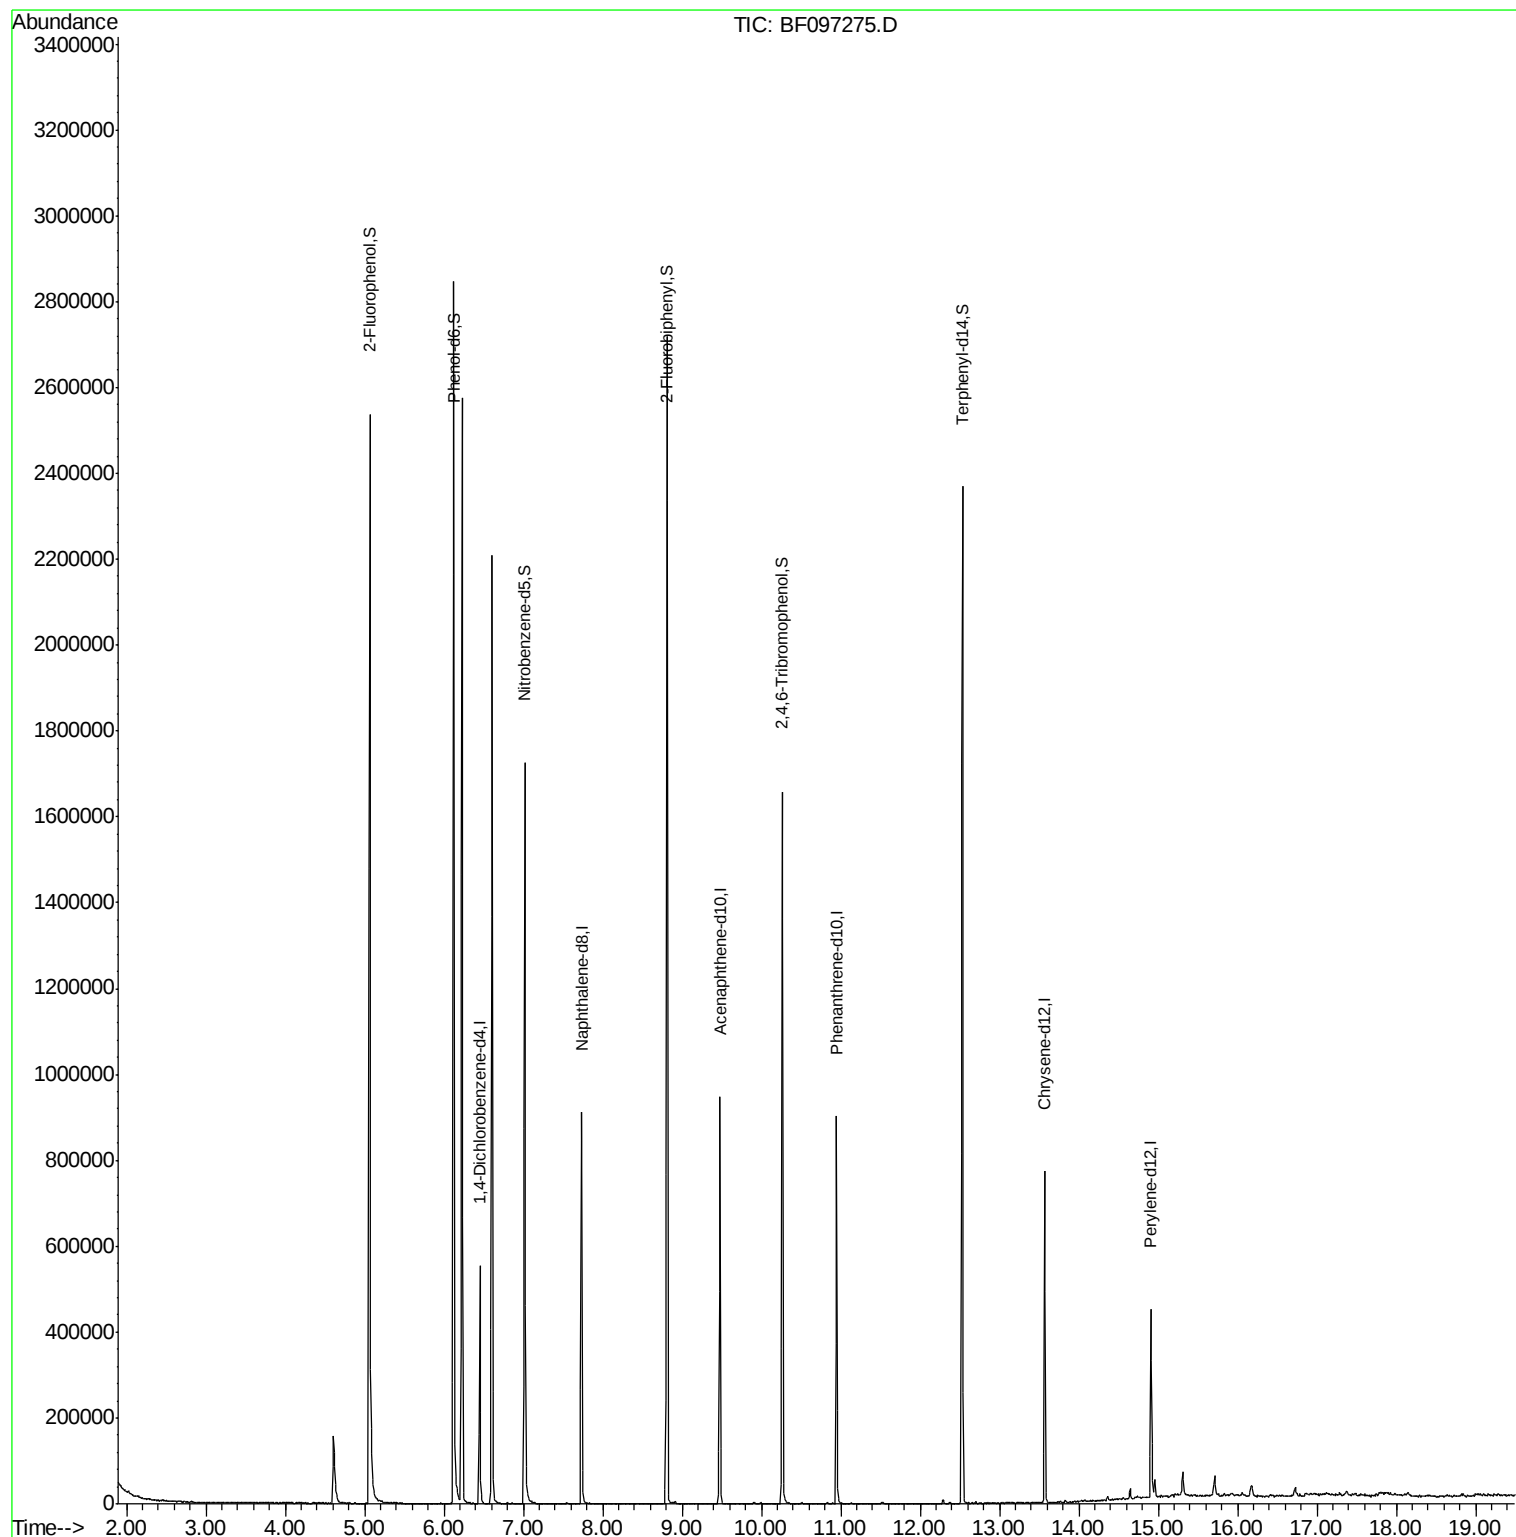

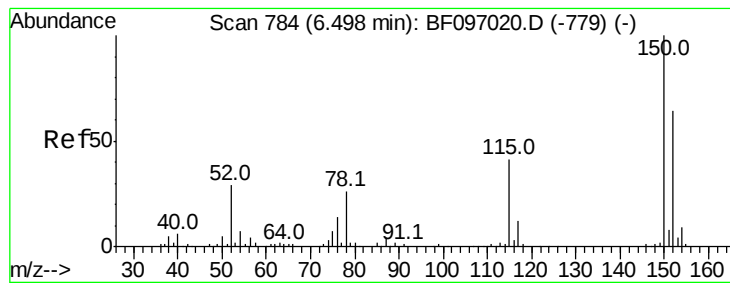


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.45 min Scan# 776
Delta R.T. 0.00 min
Lab File: BF097275.D
Acq: 2 Aug 2017 16:06

Instrument :
BNA_F
ClientSampleId :
PB101142BL

Tot Ion:152 Resp: 92092
Ion Ratio Lower Upper
152 100
150 155.7 126.2 189.2
115 61.4 52.2 78.2

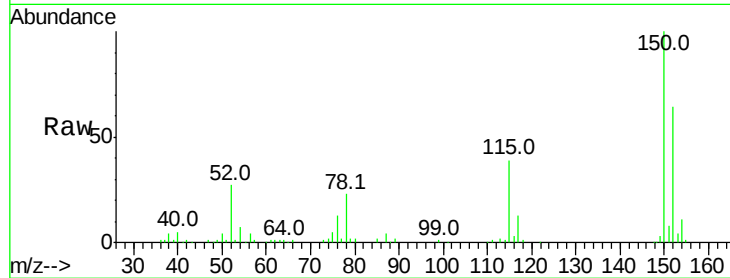


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

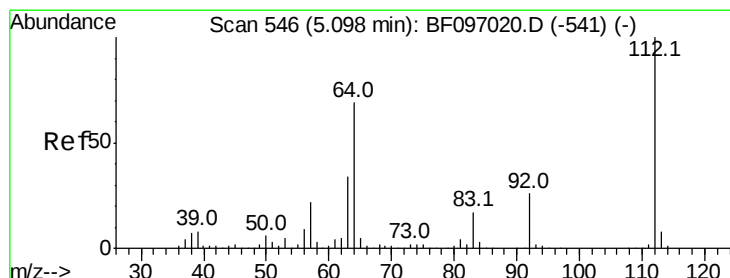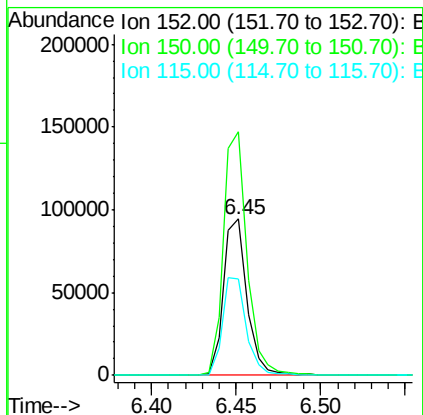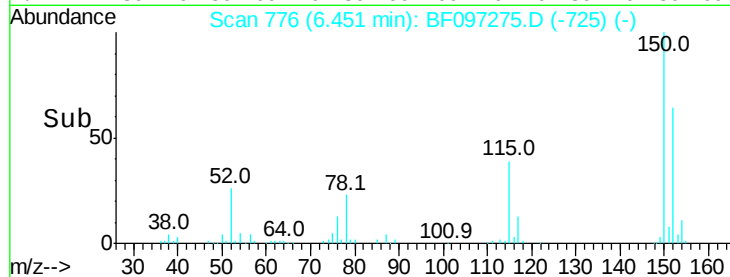



#5


2-Fluorophenol
Concen: 136.502 ng
RT: 5.06 min Scan# 540
Delta R.T. 0.01 min
Lab File: BF097275.D
Acq: 2 Aug 2017 16:06

Tgt Ion:112 Resp: 833888
Ion Ratio Lower Upper
112 100
64 65.9 46.0 69.0
63 34.2 23.4 35.0

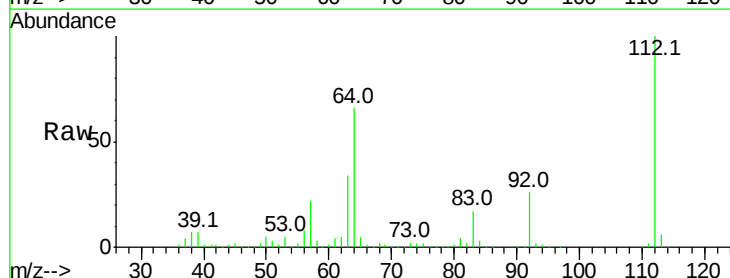

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

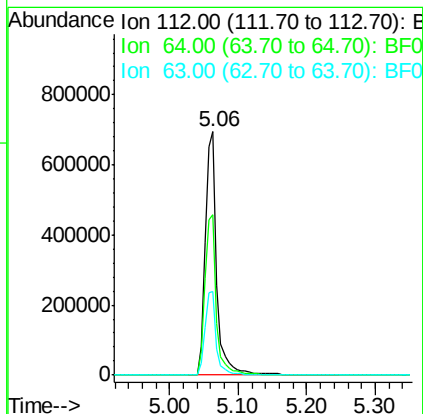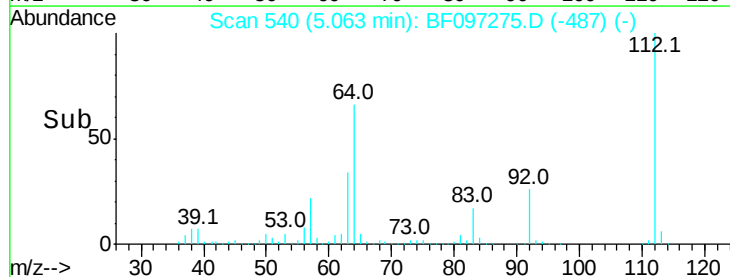

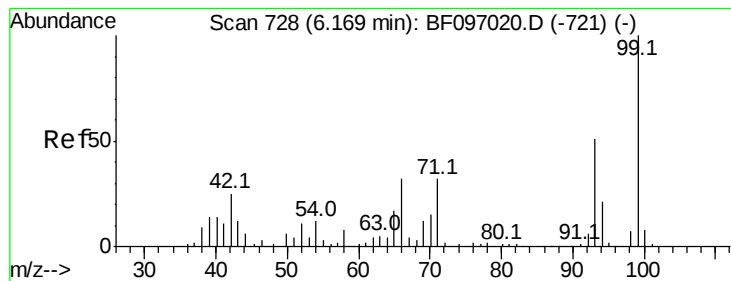

#7

Phenol-d6

Concen: 150.689 ng

RT: 6.12 min Scan# 720

Delta R.T. -0.01 min

Lab File: BF097275.D

Acq: 2 Aug 2017 16:06

Instrument :


BNA_F

ClientSampleId :




PB101142BL

Tot Ion: 99 Resp: 1050924

Ion	Ratio	Lower	Upper
99	100		
42	24.4	13.5	20.3#
71	33.3	24.5	36.7

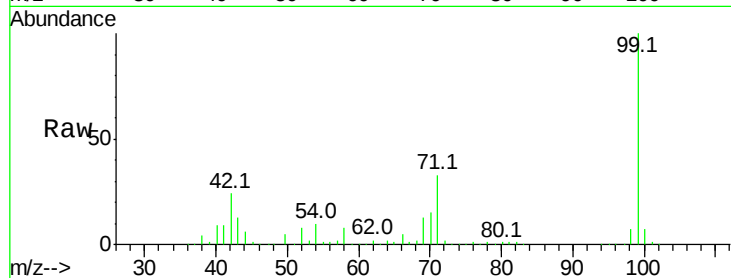

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

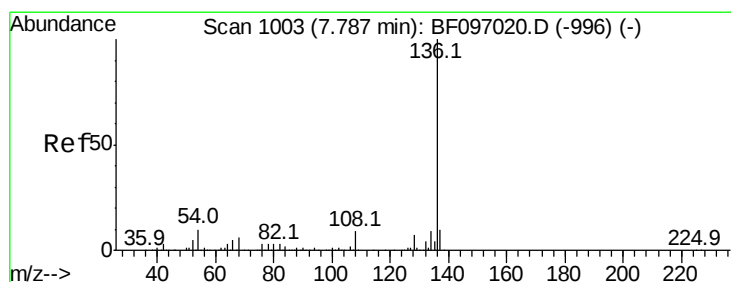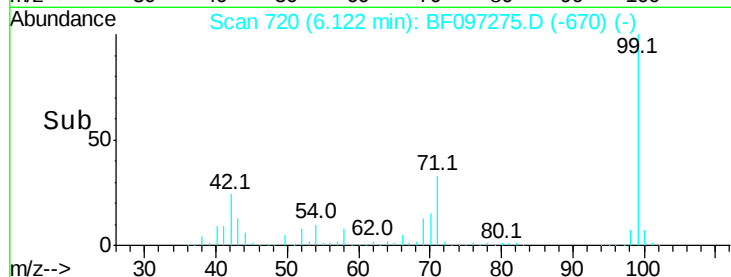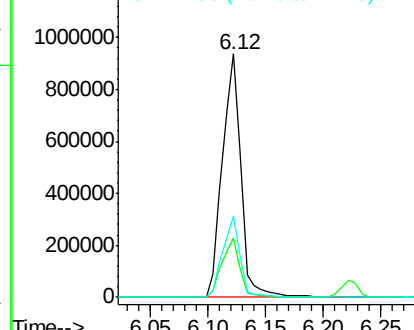

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.73 min Scan# 994

Delta R.T. -0.01 min




Lab File: BF097275.D


Acq: 2 Aug 2017 16:06

Tgt Ion: 136 Resp: 451630

Ion	Ratio	Lower	Upper
136	100		
137	10.6	8.5	12.7
54	9.9	4.9	7.3#
68	5.8	4.1	6.1

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0


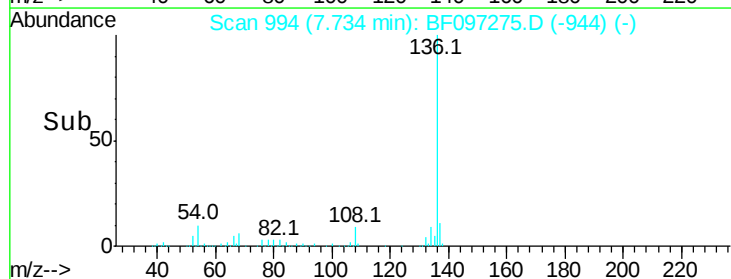
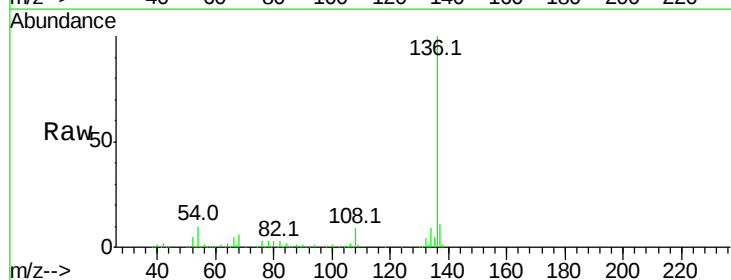
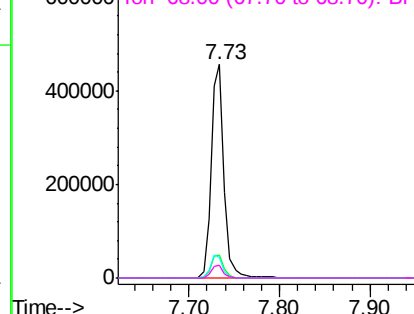


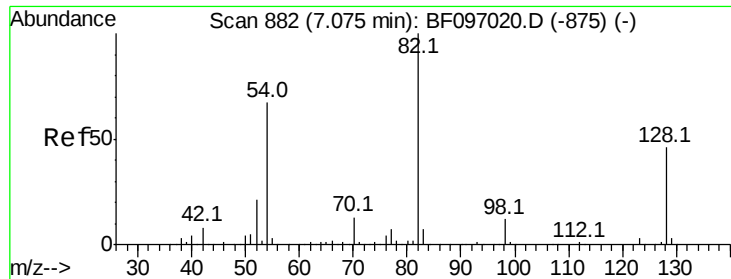

#23
 Nitrobenzene-d5
 Concen: 74.226 ng
 RT: 7.02 min Scan# 873
 Delta R.T. -0.01 min
 Lab File: BF097275.D
 Acq: 2 Aug 2017 16:06




Instrument :
 BNA_F
 ClientSampleId :
 PB101142BL

Tot Ion: 82 Resp: 571435
 Ion Ratio Lower Upper
 82 100
 128 46.8 34.0 51.0
 54 66.8 42.2 63.2#

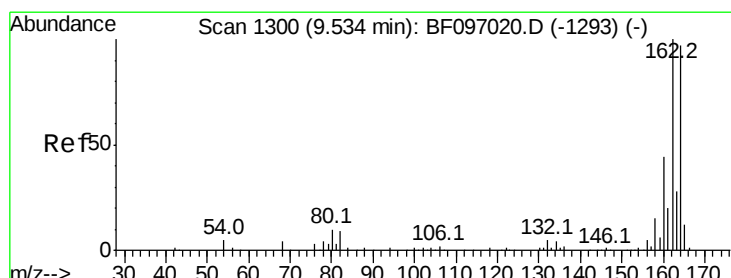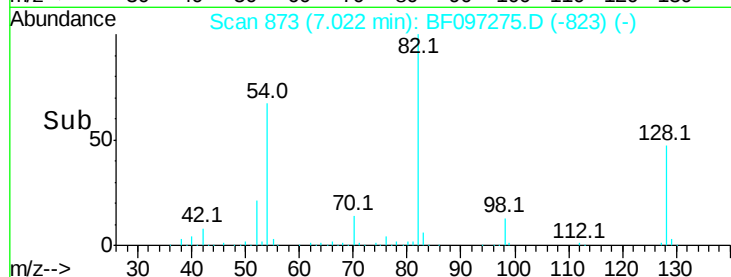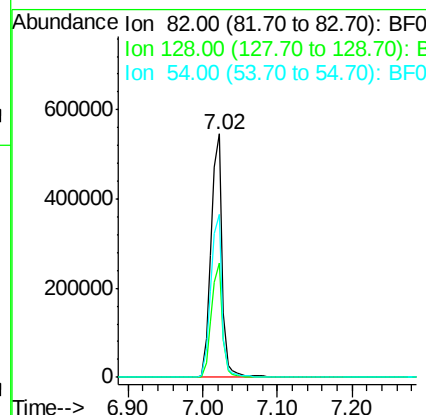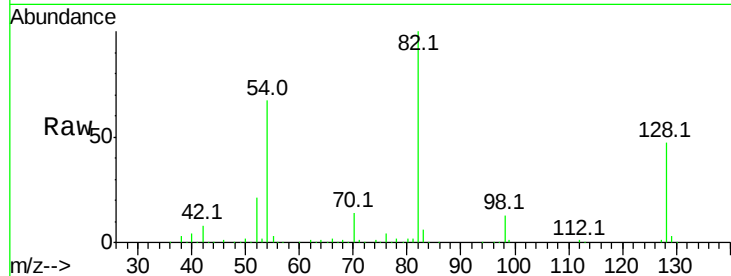

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.47 min Scan# 1290
 Delta R.T. -0.01 min
 Lab File: BF097275.D
 Acq: 2 Aug 2017 16:06

Tgt Ion:164 Resp: 177496
 Ion Ratio Lower Upper
 164 100
 162 101.6 82.6 123.8
 160 46.3 36.2 54.2

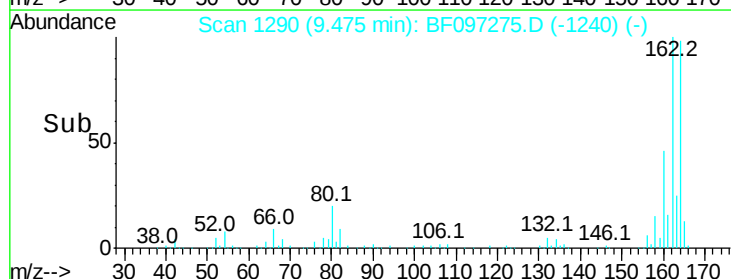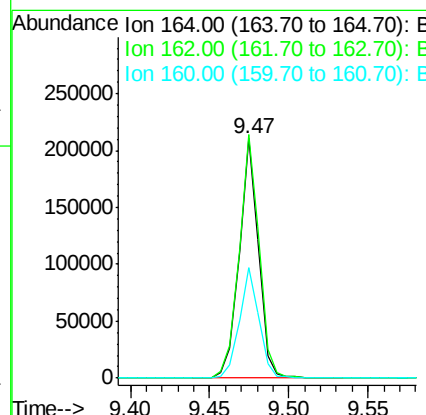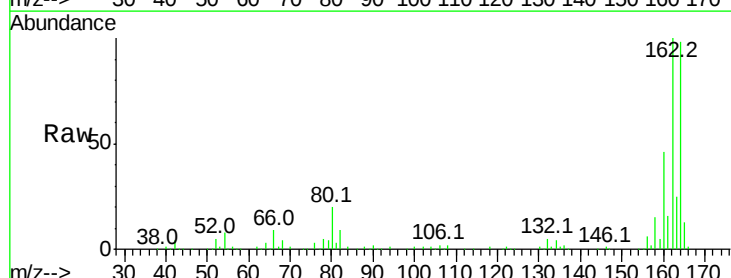







#41
 2,4,6-Tribromophenol
 Concen: 141.656 ng
 RT: 10.27 min Scan# 1425
 Delta R.T. 0.00 min
 Lab File: BF097275.D
 Acq: 2 Aug 2017 16:06

Instrument :
 BNA_F
 ClientSampleId :
 PB101142BL

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.8	76.6	115.0
141	38.2	31.4	47.2

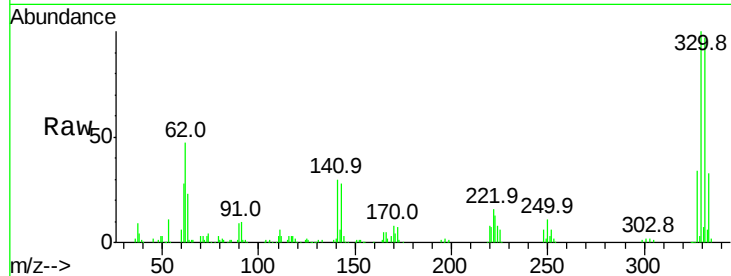


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

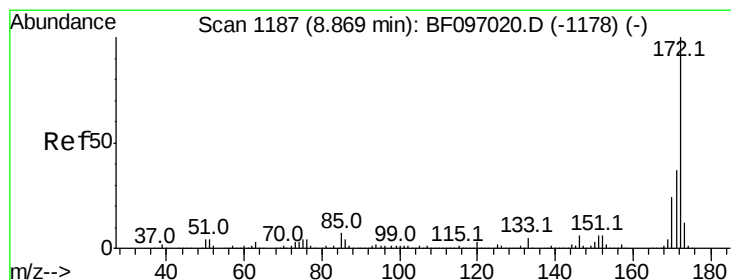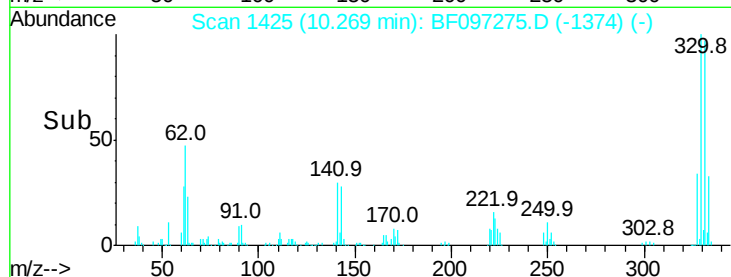
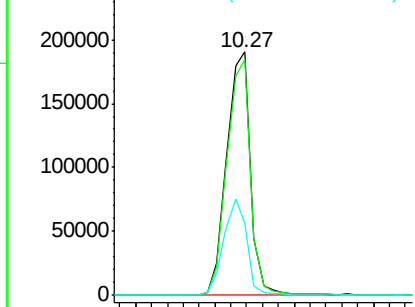



#44
 2-Fluorobiphenyl
 Concen: 93.190 ng
 RT: 8.81 min Scan# 1177
 Delta R.T. -0.01 min
 Lab File: BF097275.D
 Acq: 2 Aug 2017 16:06

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.8	29.6	44.4
170	24.6	19.8	29.8

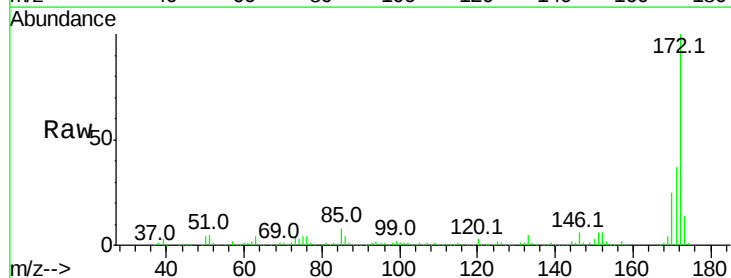

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



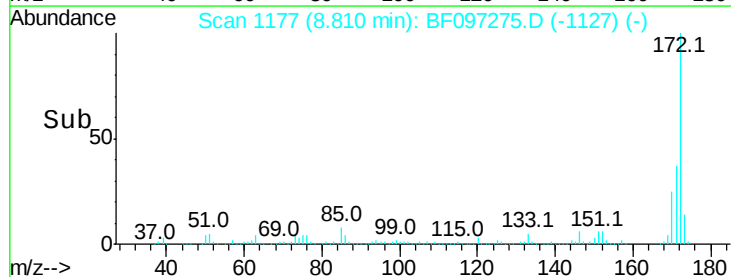
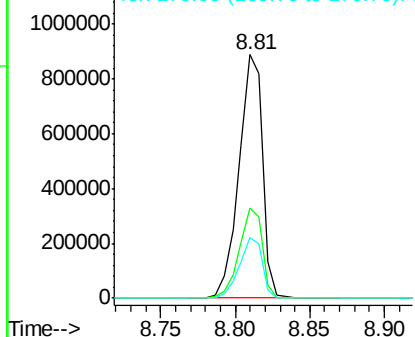


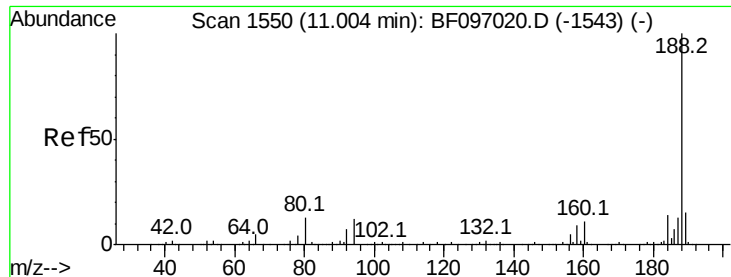

#63
 Phenanthrene-d10
 Concen: 20.000 ng
 RT: 10.95 min Scan# 1540
 Delta R.T. -0.01 min
 Lab File: BF097275.D
 Acq: 2 Aug 2017 16:06




Instrument :
 BNA_F
 ClientSampleId :
 PB101142BL


Tot Ion	Ratio	Lower	Upper
188	100		
94	12.1	9.4	14.2
80	12.2	10.2	15.2

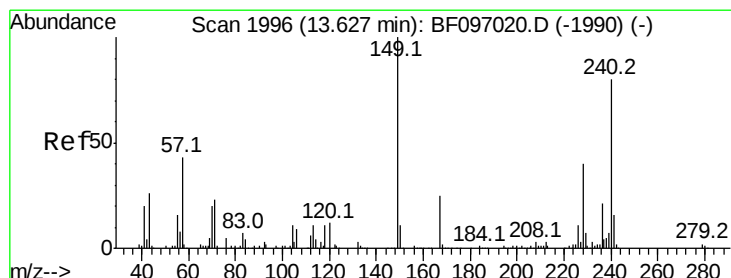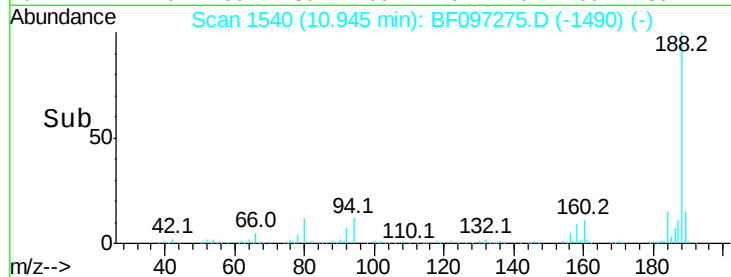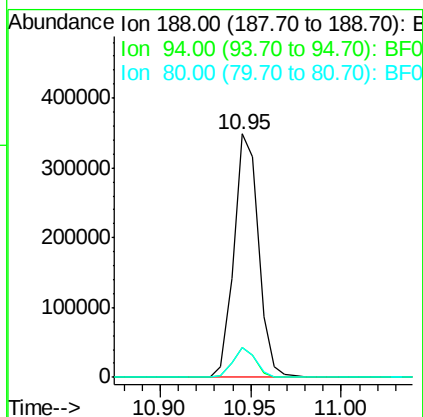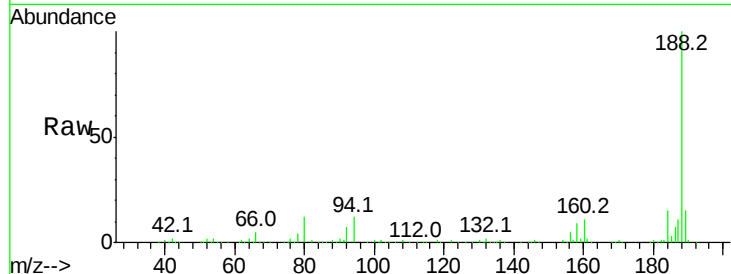

#75
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.57 min Scan# 1986
 Delta R.T. -0.01 min
 Lab File: BF097275.D
 Acq: 2 Aug 2017 16:06

Tgt Ion	Ratio	Lower	Upper
240	100		
120	15.1	5.8	8.8#
236	25.5	20.5	30.7

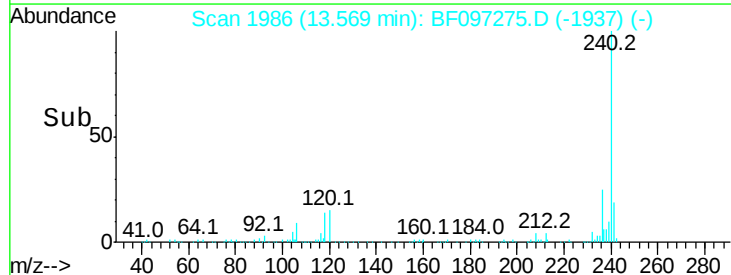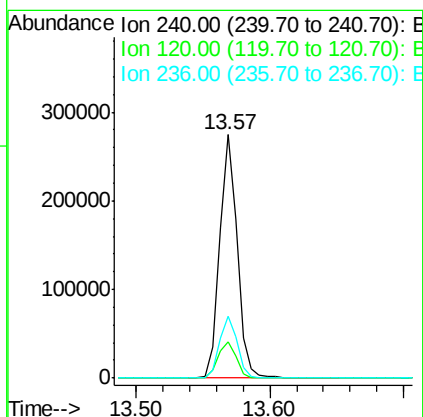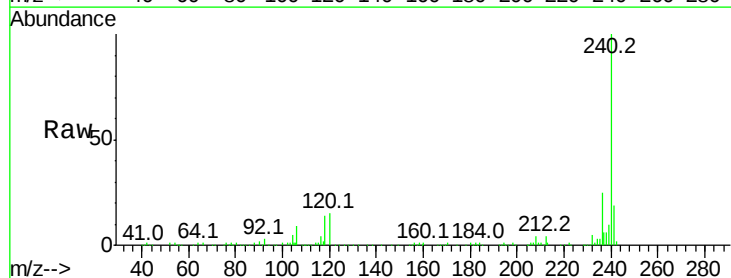

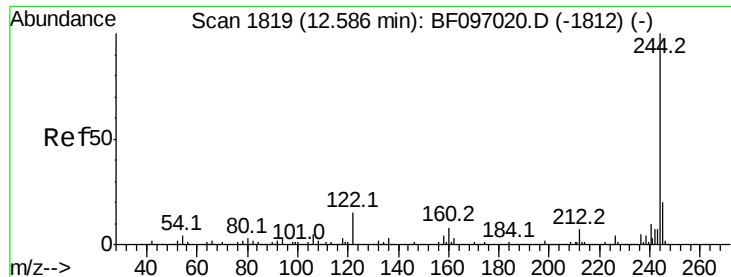

#78

Terphenyl-d14

Concen: 65.671 ng

RT: 12.53 min Scan# 1810

Delta R.T. -0.01 min

Lab File: BF097275.D

Acq: 2 Aug 2017 16:06

Instrument :

BNA_F

ClientSampleId :

PB101142BL


Tot Ion:244 Resp: 826654

Ion Ratio Lower Upper

244 100

212 6.9 6.0 9.0




122 15.3 10.3 15.5

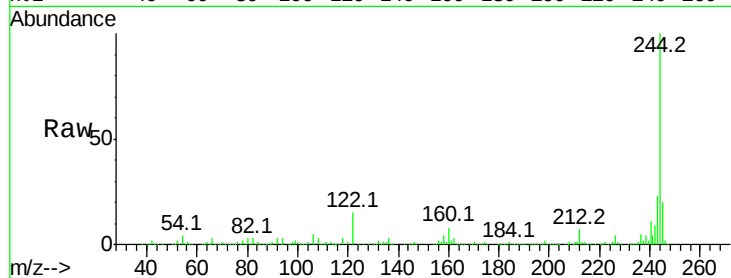

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

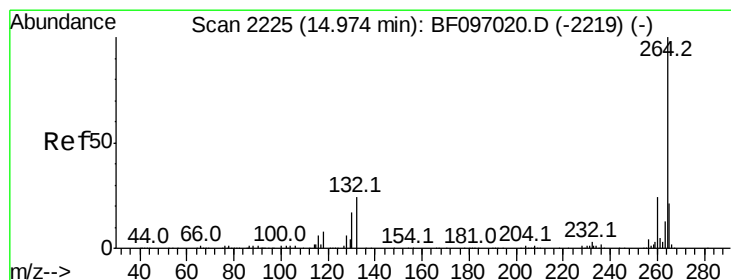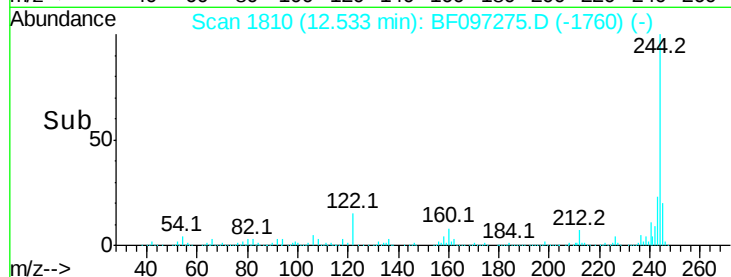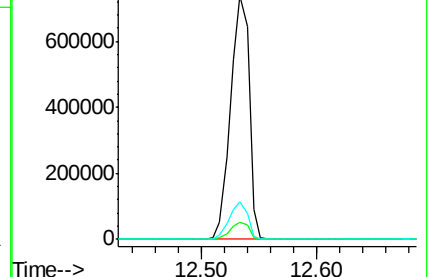

#86

Perylene-d12

Concen: 20.000 ng

RT: 14.91 min Scan# 2214

Delta R.T. -0.01 min

Lab File: BF097275.D

Acq: 2 Aug 2017 16:06


Tgt Ion:264 Resp: 170547

Ion Ratio Lower Upper

264 100

260 23.4 19.5 29.3

265 20.3 17.2 25.8

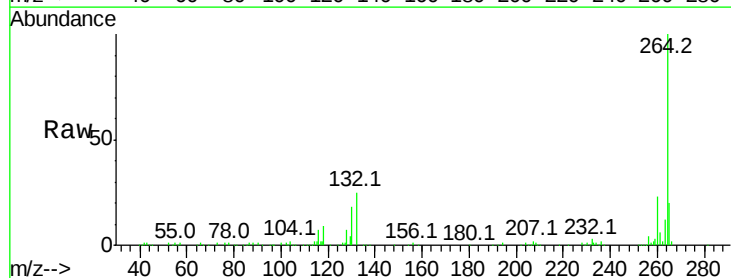

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

