
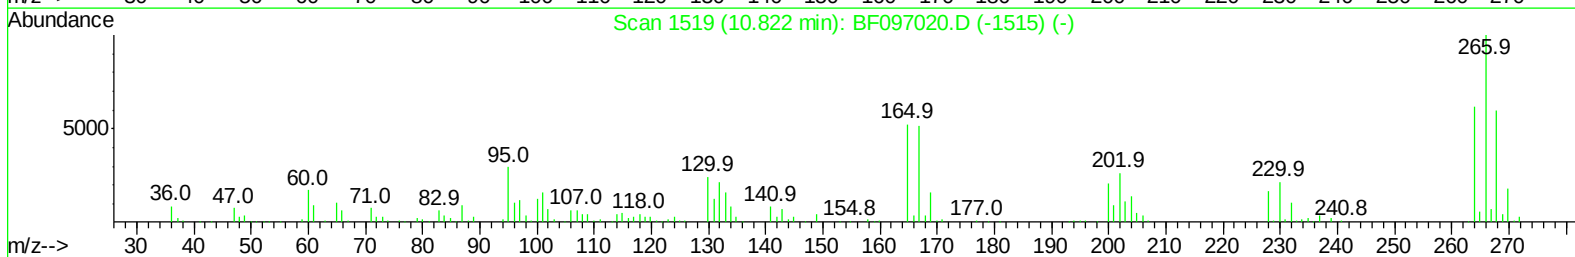
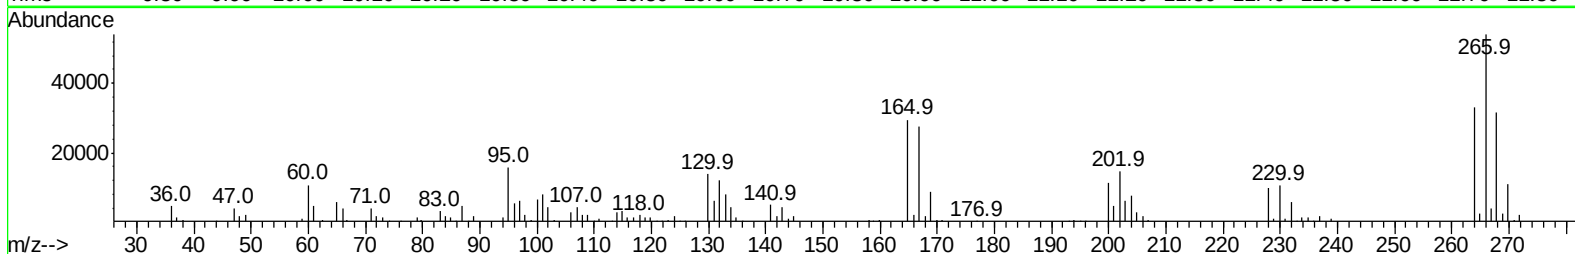


Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\  
Data File : BF097270.D  
Acq On : 2 Aug 2017 13:37  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:09:46 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 02 17:05:06 2017  
Response via : Initial Calibration

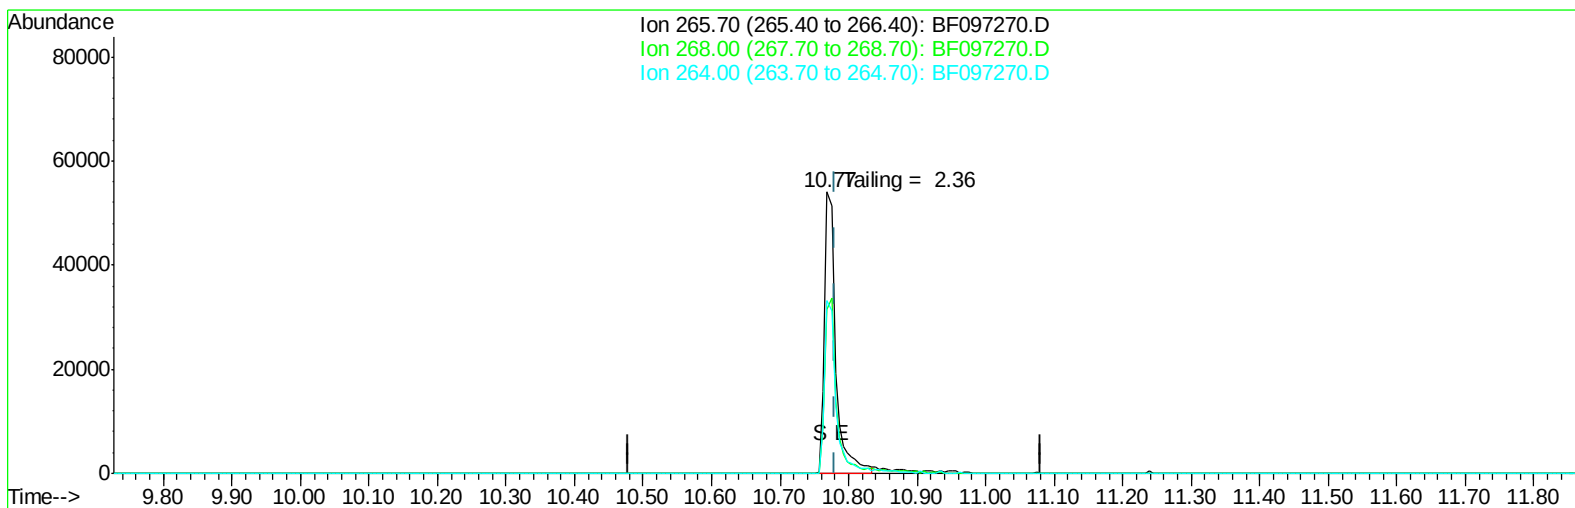

TIC: BF097270.D

(69) Pentachlorophenol (C)




10.769min (-0.012) 0.00ng

response 61784

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 58.22 |
| 264.00 | 64.60 | 61.38 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF080217\  
Data File : BF097270.D  
Acq On : 2 Aug 2017 13:37  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 02 18:09:46 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF072517.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 02 17:05:06 2017  
Response via : Initial Calibration

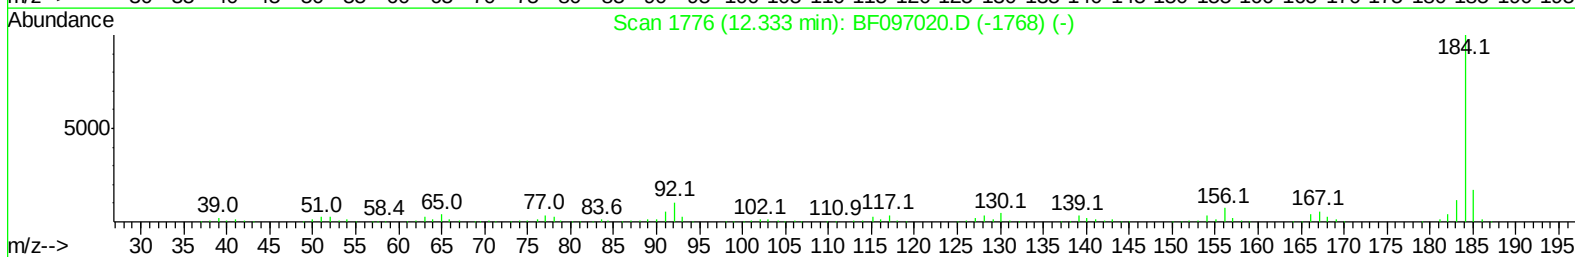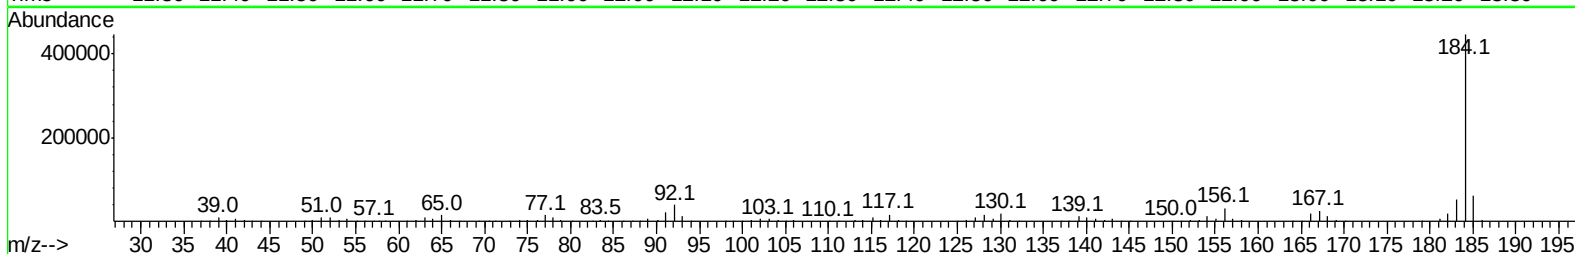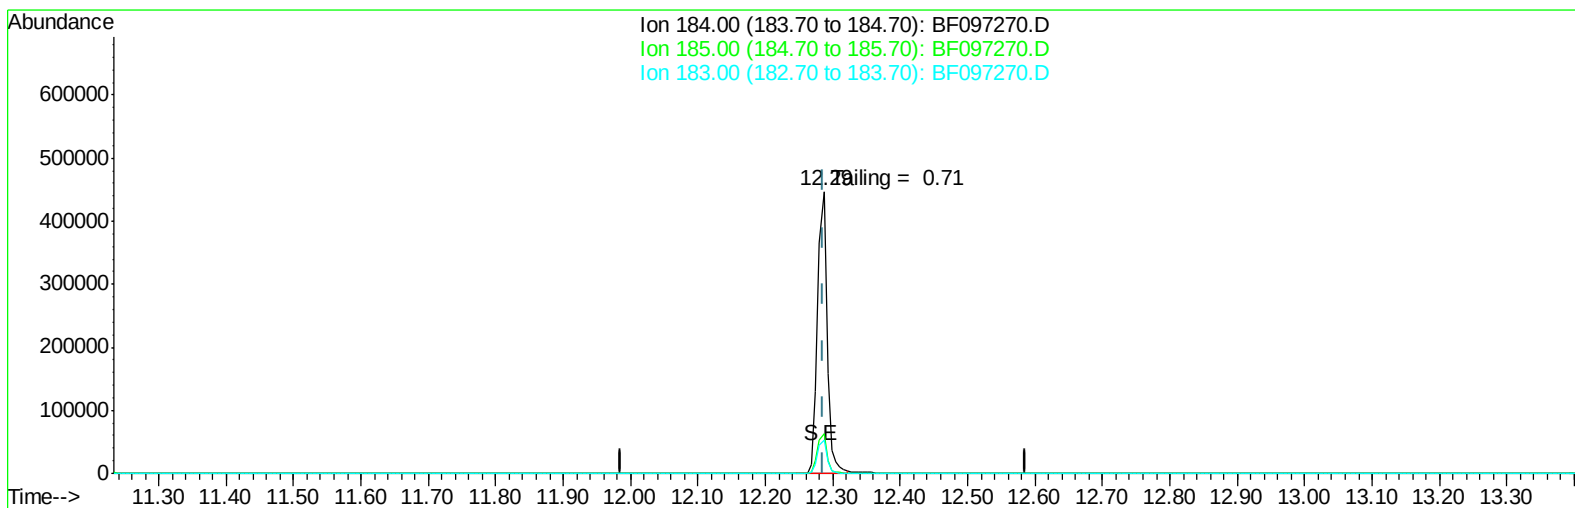

TIC: BF097270.D

(76) Benzidine

12.286min (+0.000) 102259.54ng

response 424964

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 13.90# |
| 183.00 | 12.20 | 11.75  |
| 0.00   | 0.00  | 0.00   |